

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
 Data File : FB027462.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jun 2022 13:44
 Operator : AJ/MA
 Sample : N3373-12MS
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 DS-7DMS

Integration File: Calibration.e
 Quant Time: Jun 21 01:10:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	158754	14.153 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	337456	20.030 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	271628	15.470 ng/ml
3) t n-Heptane	7.752	78393	4.475 ng/ml
4) t Benzene	7.886	165327	8.107 ng/ml
6) t Toluene	10.618	446296	23.050 ng/ml
7) t Ethylbenzene	13.056	134913	7.450 ng/ml
8) t m-Xylene	13.188	268340	15.053 ng/ml
9) t O-Xylene	13.915	277462	15.968 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	279418	16.266 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
Data File : FB027462.D
Signal(s) : FID2B.CH
Acq On : 20 Jun 2022 13:44
Operator : AJ/MA
Sample : N3373-12MS
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
DS-7DMS

Integration File: Calibration.e
Quant Time: Jun 21 01:10:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

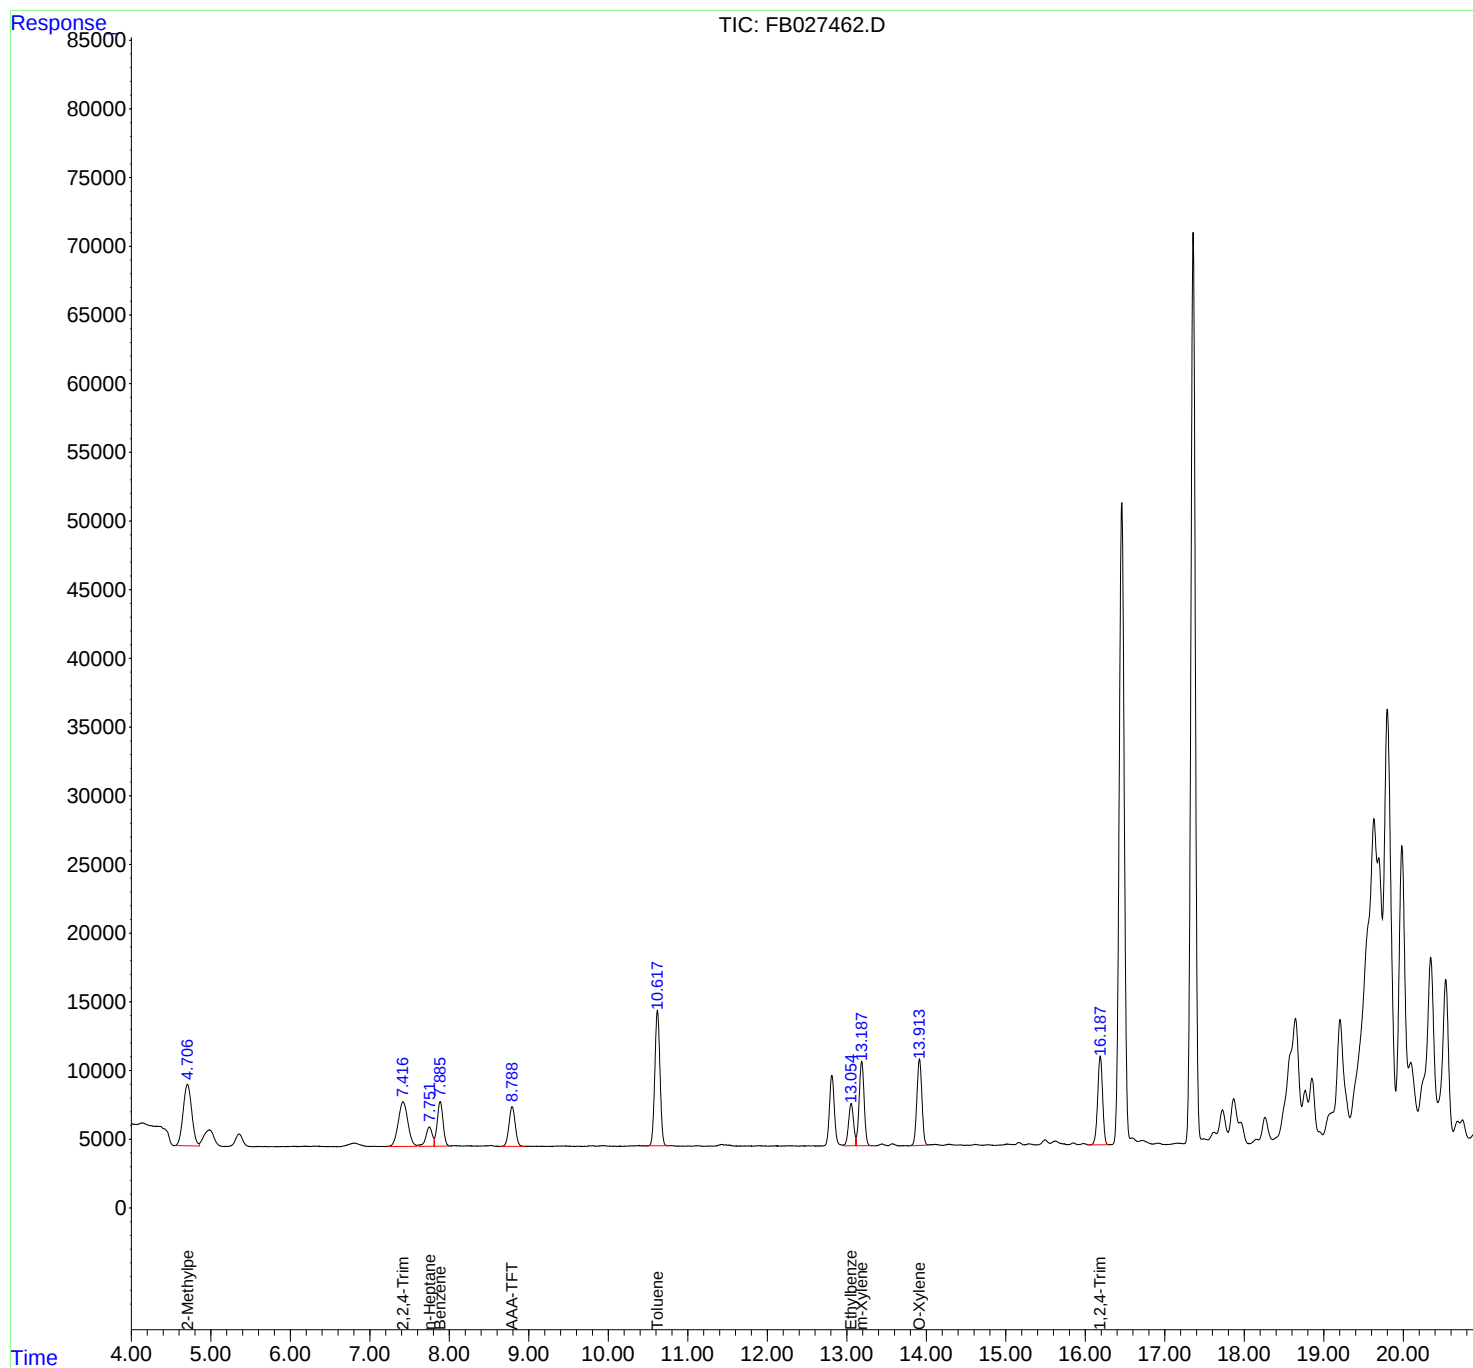


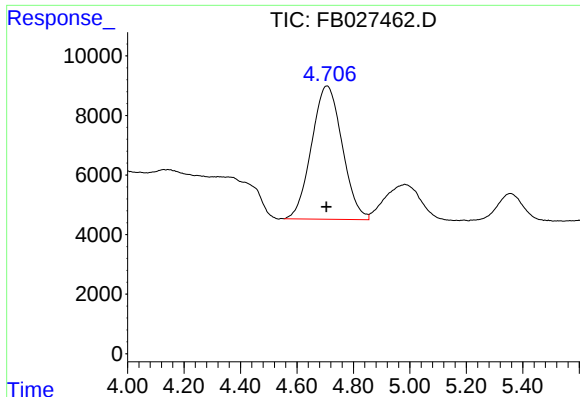

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.003 min
Response: 337456
Conc: 20.03 ng/ml

Instrument :
FID_B
ClientSampleId :
DS-7DMS

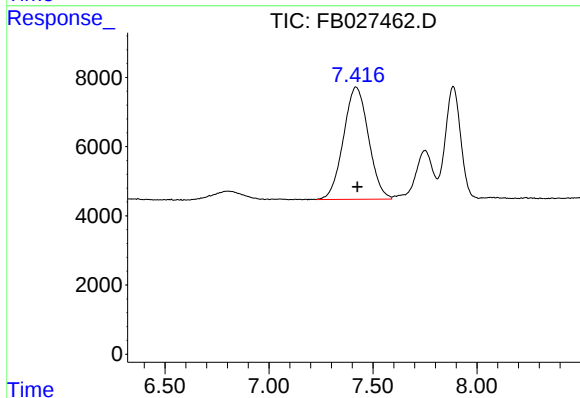


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.009 min
Response: 271628
Conc: 15.47 ng/ml

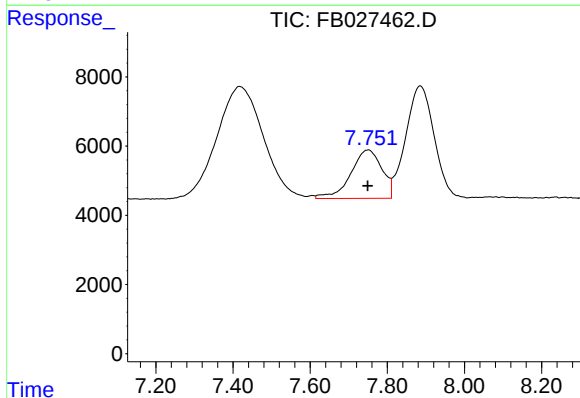


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.003 min
Response: 78393
Conc: 4.47 ng/ml

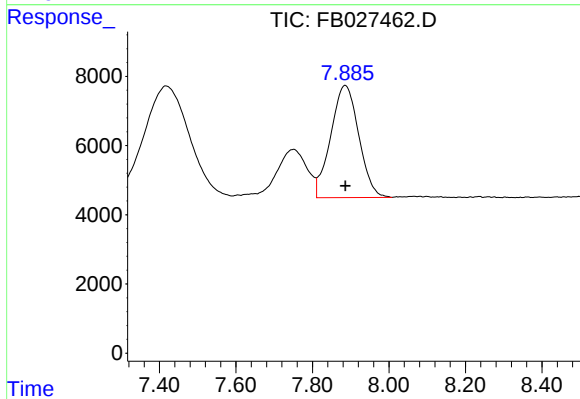

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 165327
Conc: 8.11 ng/ml

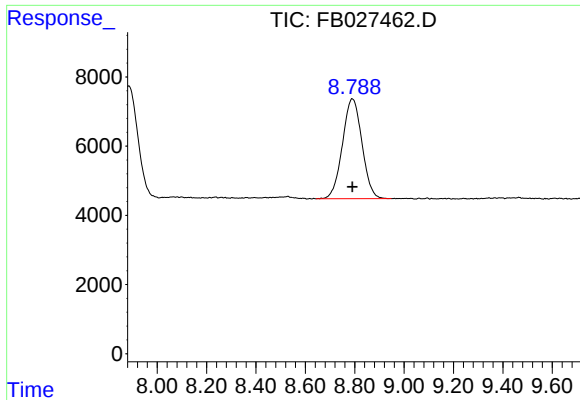

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 158754
Conc: 14.15 ng/ml

Instrument :
FID_B
ClientSampleId :
DS-7DMS

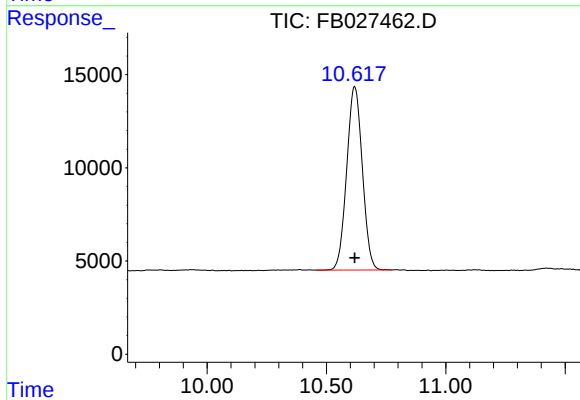


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 446296
Conc: 23.05 ng/ml

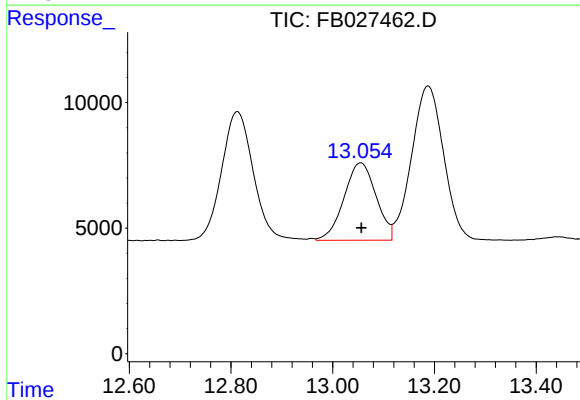


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 134913
Conc: 7.45 ng/ml

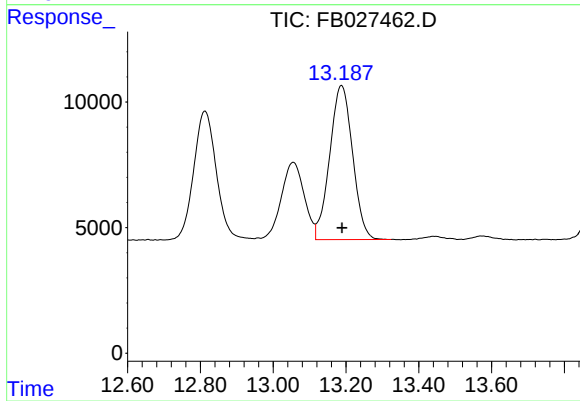

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 268340
Conc: 15.05 ng/ml

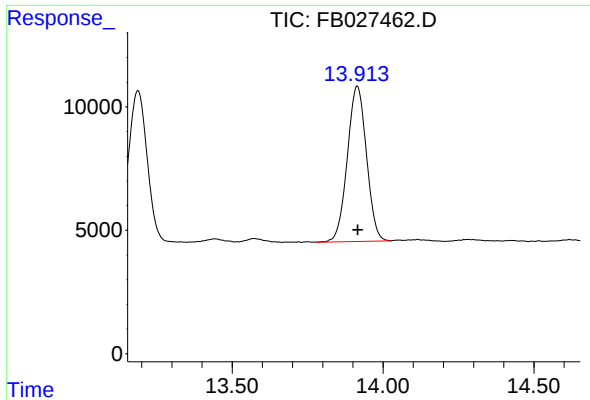

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.001 min
Response: 277462
Conc: 15.97 ng/ml

Instrument :
FID_B
ClientSampleId :
DS-7DMS

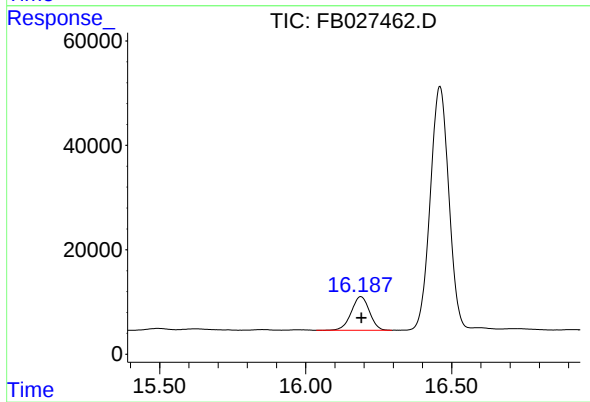

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.003 min
Response: 279418
Conc: 16.27 ng/ml