

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
 Data File : FB027463.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jun 2022 14:32
 Operator : AJ/MA
 Sample : N3373-12MSD
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 DS-7DMSD

Integration File: Calibration.e
 Quant Time: Jun 21 01:10:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	157594	14.050 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	333001	19.766 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	254590	14.500 ng/ml
3) t n-Heptane	7.749	87877	5.016 ng/ml
4) t Benzene	7.886	174349	8.550 ng/ml
6) t Toluene	10.618	462953	23.910 ng/ml
7) t Ethylbenzene	13.055	133257	7.358 ng/ml
8) t m-Xylene	13.188	258291	14.489 ng/ml
9) t O-Xylene	13.914	256874	14.783 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	243971	14.202 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
Data File : FB027463.D
Signal(s) : FID2B.CH
Acq On : 20 Jun 2022 14:32
Operator : AJ/MA
Sample : N3373-12MSD
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
DS-7DMSD

Integration File: Calibration.e
Quant Time: Jun 21 01:10:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

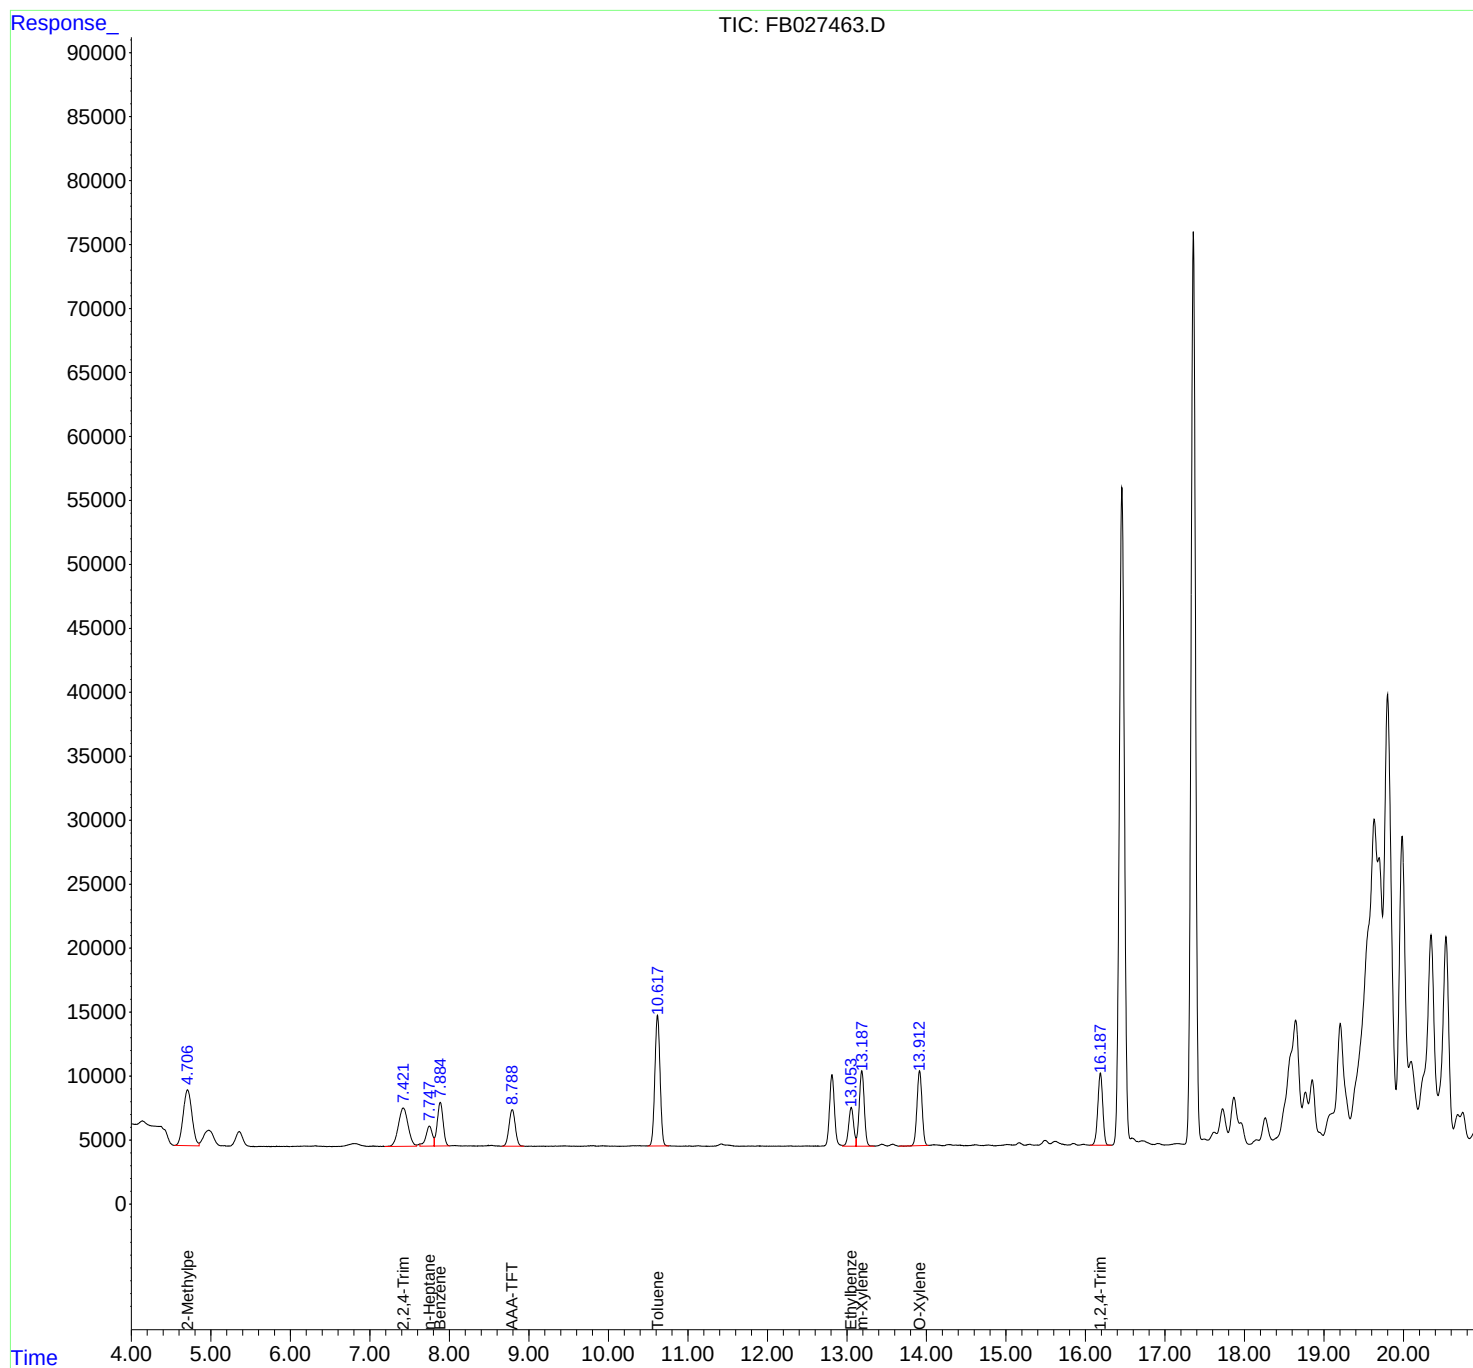


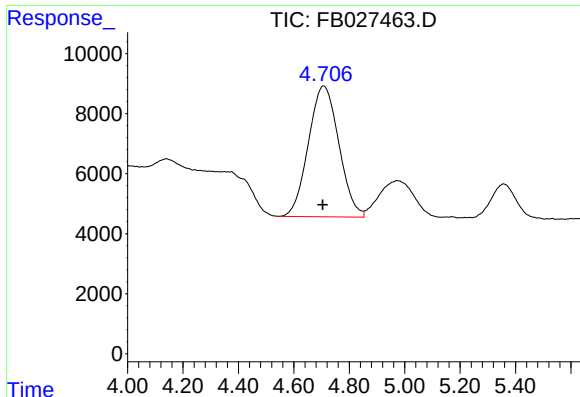

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.003 min
Response: 333001
Conc: 19.77 ng/ml

Instrument :
FID_B
ClientSampleId :
DS-7DMSD

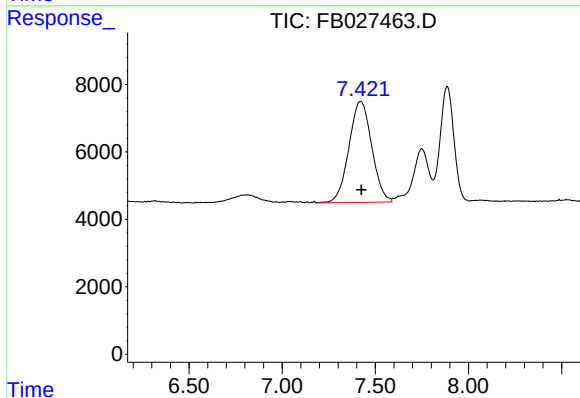


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: -0.004 min
Response: 254590
Conc: 14.50 ng/ml

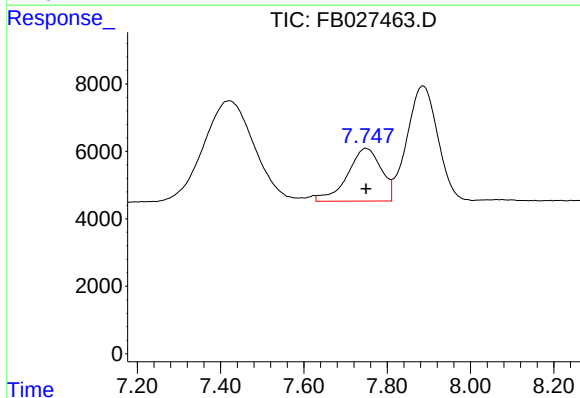


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 87877
Conc: 5.02 ng/ml

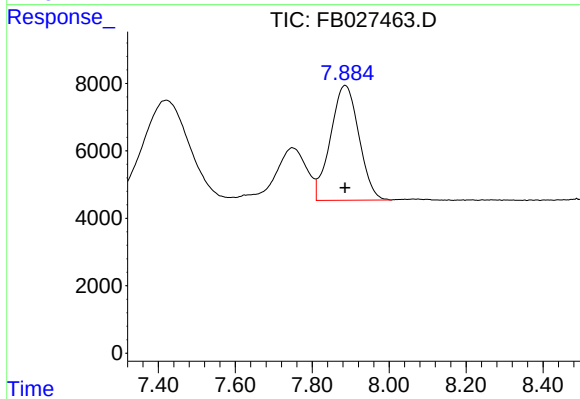

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 174349
Conc: 8.55 ng/ml

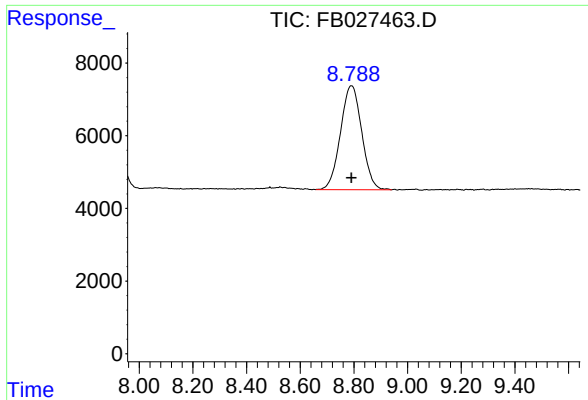

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 157594
Conc: 14.05 ng/ml

Instrument :
FID_B
ClientSampleId :
DS-7DMSD

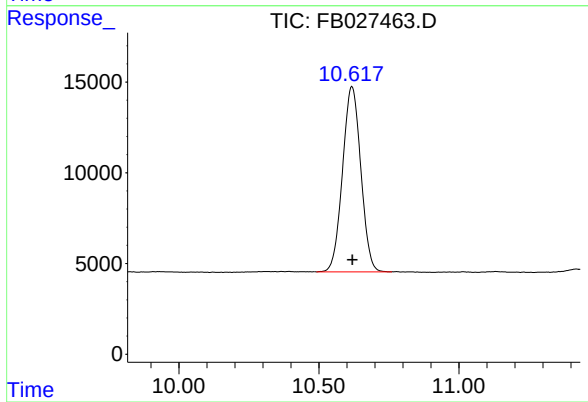


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.001 min
Response: 462953
Conc: 23.91 ng/ml

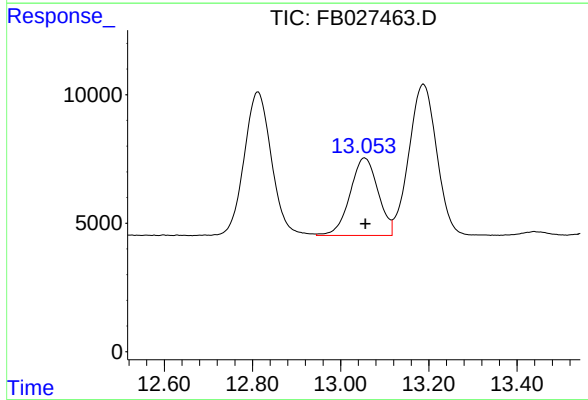


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.002 min
Response: 133257
Conc: 7.36 ng/ml

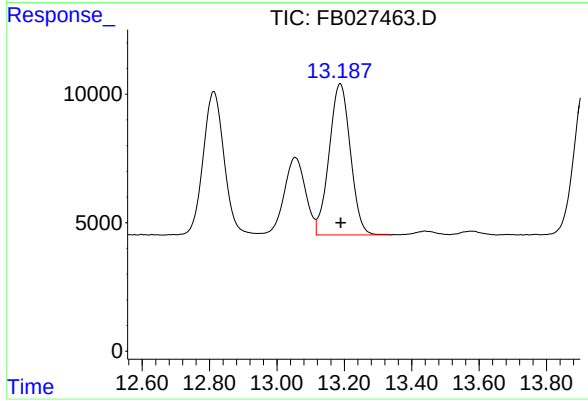

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.001 min
Response: 258291
Conc: 14.49 ng/ml

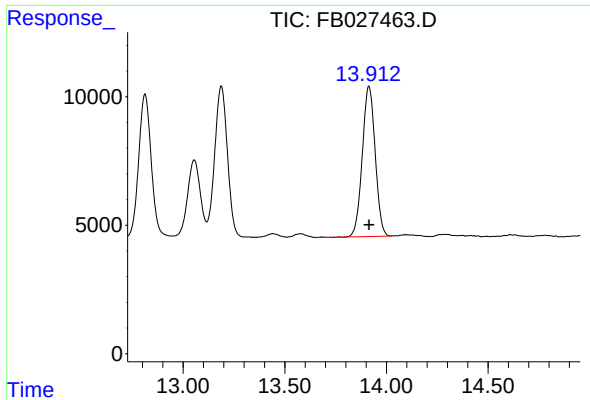

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.002 min
Response: 256874
Conc: 14.78 ng/ml

Instrument :
FID_B
ClientSampleId :
DS-7DMSD

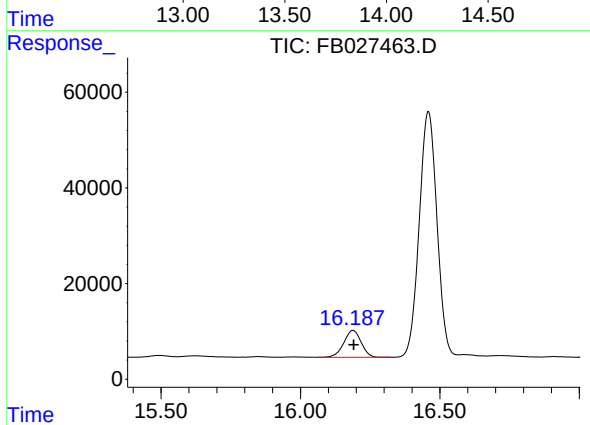

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.003 min
Response: 243971
Conc: 14.20 ng/ml