

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
 Data File : FB027466.D
 Signal(s) : FID2B.CH
 Acq On : 20 Jun 2022 16:36
 Operator : AJ/MA
 Sample : BSF0620S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0620S2

Integration File: Calibration.e
 Quant Time: Jun 21 01:11:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	202724	18.073 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	442781	26.282 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	477960	27.221 ng/ml
3) t n-Heptane	7.752	149356	8.526 ng/ml
4) t Benzene	7.889	180681	8.860 ng/ml
6) t Toluene	10.621	509599	26.319 ng/ml
7) t Ethylbenzene	13.057	157434	8.694 ng/ml
8) t m-Xylene	13.190	313100	17.564 ng/ml
9) t O-Xylene	13.917	307434	17.693 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	313824	18.269 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062022\
Data File : FB027466.D
Signal(s) : FID2B.CH
Acq On : 20 Jun 2022 16:36
Operator : AJ/MA
Sample : BSF0620S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0620S2

Integration File: Calibration.e
Quant Time: Jun 21 01:11:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

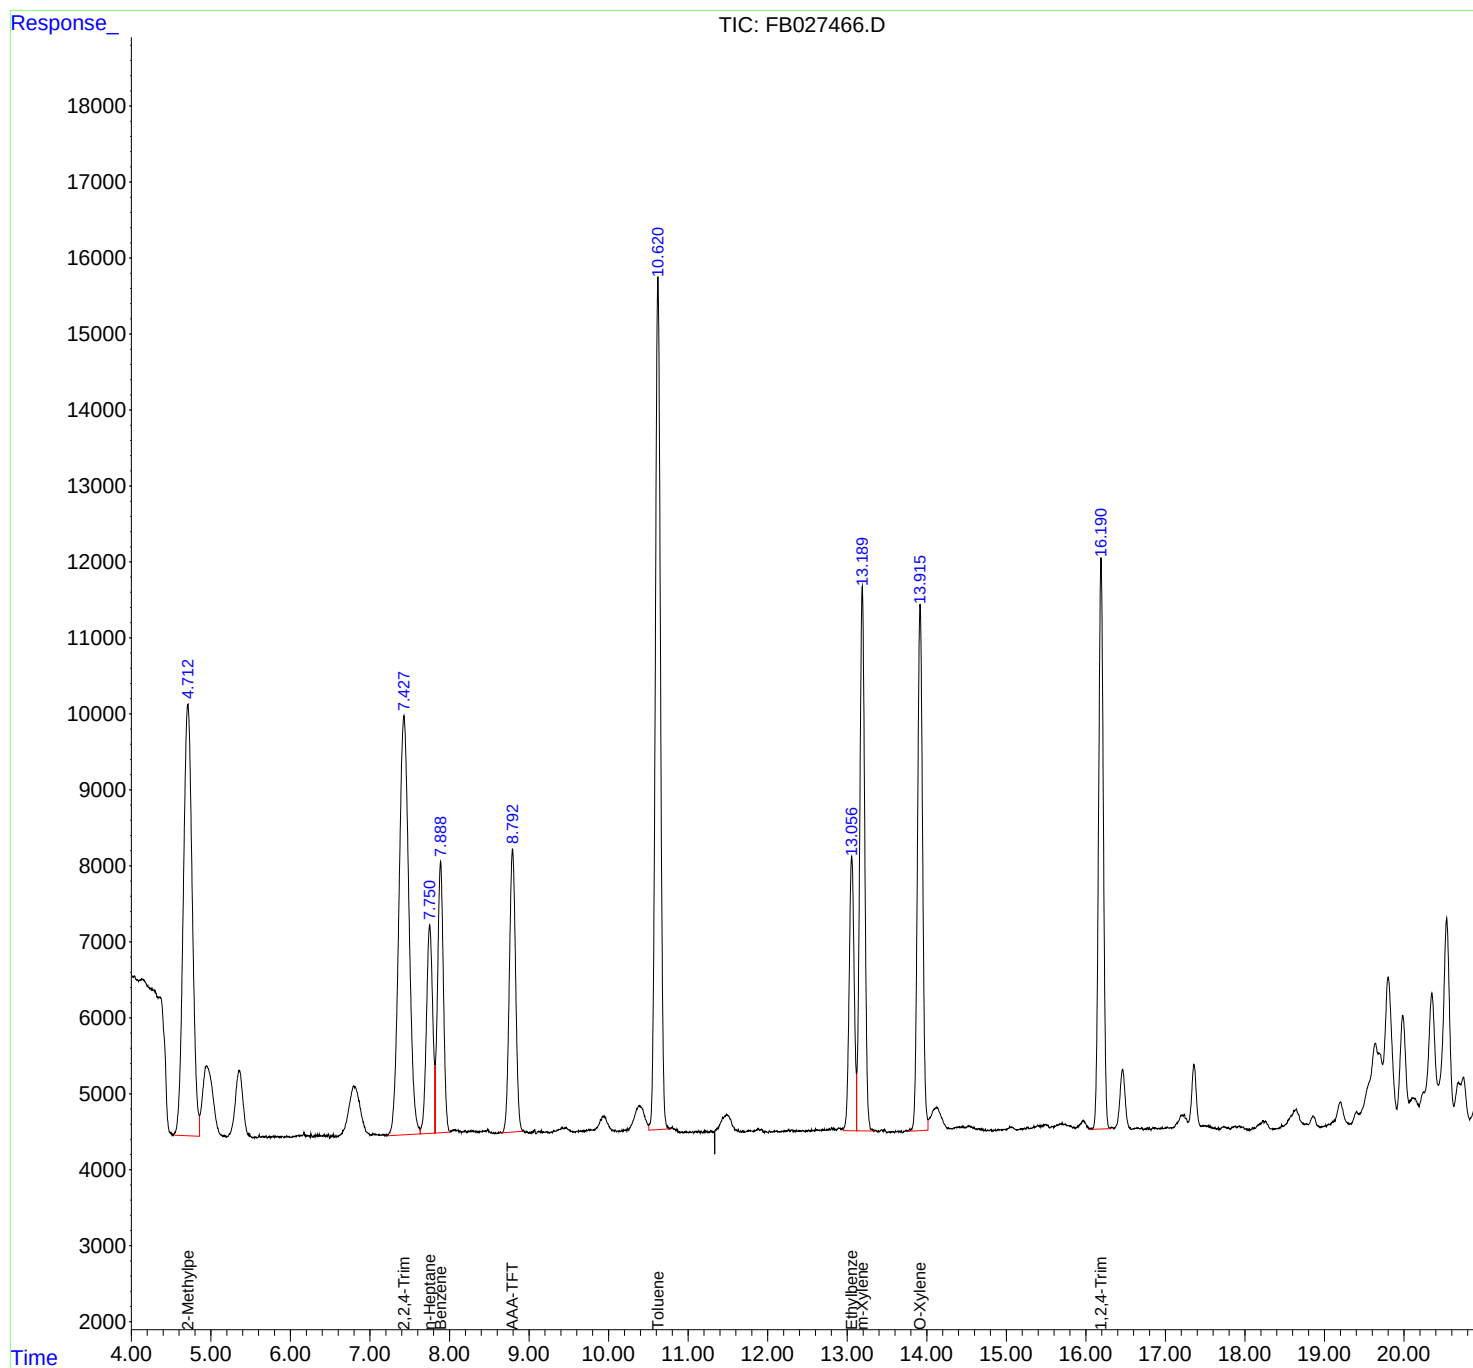


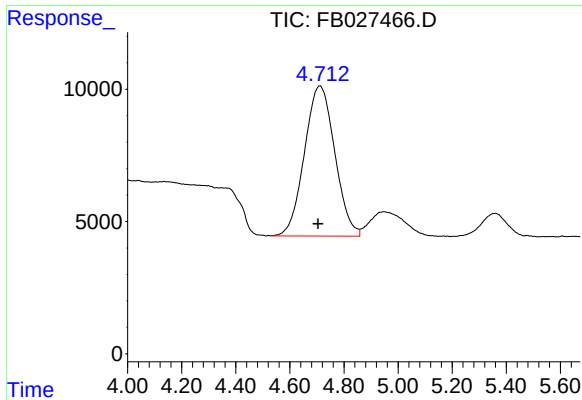

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.008 min
Response: 442781
Conc: 26.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0620S2

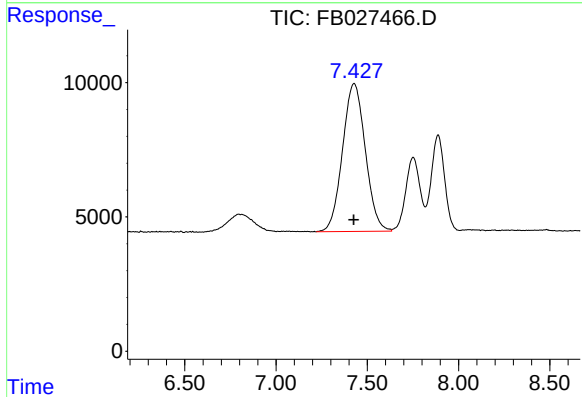


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: 0.002 min
Response: 477960
Conc: 27.22 ng/ml

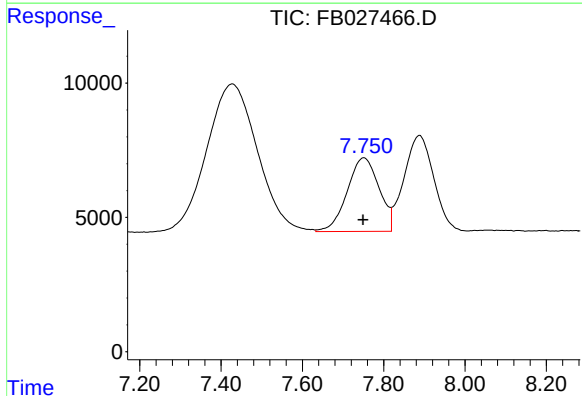


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.002 min
Response: 149356
Conc: 8.53 ng/ml

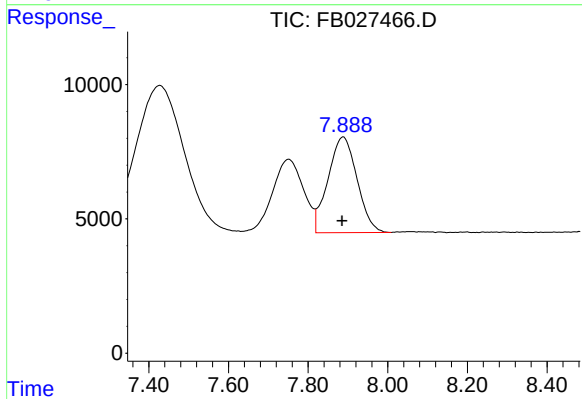

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 180681
Conc: 8.86 ng/ml

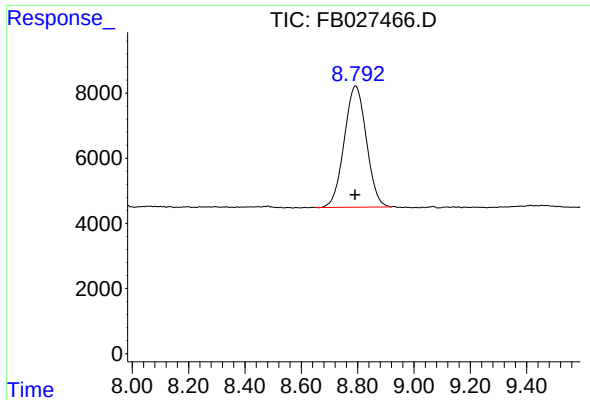

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.003 min
Response: 202724
Conc: 18.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0620S2

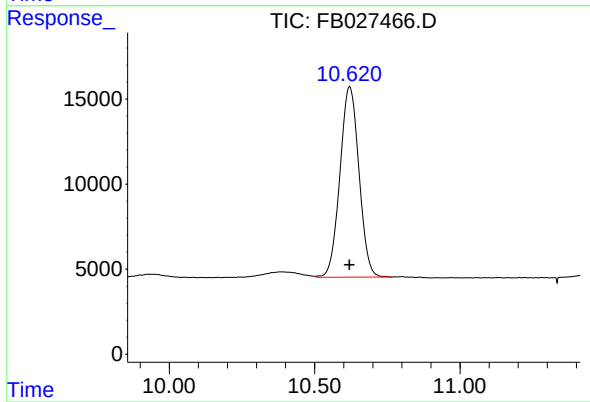


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 509599
Conc: 26.32 ng/ml

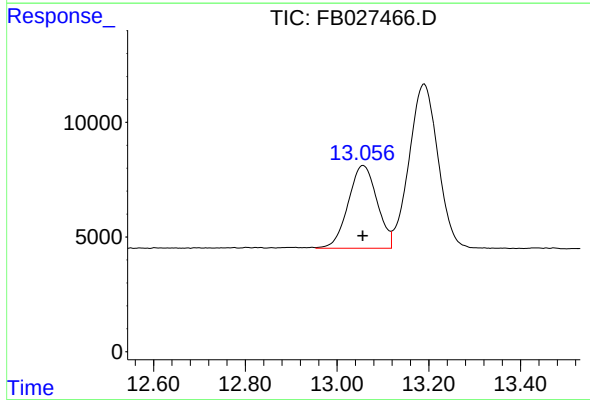


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 157434
Conc: 8.69 ng/ml

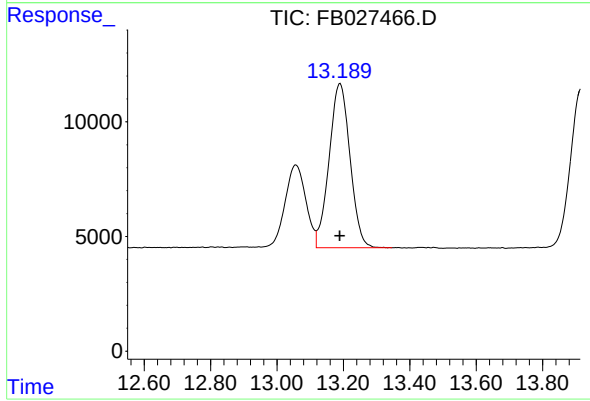

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.001 min
Response: 313100
Conc: 17.56 ng/ml

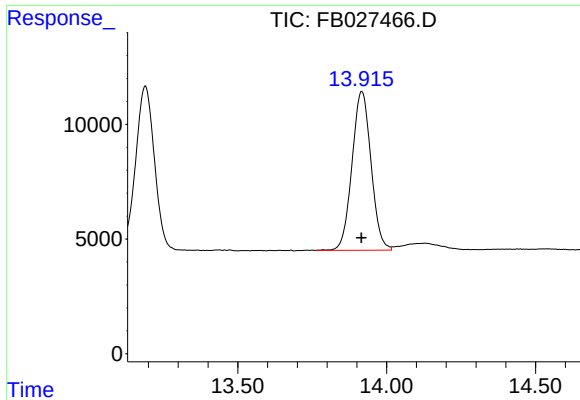

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 307434
Conc: 17.69 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0620S2

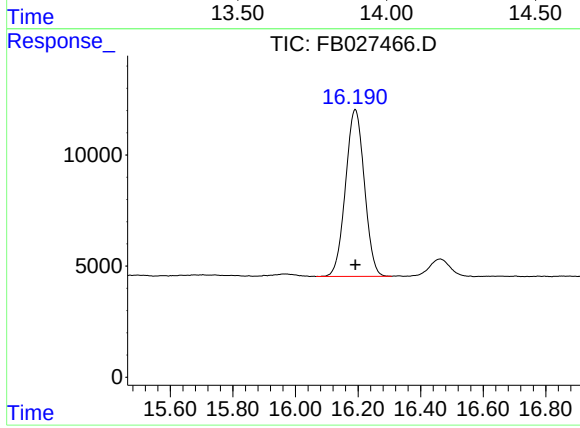

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 313824
Conc: 18.27 ng/ml