

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062119\
 Data File : FB021465.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2019 14:06
 Operator : MJ/SJ
 Sample : K3158-05MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 22 00:15:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
 Quant Title :
 QLast Update : Wed May 29 12:01:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.994	245634	16.660 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.869	533728	14.197 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	511350	14.973 ng/ml
3) t n-Heptane	7.950	147415	4.522 ng/ml
4) t Benzene	8.093	408960	11.848 ng/ml
6) t Toluene	10.835	718441	30.311 ng/ml
7) t Ethylbenzene	13.278	188422	8.064 ng/ml
8) t m-Xylene	13.410	422417	16.924 ng/ml
9) t O-Xylene	14.139	440248	16.876 ng/ml
10) t 1,2,4-Trimethylbenzene	16.419	412472	15.359 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062119\
Data File : FB021465.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2019 14:06
Operator : MJ/SJ
Sample : K3158-05MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 22 00:15:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB052919.M
Quant Title :
QLast Update : Wed May 29 12:01:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

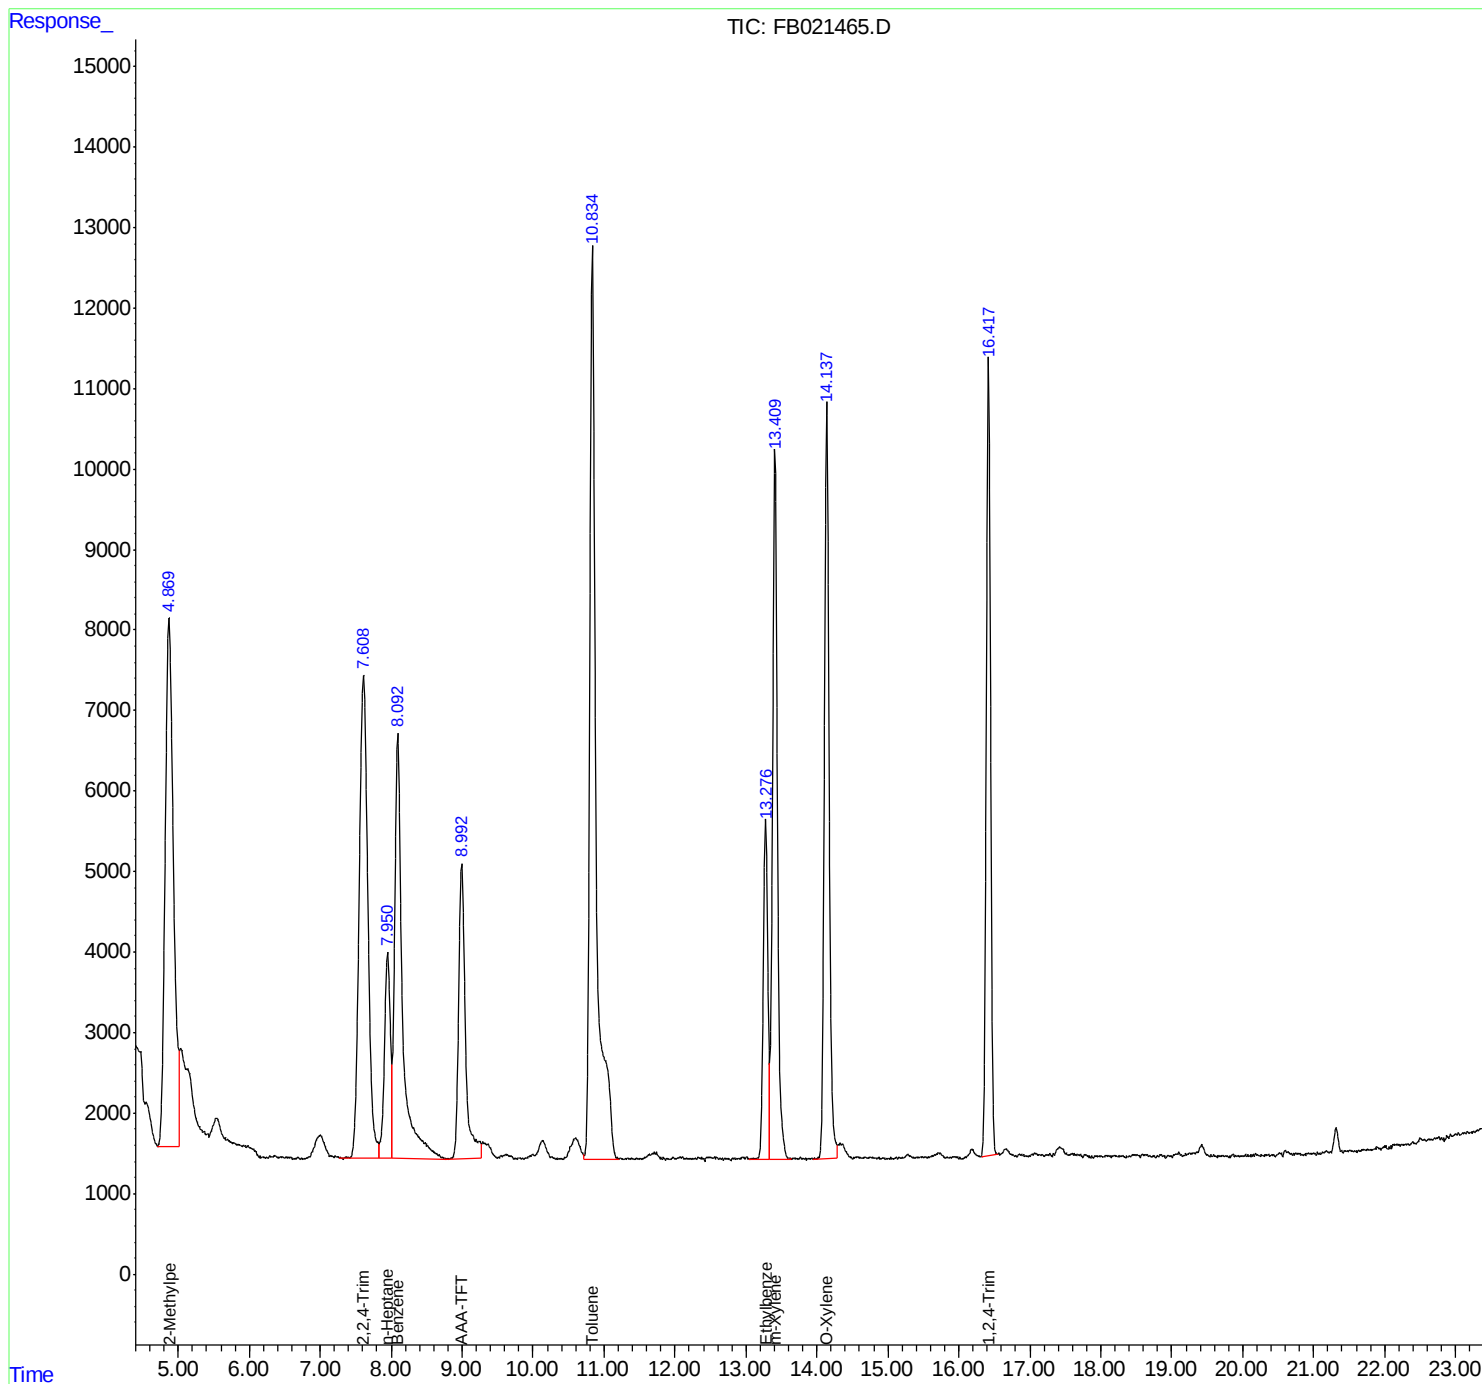

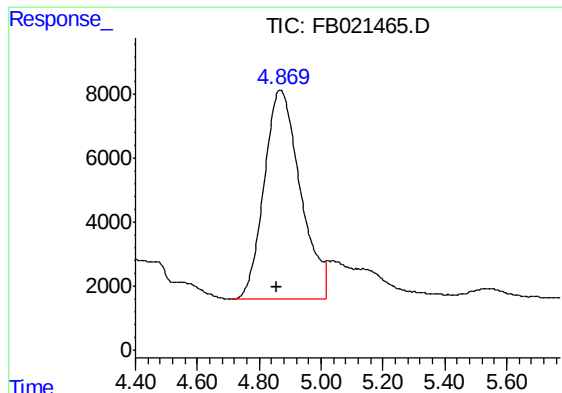


#1 2-Methylpentane

R.T.: 4.869 min
Delta R.T.: 0.011 min
Response: 533728
Conc: 14.20 ng/ml

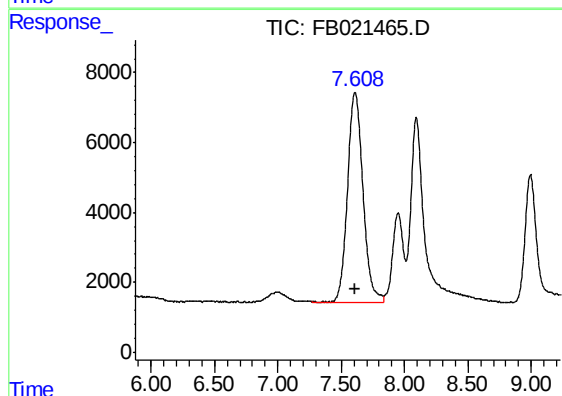


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.003 min
Response: 511350
Conc: 14.97 ng/ml

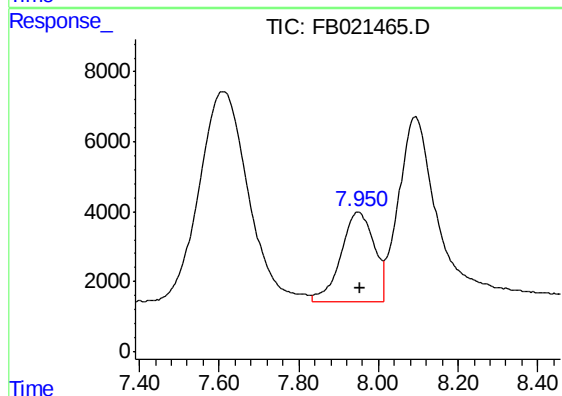


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.004 min
Response: 147415
Conc: 4.52 ng/ml

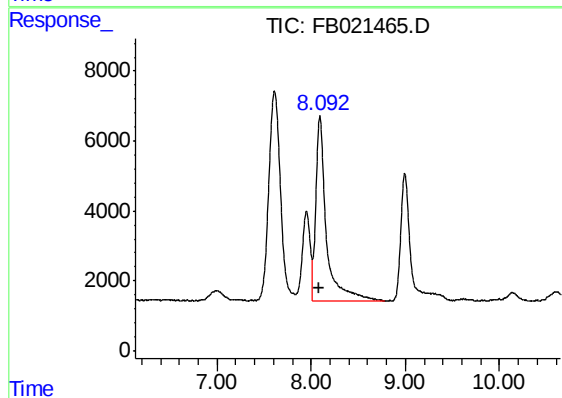


#4 Benzene

R.T.: 8.093 min
Delta R.T.: 0.002 min
Response: 408960
Conc: 11.85 ng/ml

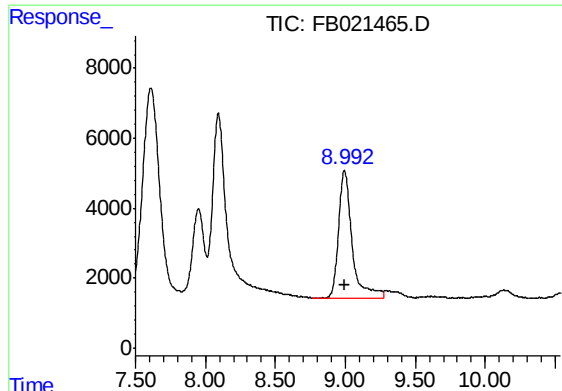


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: -0.004 min
Response: 245634
Conc: 16.66 ng/ml

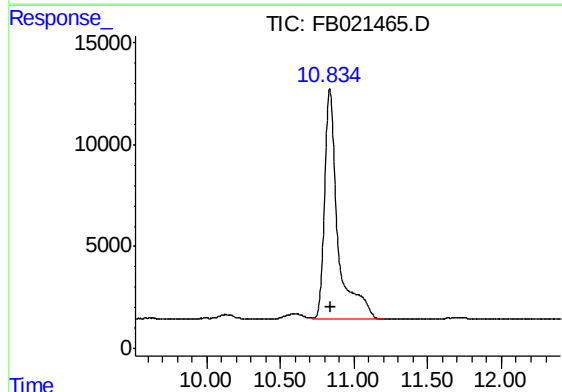


#6 Toluene

R.T.: 10.835 min
Delta R.T.: -0.007 min
Response: 718441
Conc: 30.31 ng/ml

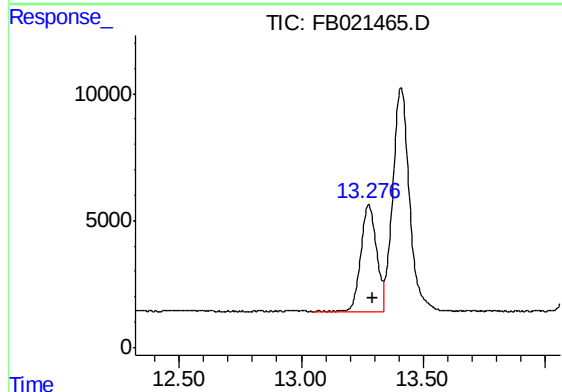


#7 Ethylbenzene

R.T.: 13.278 min
Delta R.T.: -0.016 min
Response: 188422
Conc: 8.06 ng/ml

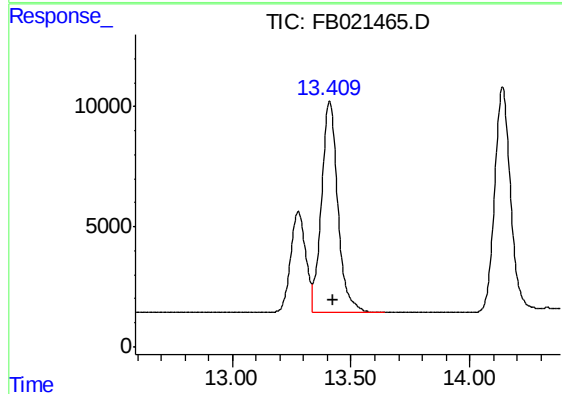


#8 m-Xylene

R.T.: 13.410 min
Delta R.T.: -0.016 min
Response: 422417
Conc: 16.92 ng/ml

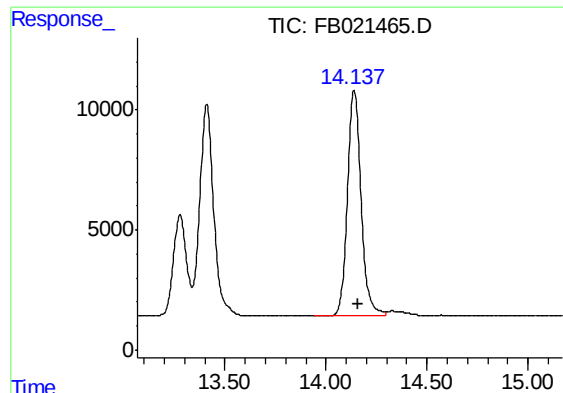

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: -0.018 min
Response: 440248
Conc: 16.88 ng/ml

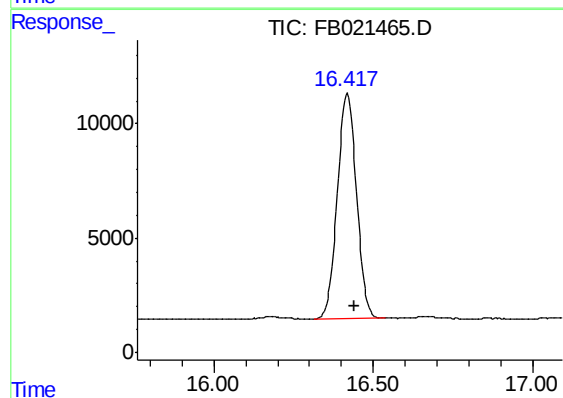

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: -0.022 min
Response: 412472
Conc: 15.36 ng/ml