

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
 Data File : FB027474.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2022 16:40
 Operator : AJ/MA
 Sample : N3422-11
 Misc : 4.99G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 22 04:27:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.857	992588	88.492 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.700	298688	17.729 ng/ml
2) t 2,2,4-Trimethylpentane	7.375	306917	17.480 ng/ml
3) t n-Heptane	7.758	636945	36.358 ng/ml
7) t Ethylbenzene	13.024	186005	10.271 ng/ml
8) t m-Xylene	13.183	50096	2.810 ng/ml
9) t O-Xylene	13.917	31266	1.799 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
Data File : FB027474.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2022 16:40
Operator : AJ/MA
Sample : N3422-11
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 22 04:27:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

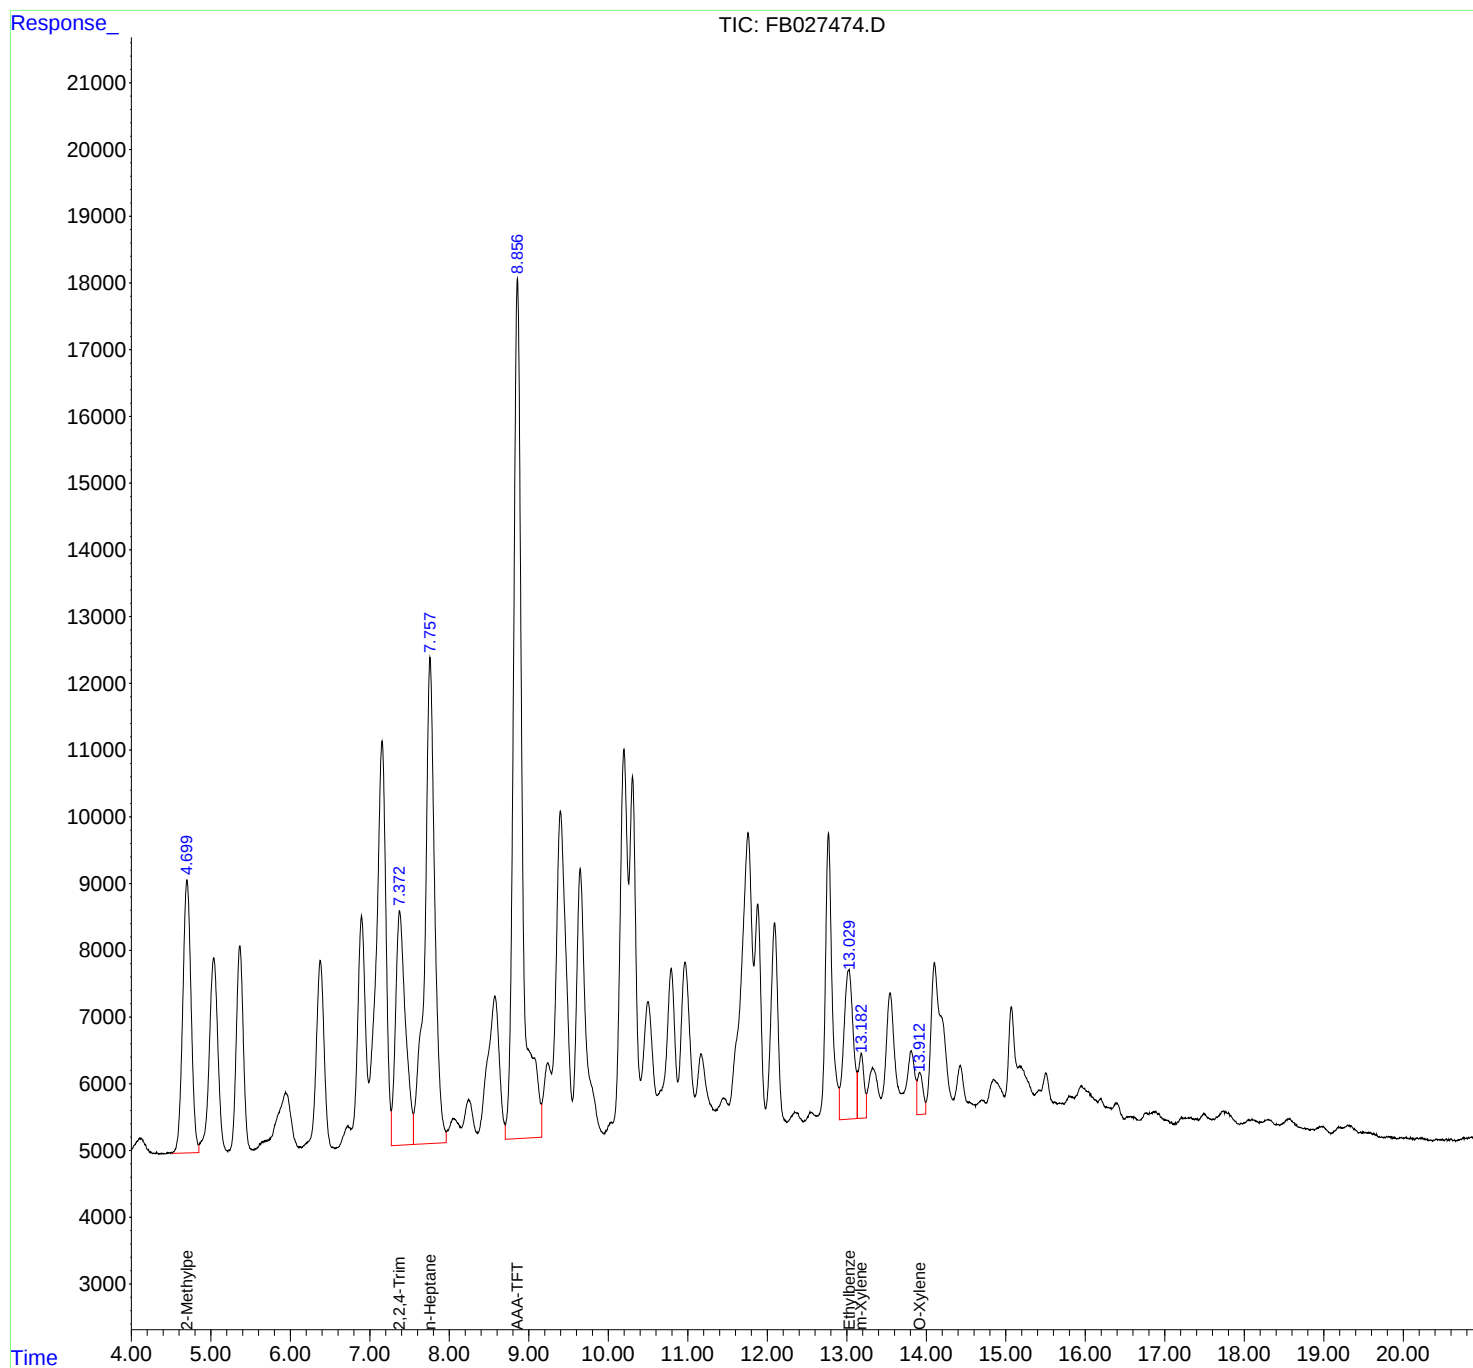


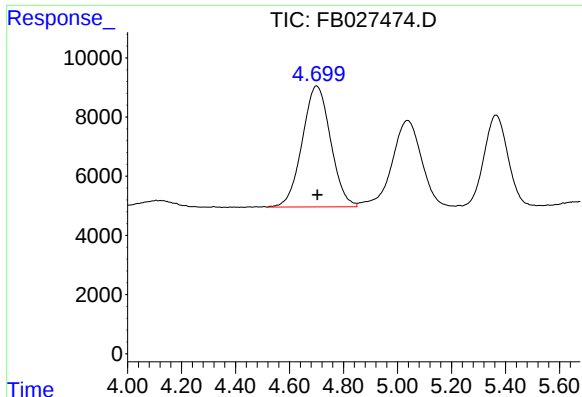

#1 2-Methylpentane


R.T.: 4.700 min
Delta R.T.: -0.004 min
Response: 298688
Conc: 17.73 ng/ml

Instrument :
FID_B
ClientSampleId :

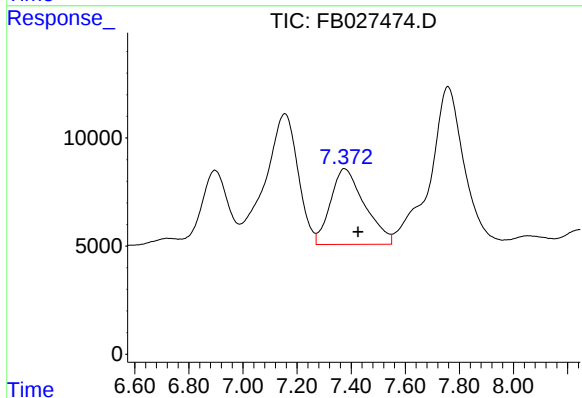


#2 2,2,4-Trimethylpentane

R.T.: 7.375 min
Delta R.T.: -0.051 min
Response: 306917
Conc: 17.48 ng/ml

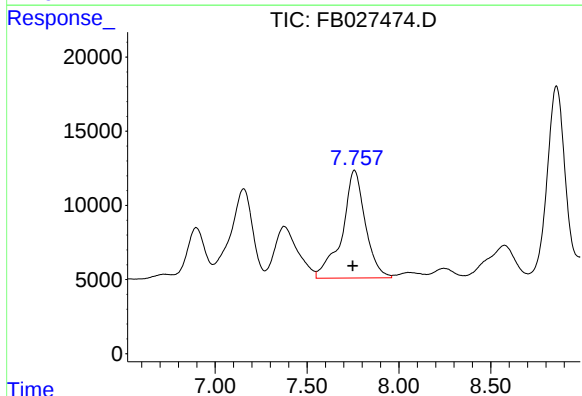


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.008 min
Response: 636945
Conc: 36.36 ng/ml

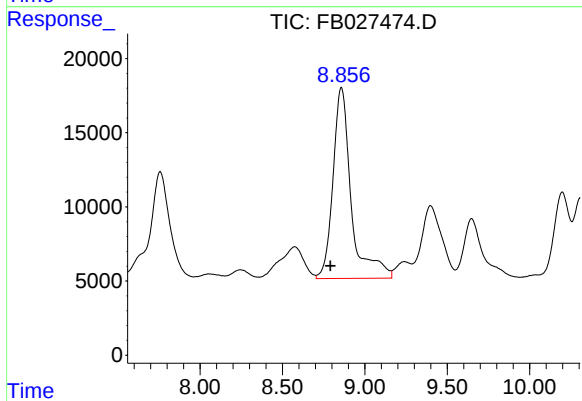

#5 AAA-TFT


R.T.: 8.857 min
Delta R.T.: 0.066 min
Response: 992588
Conc: 88.49 ng/ml

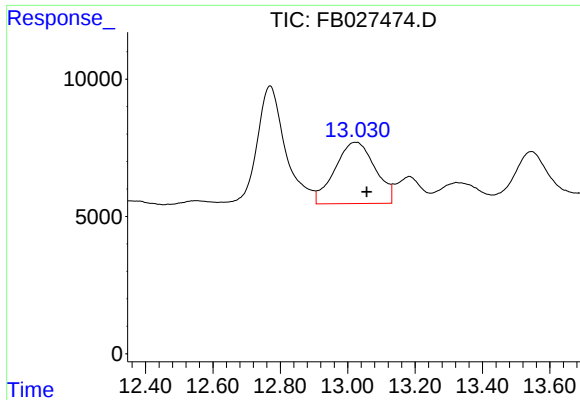

#7 Ethylbenzene


R.T.: 13.024 min
Delta R.T.: -0.032 min
Response: 186005
Conc: 10.27 ng/ml

Instrument :
FID_B
ClientSampleId :

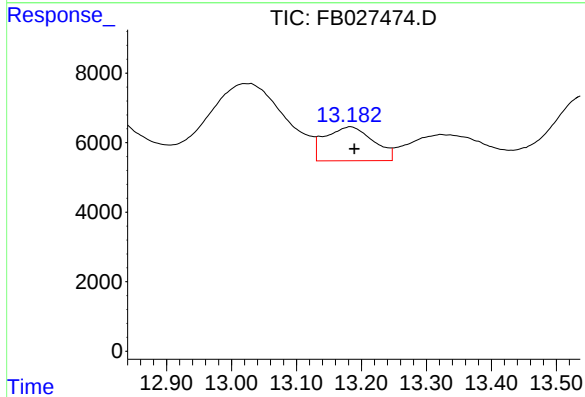

#8 m-Xylene

R.T.: 13.183 min
Delta R.T.: -0.006 min
Response: 50096
Conc: 2.81 ng/ml

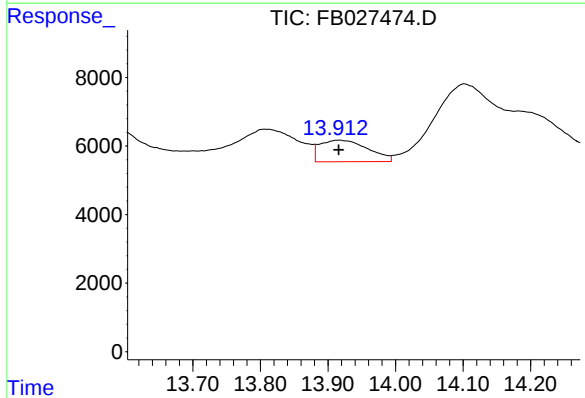

#9 o-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 31266
Conc: 1.80 ng/ml