

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
 Data File : FB027475.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2022 17:17
 Operator : AJ/MA
 Sample : N3422-05
 Misc : 4.99G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 22 04:27:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.824	280129	24.974 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.699	15667	0.930 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	19041	1.084 ng/ml
3) t n-Heptane	7.815	52794	3.014 ng/ml
6) t Toluene	10.613	1982	0.102 ng/ml
7) t Ethylbenzene	13.024	413890	22.855 ng/ml
9) t O-Xylene	13.929	79661	4.585 ng/ml
10) t 1,2,4-Trimethylbenzene	16.223	336804	19.606 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
Data File : FB027475.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2022 17:17
Operator : AJ/MA
Sample : N3422-05
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 22 04:27:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

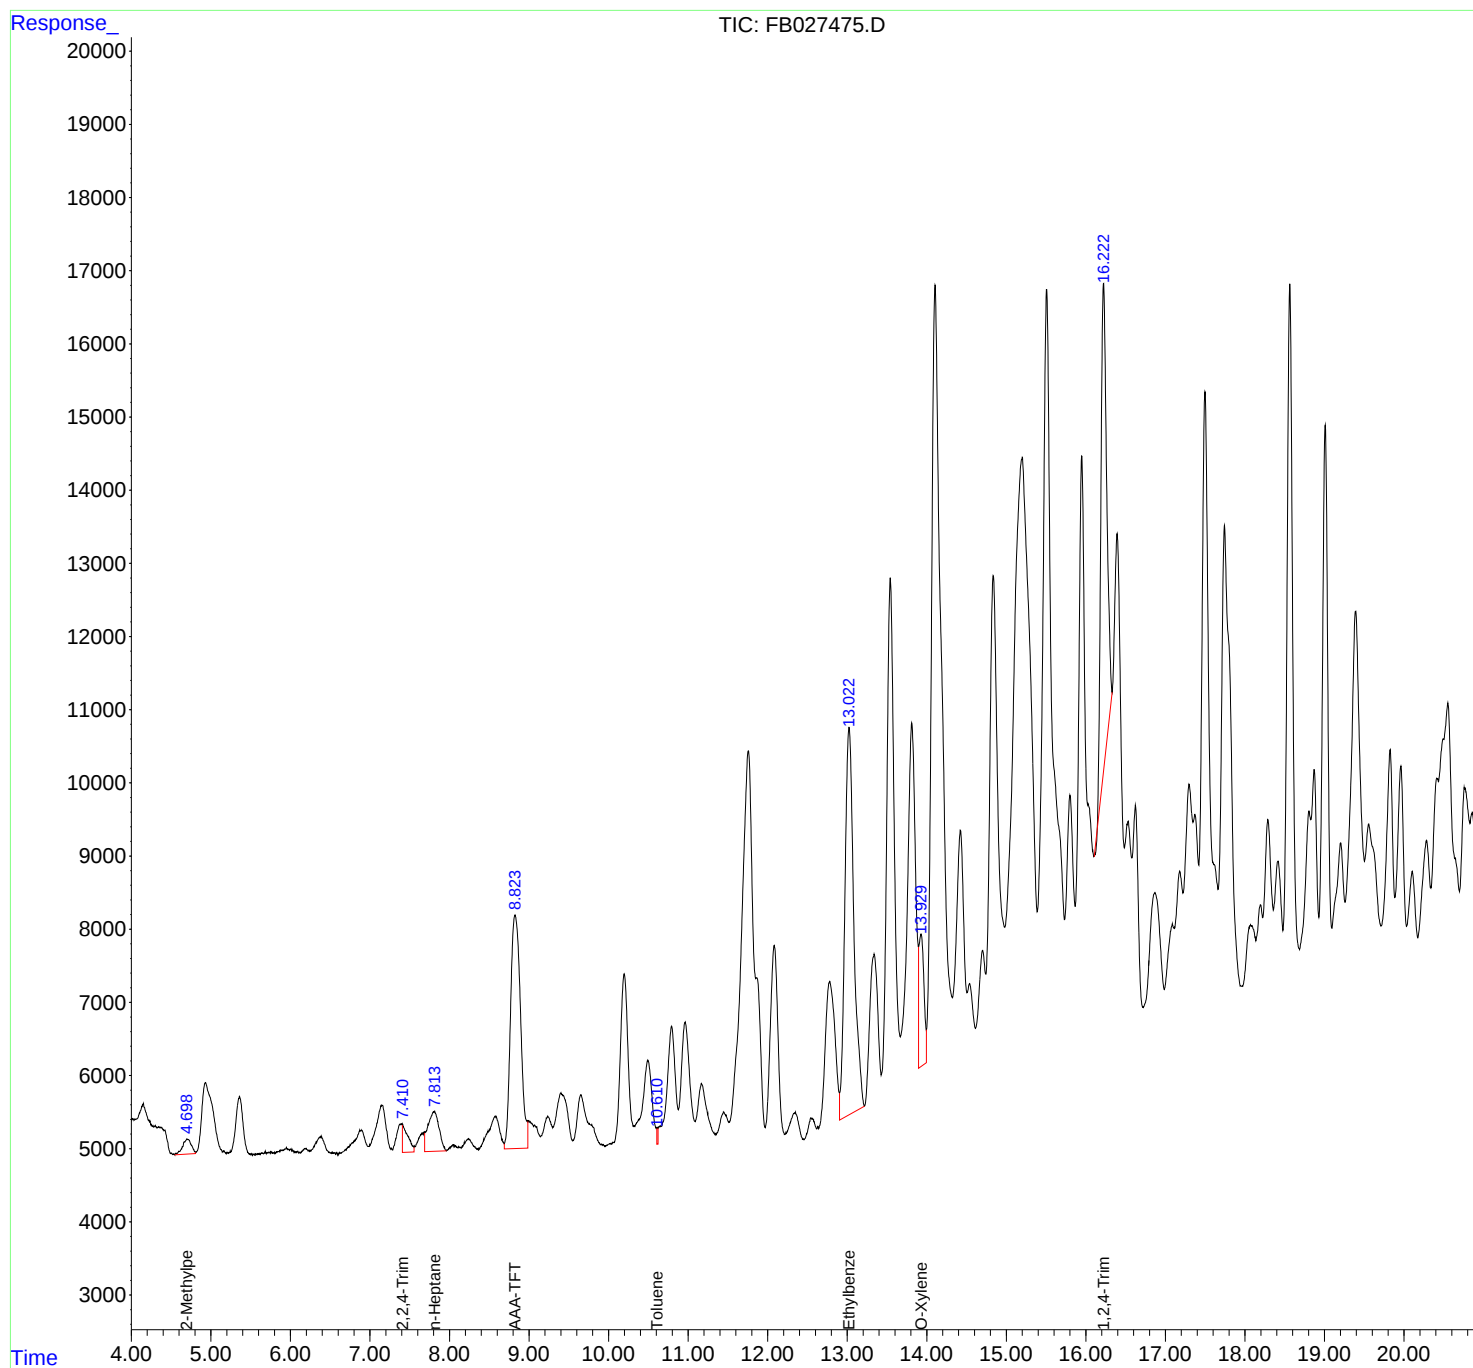


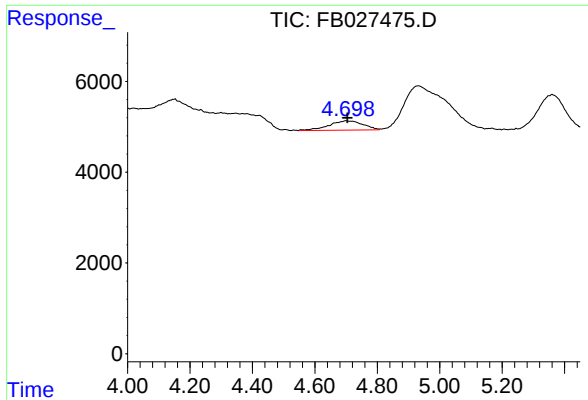

#1 2-Methylpentane

R.T.: 4.699 min
Delta R.T.: -0.005 min
Response: 15667
Conc: 0.93 ng/ml

Instrument :
FID_B
ClientSampleId :

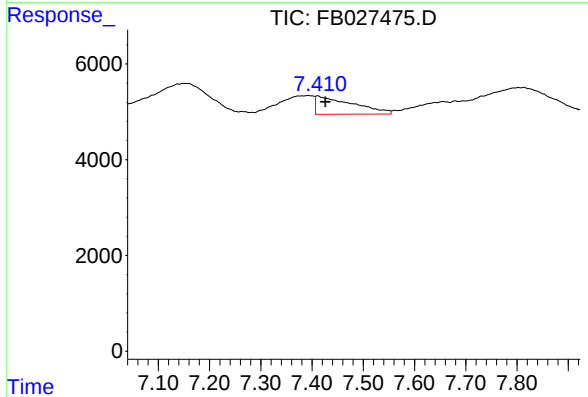

#2 2,2,4-Trimethylpentane


R.T.: 7.412 min
Delta R.T.: -0.014 min
Response: 19041
Conc: 1.08 ng/ml

#3 n-Heptane

R.T.: 7.815 min
Delta R.T.: 0.065 min
Response: 52794
Conc: 3.01 ng/ml

#5 AAA-TFT


R.T.: 8.824 min
Delta R.T.: 0.034 min
Response: 280129
Conc: 24.97 ng/ml

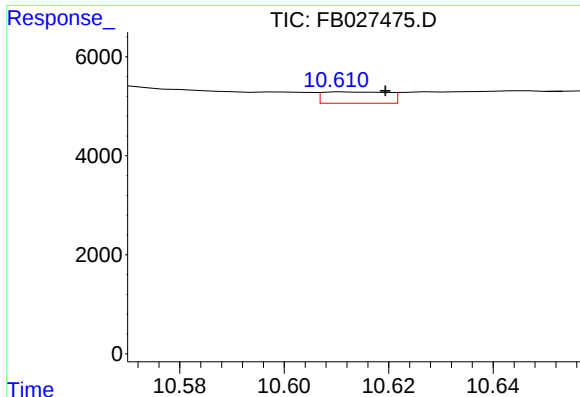

#6 Toluene


R.T.: 10.613 min
Delta R.T.: -0.007 min
Response: 1982
Conc: 0.10 ng/ml

Instrument :
FID_B
ClientSampleId :

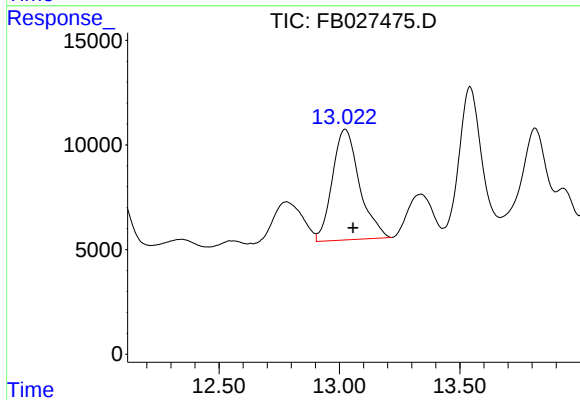


#7 Ethylbenzene

R.T.: 13.024 min
Delta R.T.: -0.032 min
Response: 413890
Conc: 22.85 ng/ml

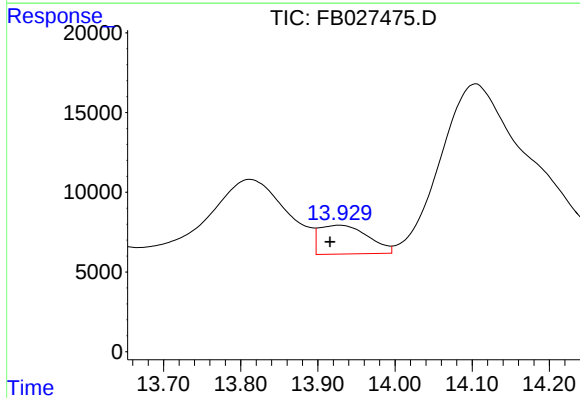

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.013 min
Response: 79661
Conc: 4.58 ng/ml

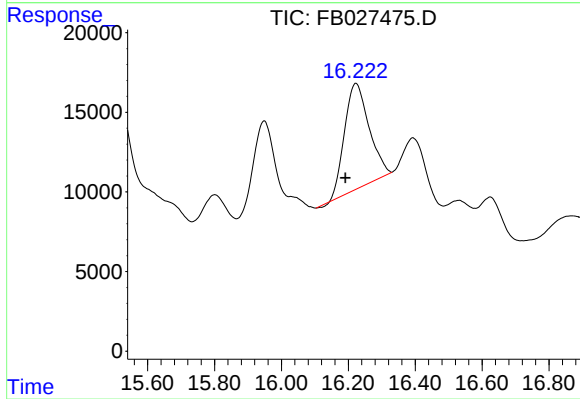

#10 1,2,4-Trimethylbenzene

R.T.: 16.223 min
Delta R.T.: 0.032 min
Response: 336804
Conc: 19.61 ng/ml