

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
 Data File : FB027476.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2022 17:54
 Operator : AJ/MA
 Sample : N3422-11
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 22 04:28:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.857	3617644	322.524 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.700	1231827	73.117 ng/ml
2) t 2,2,4-Trimethylpentane	7.376	1131196	64.425 ng/ml
3) t n-Heptane	7.756	2821087	161.032 ng/ml
7) t Ethylbenzene	13.028	962969	53.175 ng/ml
8) t m-Xylene	13.182	271171	15.212 ng/ml
9) t O-Xylene	13.918	188861	10.869 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	104205	6.066 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
Data File : FB027476.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2022 17:54
Operator : AJ/MA
Sample : N3422-11
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 22 04:28:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

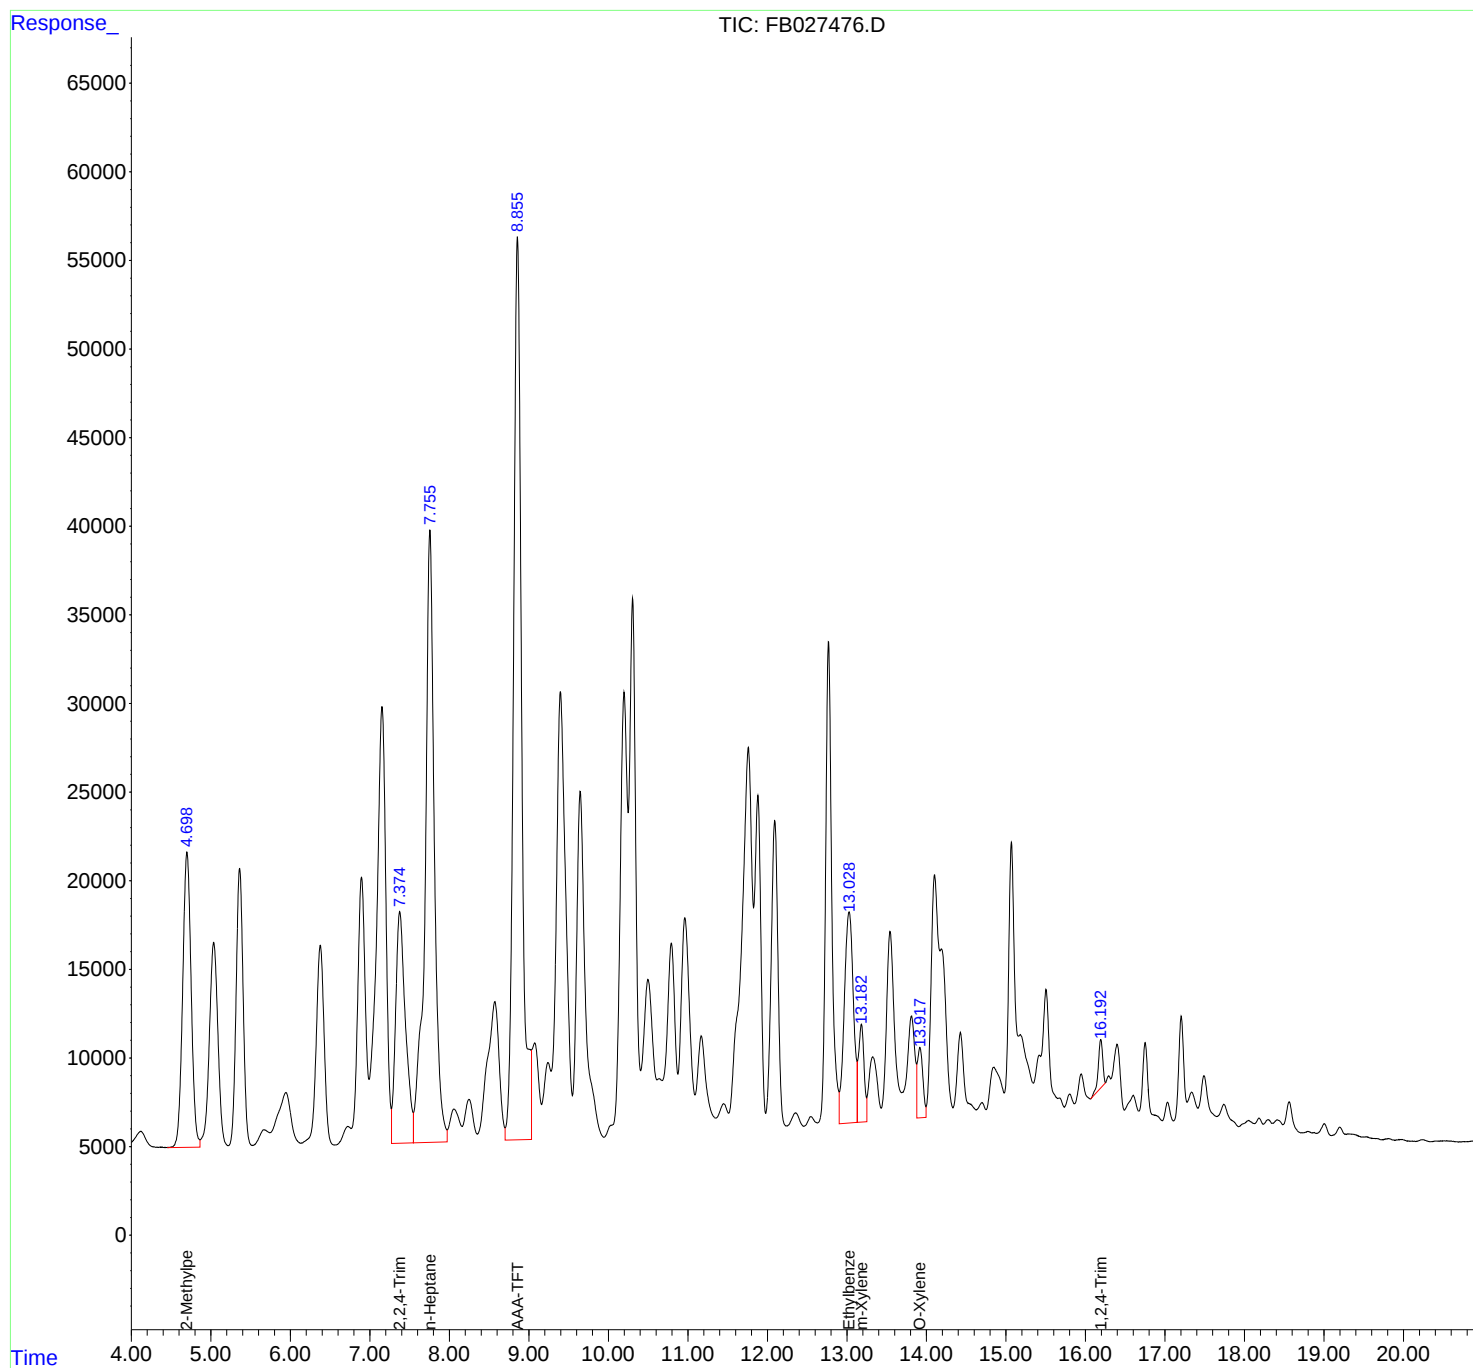


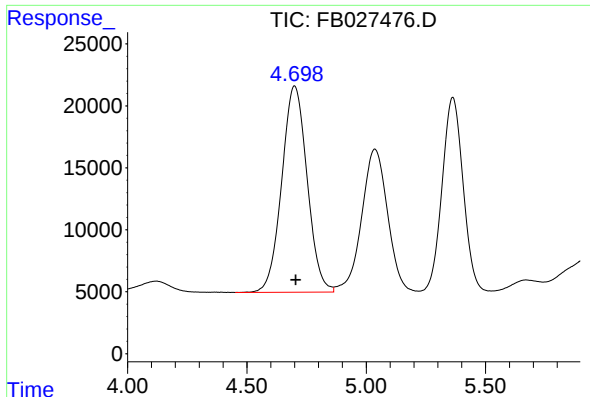

#1 2-Methylpentane


R.T.: 4.700 min
Delta R.T.: -0.004 min
Response: 1231827
Conc: 73.12 ng/ml

Instrument :
FID_B
ClientSampleId :

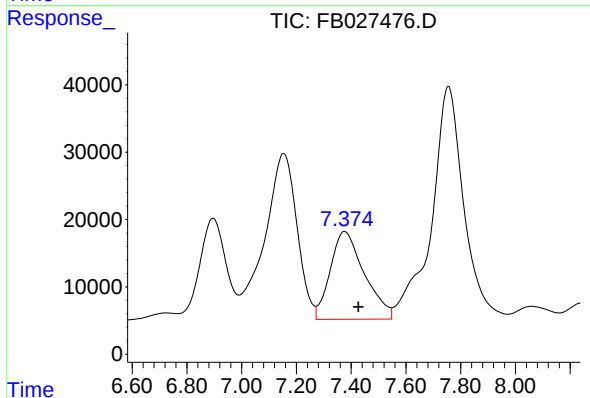


#2 2,2,4-Trimethylpentane

R.T.: 7.376 min
Delta R.T.: -0.050 min
Response: 1131196
Conc: 64.42 ng/ml

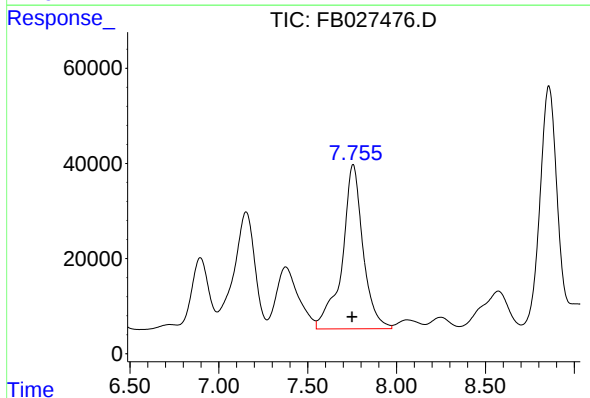


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.006 min
Response: 2821087
Conc: 161.03 ng/ml

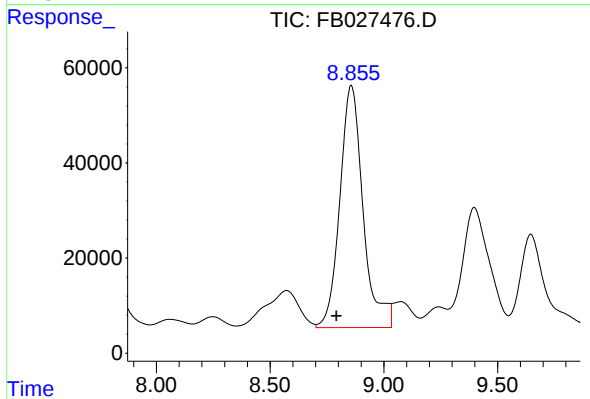

#5 AAA-TFT


R.T.: 8.857 min
Delta R.T.: 0.066 min
Response: 3617644
Conc: 322.52 ng/ml

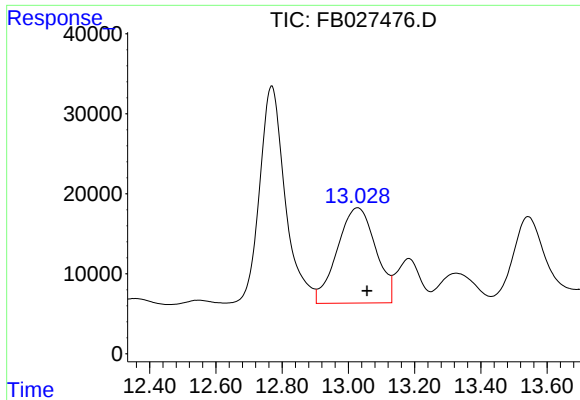

#7 Ethylbenzene


R.T.: 13.028 min
Delta R.T.: -0.029 min
Response: 962969
Conc: 53.18 ng/ml

Instrument :
FID_B
ClientSampleId :

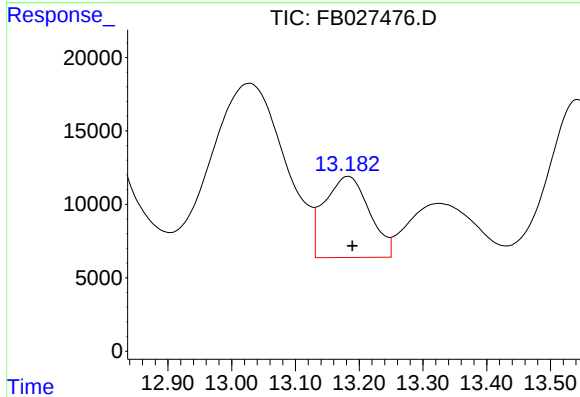


#8 m-Xylene

R.T.: 13.182 min
Delta R.T.: -0.007 min
Response: 271171
Conc: 15.21 ng/ml

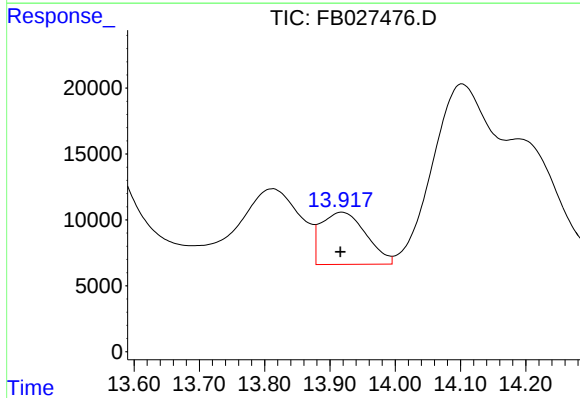

#9 o-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 188861
Conc: 10.87 ng/ml

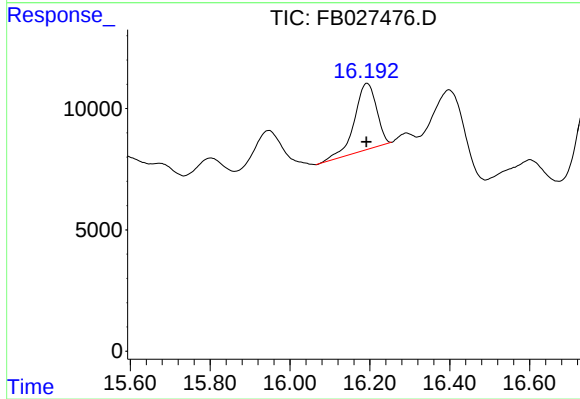

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.002 min
Response: 104205
Conc: 6.07 ng/ml