

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
 Data File : FB027478.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2022 19:07
 Operator : AJ/MA
 Sample : N3422-05MSD
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 22 04:28:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.827	27731	2.472 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.698	17791	1.056 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	6954	0.396 ng/ml
3) t n-Heptane	7.765	3703	0.211 ng/ml
4) t Benzene	7.891	10356	0.508 ng/ml
6) t Toluene	10.625	18815	0.972 ng/ml
7) t Ethylbenzene	13.032	43064	2.378 ng/ml
8) t m-Xylene	13.189	5674	0.318 ng/ml
9) t O-Xylene	13.926	10442	0.601 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	5552	0.323 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
Data File : FB027478.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2022 19:07
Operator : AJ/MA
Sample : N3422-05MSD
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 22 04:28:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

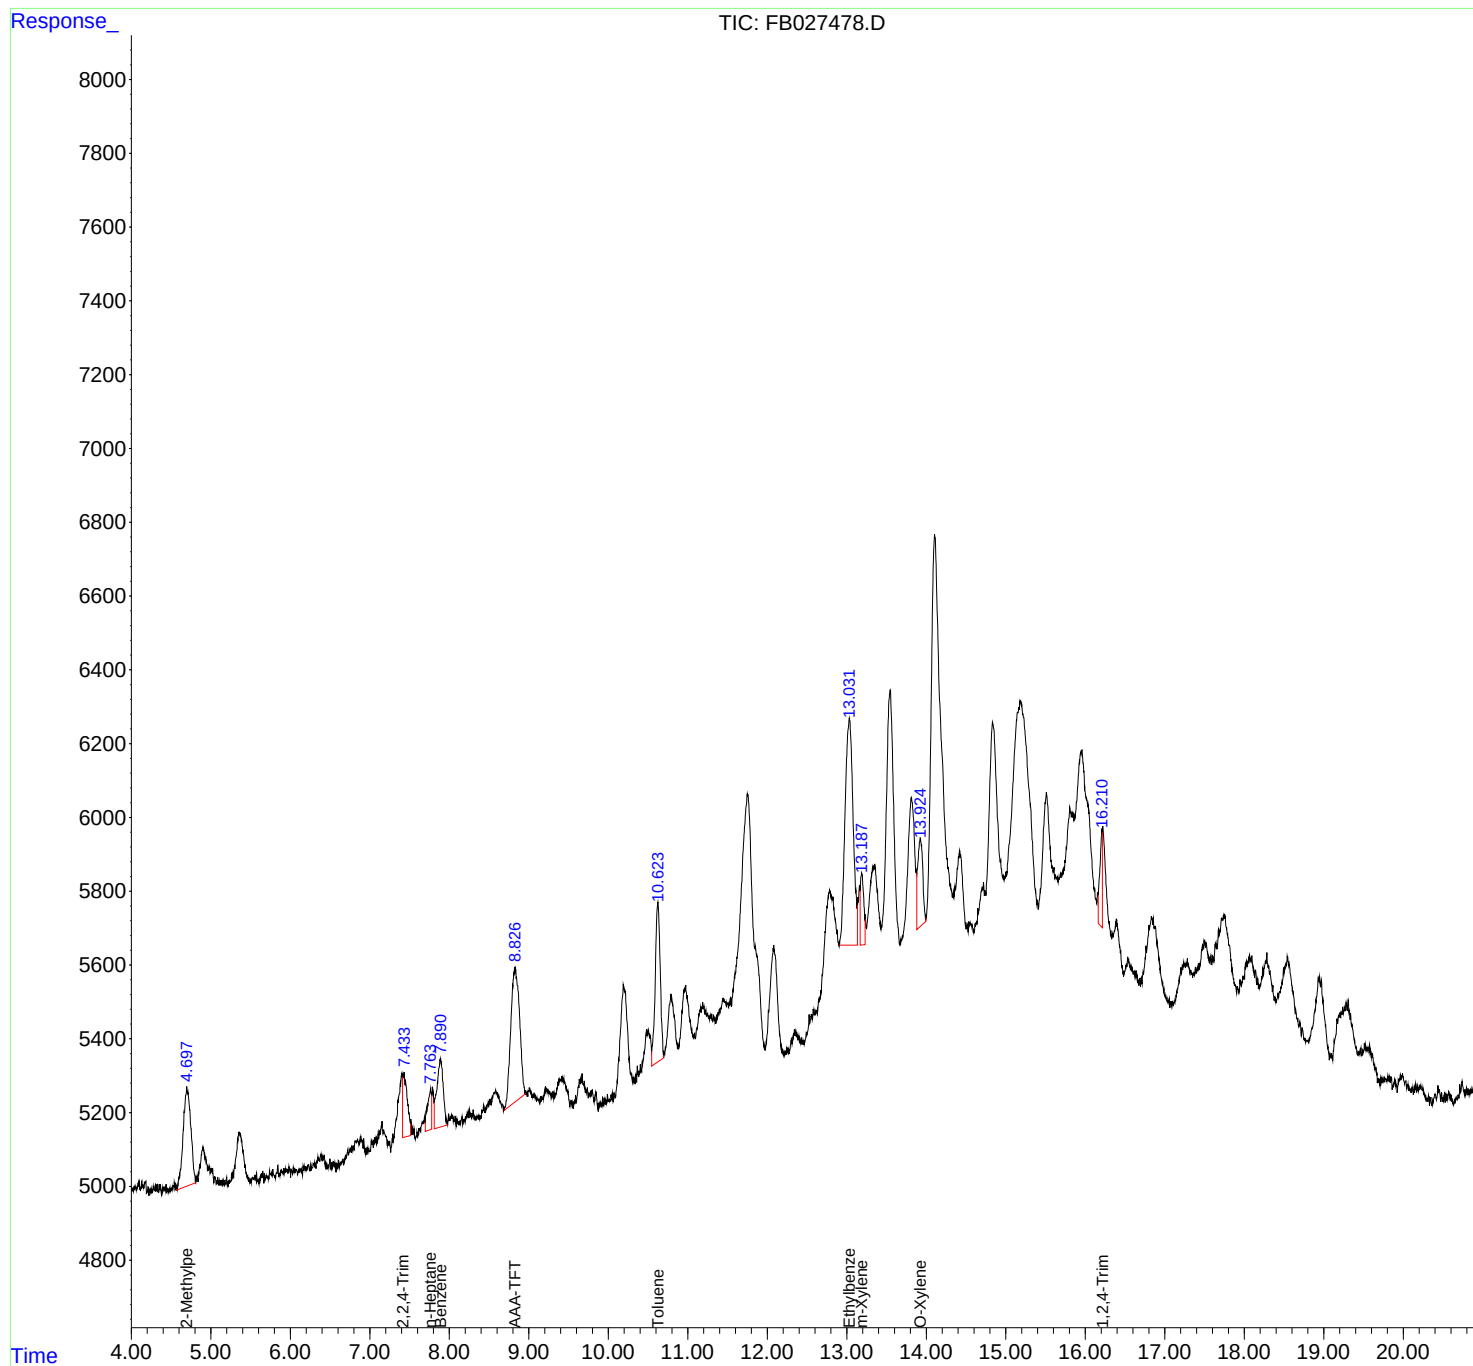


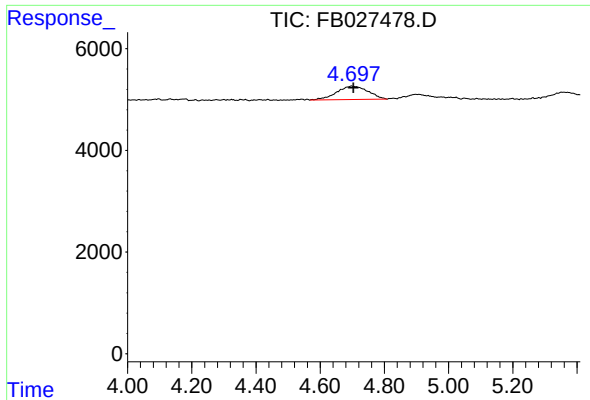

#1 2-Methylpentane


R.T.: 4.698 min
Delta R.T.: -0.006 min
Response: 17791
Conc: 1.06 ng/ml

Instrument :
FID_B
ClientSampleId :

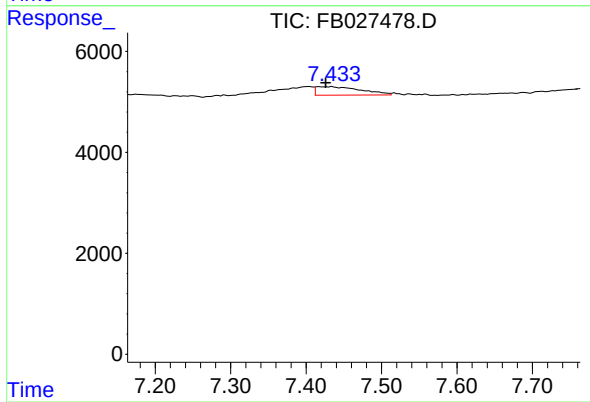


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.009 min
Response: 6954
Conc: 0.40 ng/ml

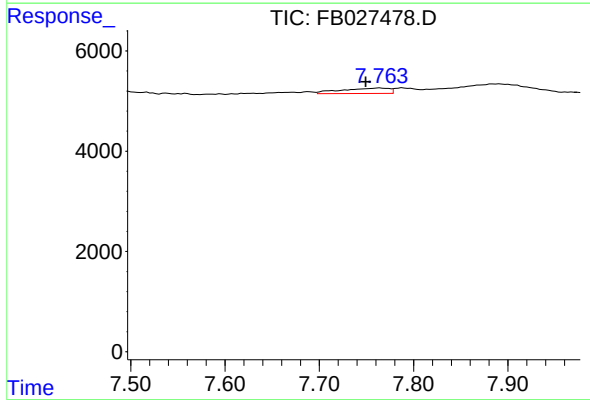


#3 n-Heptane

R.T.: 7.765 min
Delta R.T.: 0.015 min
Response: 3703
Conc: 0.21 ng/ml

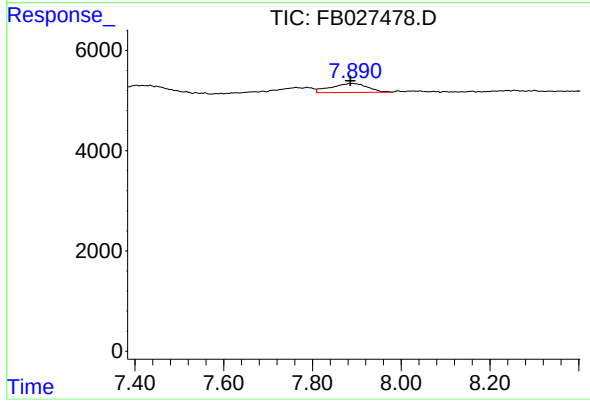

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.006 min
Response: 10356
Conc: 0.51 ng/ml

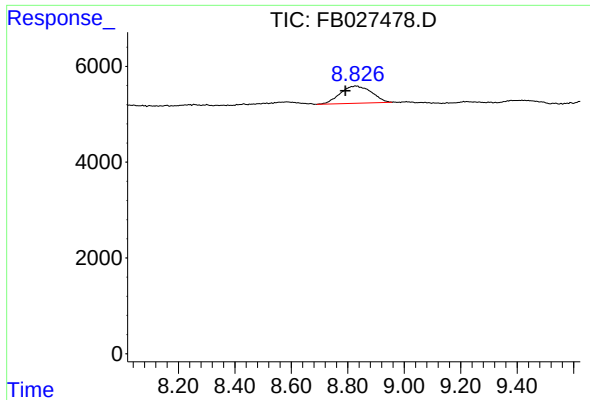

#5 AAA-TFT


R.T.: 8.827 min
Delta R.T.: 0.036 min
Response: 27731
Conc: 2.47 ng/ml

Instrument :
FID_B
ClientSampleId :

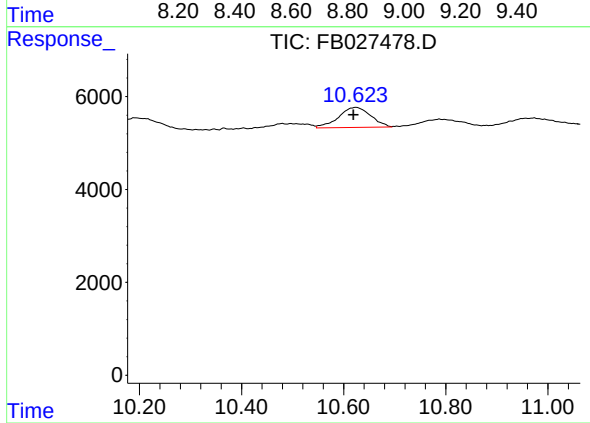


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.006 min
Response: 18815
Conc: 0.97 ng/ml

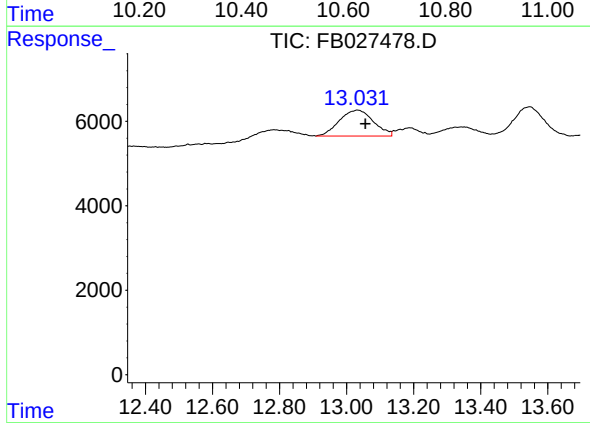


#7 Ethylbenzene

R.T.: 13.032 min
Delta R.T.: -0.024 min
Response: 43064
Conc: 2.38 ng/ml

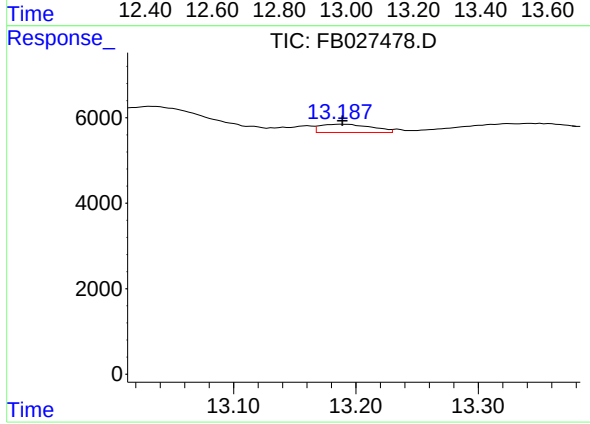

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 5674
Conc: 0.32 ng/ml

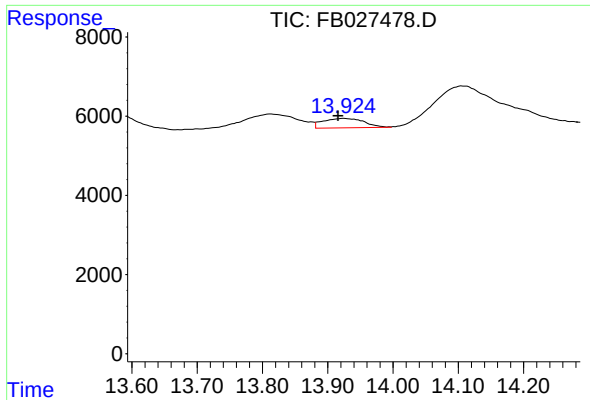

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.010 min
Response: 10442
Conc: 0.60 ng/ml

Instrument :
FID_B
ClientSampleId :

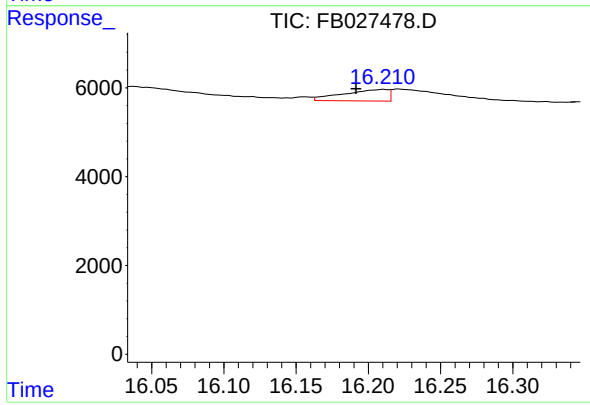

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.020 min
Response: 5552
Conc: 0.32 ng/ml