

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
 Data File : FB027480.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2022 20:20
 Operator : AJ/MA
 Sample : N3422-05MSD
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 22 04:28:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.836	302329	26.954 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.697	126784	7.526 ng/ml
2) t 2,2,4-Trimethylpentane	7.401	108020	6.152 ng/ml
3) t n-Heptane	7.764	78725	4.494 ng/ml
4) t Benzene	7.886	114101	5.595 ng/ml
6) t Toluene	10.622	270729	13.982 ng/ml
7) t Ethylbenzene	13.029	834374	46.074 ng/ml
8) t m-Xylene	13.176	123918	6.952 ng/ml
9) t O-Xylene	13.921	264505	15.222 ng/ml
10) t 1,2,4-Trimethylbenzene	16.221	752951	43.831 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
Data File : FB027480.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2022 20:20
Operator : AJ/MA
Sample : N3422-05MSD
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 22 04:28:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

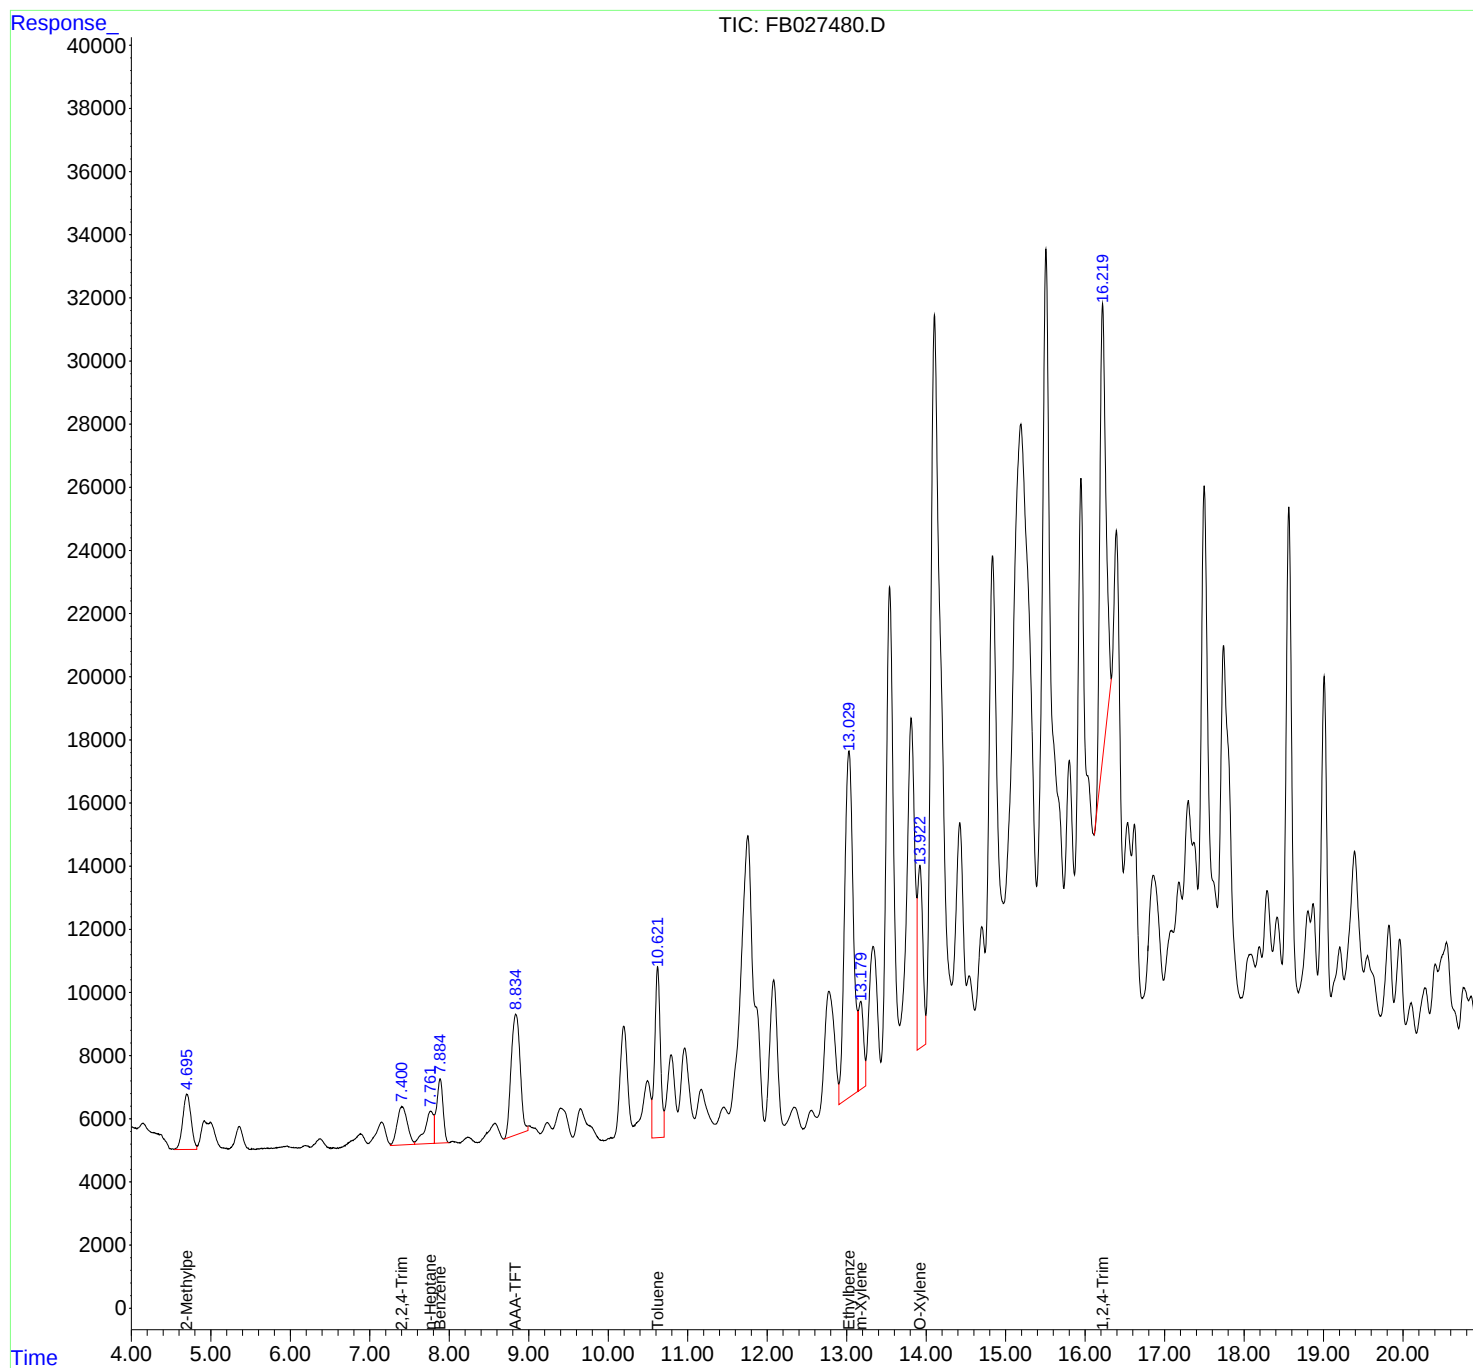


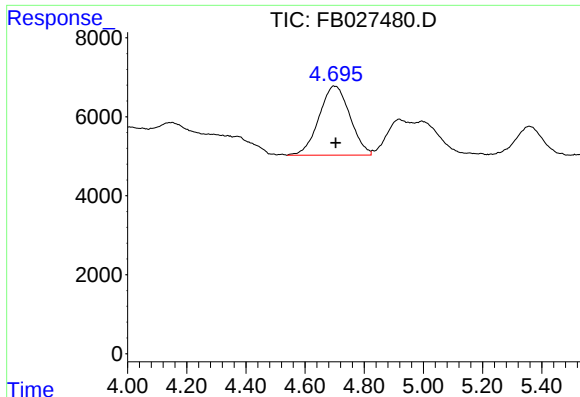

#1 2-Methylpentane


R.T.: 4.697 min
Delta R.T.: -0.007 min
Response: 126784
Conc: 7.53 ng/ml

Instrument :
FID_B
ClientSampleId :

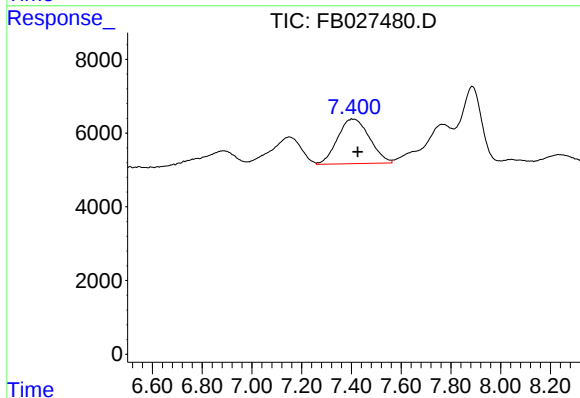


#2 2,2,4-Trimethylpentane

R.T.: 7.401 min
Delta R.T.: -0.025 min
Response: 108020
Conc: 6.15 ng/ml

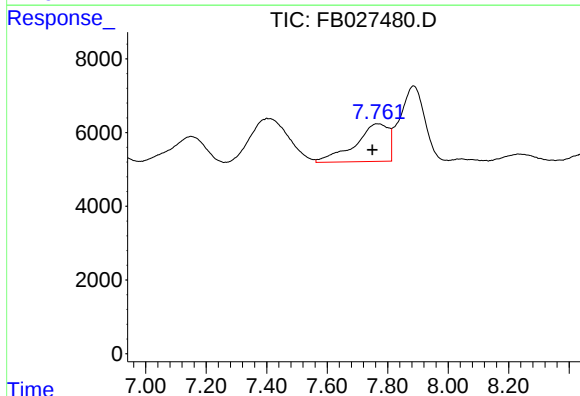


#3 n-Heptane

R.T.: 7.764 min
Delta R.T.: 0.014 min
Response: 78725
Conc: 4.49 ng/ml

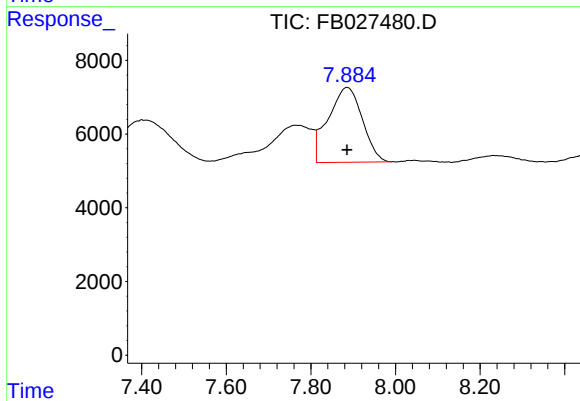

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 114101
Conc: 5.60 ng/ml

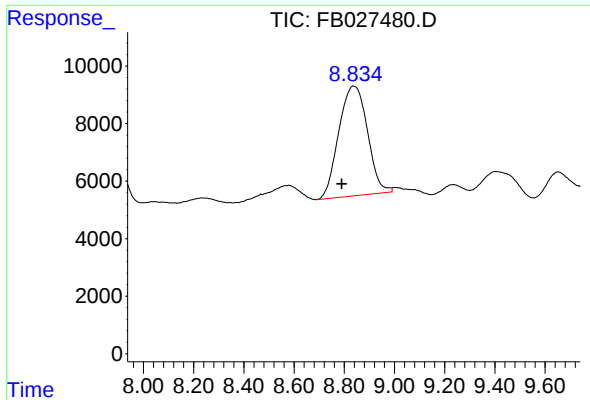

#5 AAA-TFT


R.T.: 8.836 min
Delta R.T.: 0.045 min
Response: 302329
Conc: 26.95 ng/ml

Instrument :
FID_B
ClientSampleId :

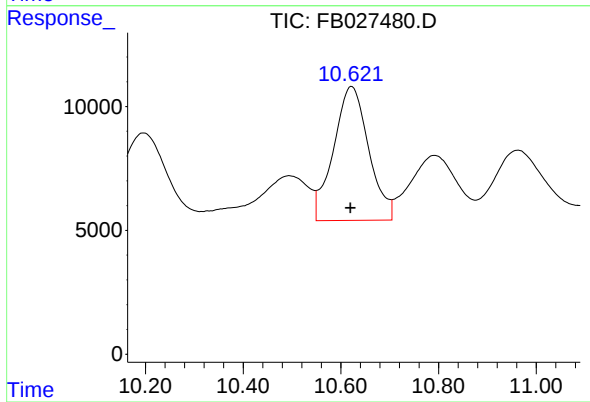


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.003 min
Response: 270729
Conc: 13.98 ng/ml

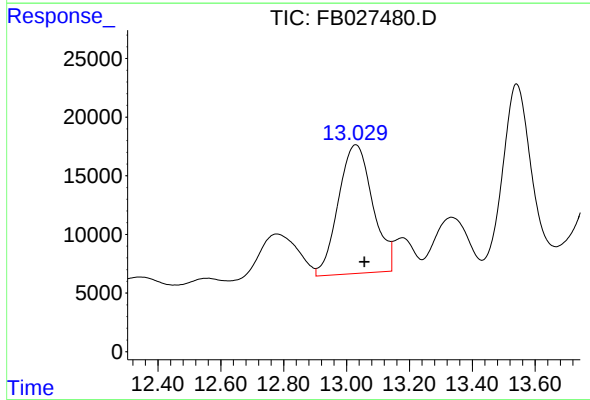


#7 Ethylbenzene

R.T.: 13.029 min
Delta R.T.: -0.027 min
Response: 834374
Conc: 46.07 ng/ml

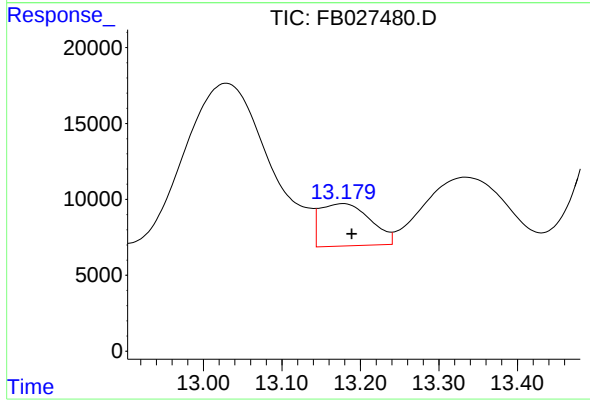

#8 m-Xylene


R.T.: 13.176 min
Delta R.T.: -0.013 min
Response: 123918
Conc: 6.95 ng/ml

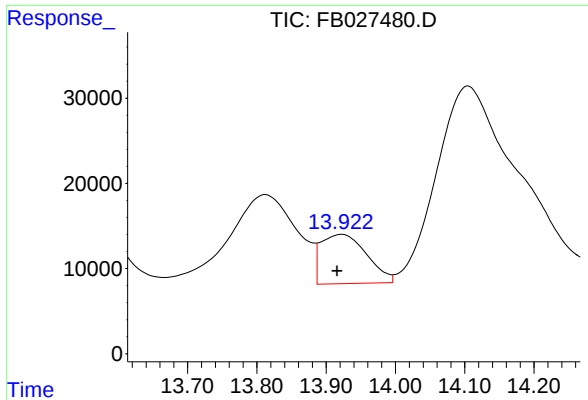

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.005 min
Response: 264505
Conc: 15.22 ng/ml

Instrument :
FID_B
ClientSampleId :

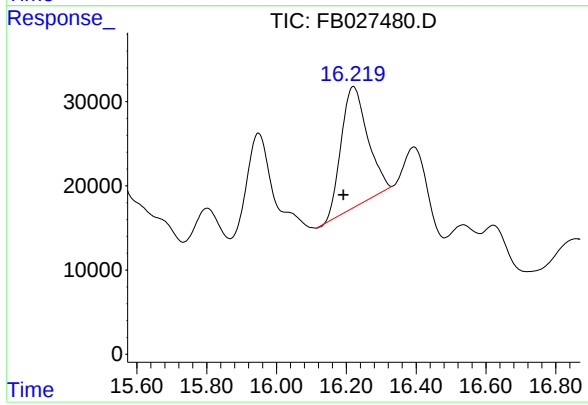

#10 1,2,4-Trimethylbenzene

R.T.: 16.221 min
Delta R.T.: 0.030 min
Response: 752951
Conc: 43.83 ng/ml