

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
 Data File : FB027486.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2022 00:37
 Operator : AJ/MA
 Sample : N3422-05MSD 50X
 Misc : 5.06G/5.00 ML MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 22 04:29:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	241550	21.535 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	407242	24.173 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	416436	23.717 ng/ml
3) t n-Heptane	7.749	136511	7.792 ng/ml
4) t Benzene	7.886	177017	8.681 ng/ml
6) t Toluene	10.619	480871	24.836 ng/ml
7) t Ethylbenzene	13.054	209984	11.595 ng/ml
8) t m-Xylene	13.189	289444	16.237 ng/ml
9) t O-Xylene	13.916	322099	18.537 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	337274	19.634 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
Data File : FB027486.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2022 00:37
Operator : AJ/MA
Sample : N3422-05MSD 50X
Misc : 5.06G/5.00 ML MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 22 04:29:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

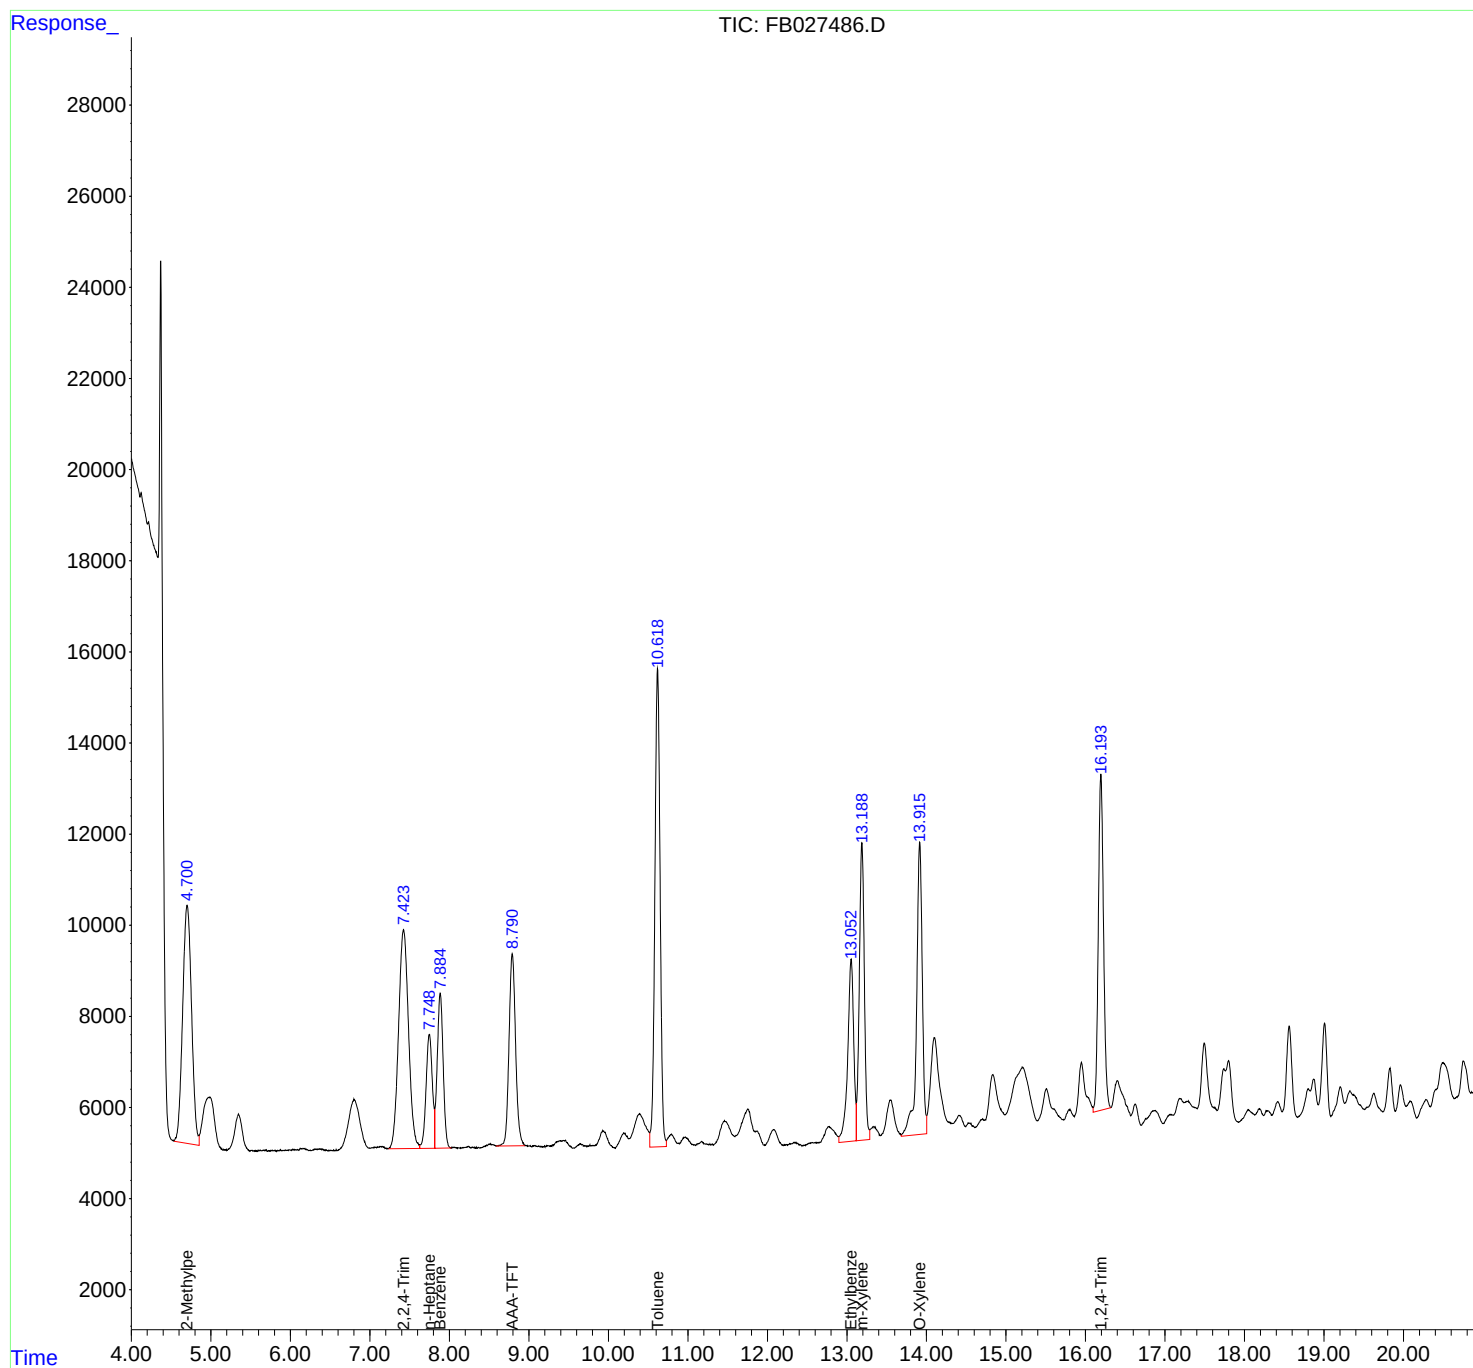


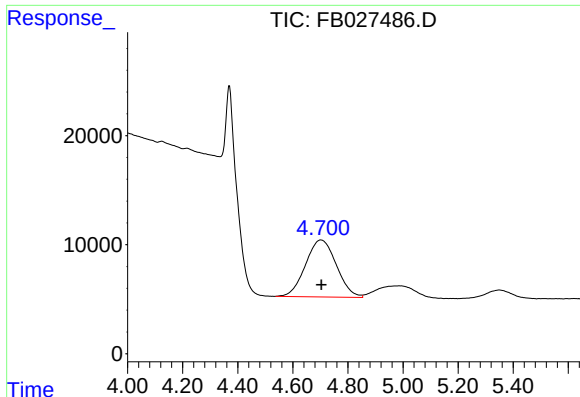

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.002 min
Response: 407242
Conc: 24.17 ng/ml

Instrument :
FID_B
ClientSampleId :

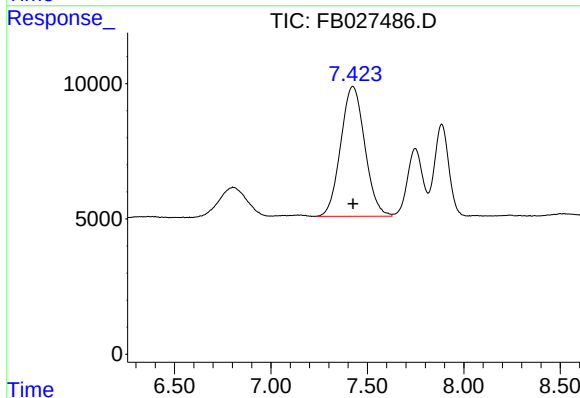


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.001 min
Response: 416436
Conc: 23.72 ng/ml

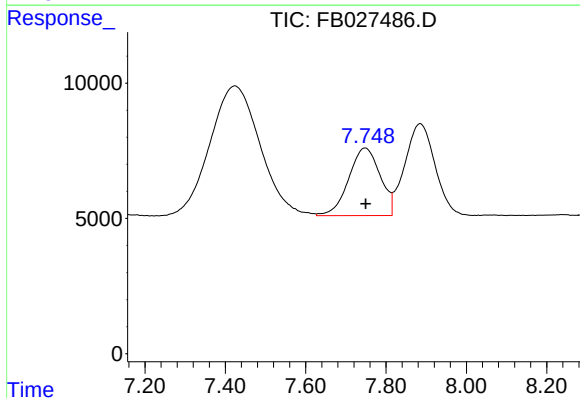


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 136511
Conc: 7.79 ng/ml

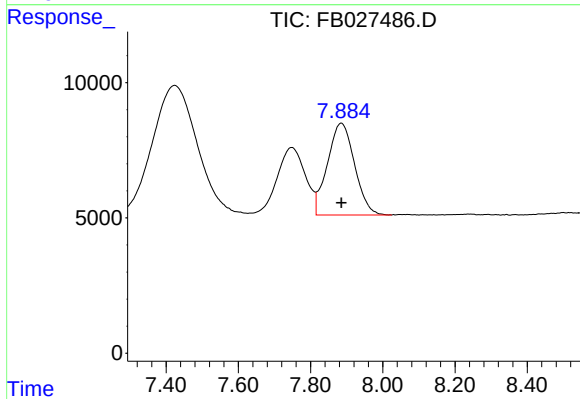

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 177017
Conc: 8.68 ng/ml

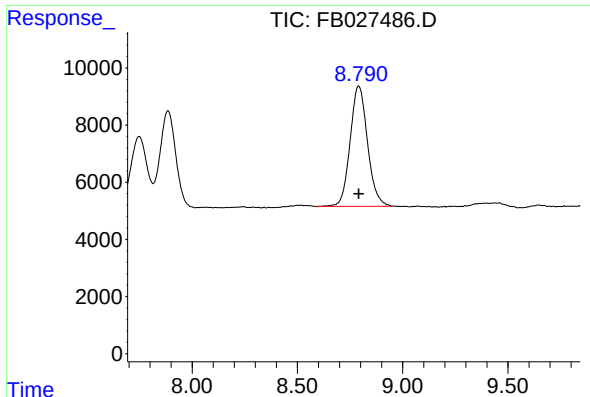

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 241550
Conc: 21.53 ng/ml

Instrument :
FID_B
ClientSampleId :

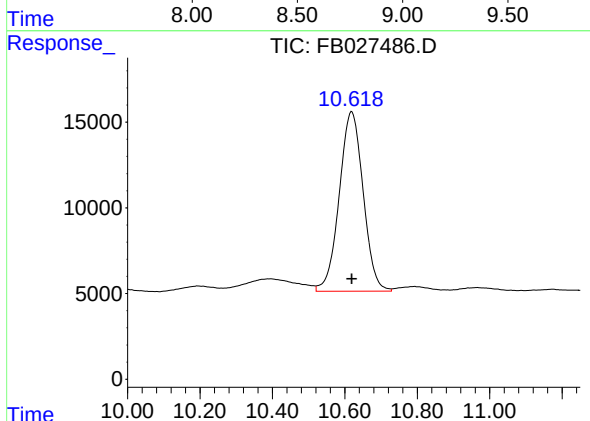


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 480871
Conc: 24.84 ng/ml

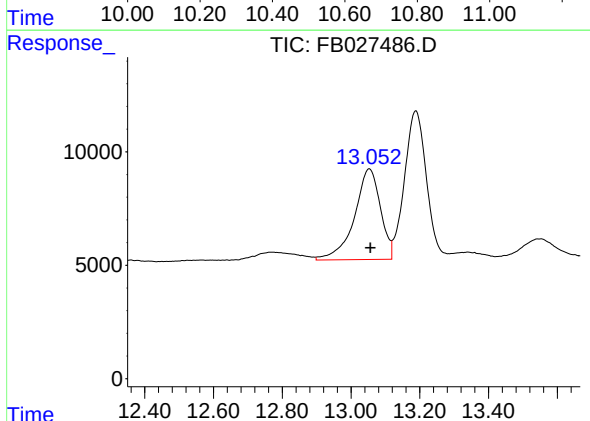


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.003 min
Response: 209984
Conc: 11.60 ng/ml

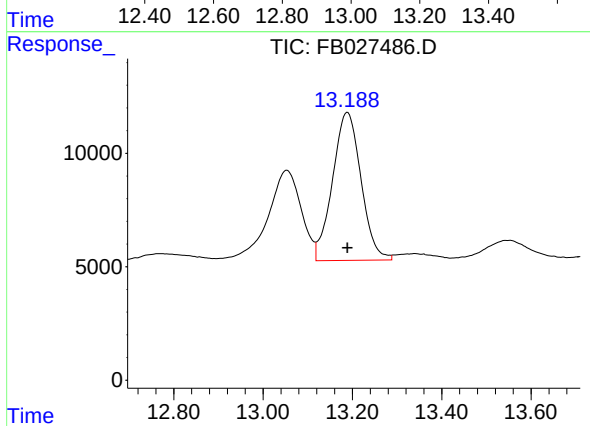

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 289444
Conc: 16.24 ng/ml

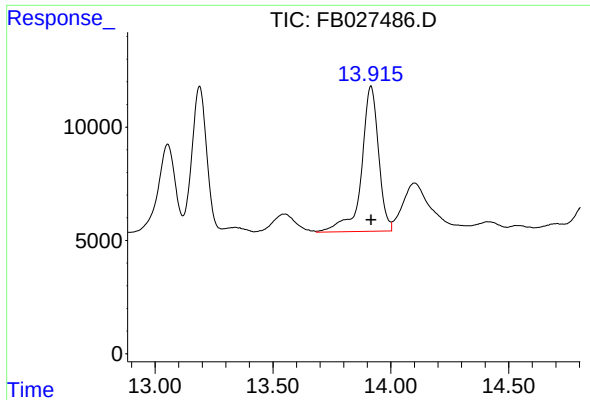

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 322099
Conc: 18.54 ng/ml

Instrument :
FID_B
ClientSampleId :

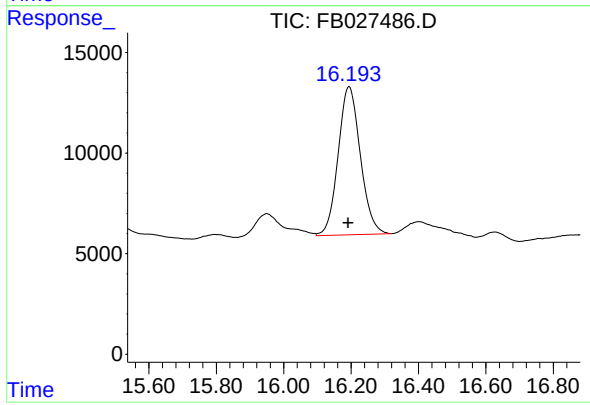

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.003 min
Response: 337274
Conc: 19.63 ng/ml