

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
 Data File : FB027472.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2022 15:27
 Operator : AJ/MA
 Sample : BSF0621S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0621S1

Integration File: SAMPLE.e
 Quant Time: Jun 22 04:27:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	244876	21.831 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	459787	27.291 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	492135	28.029 ng/ml
3) t n-Heptane	7.751	159263	9.091 ng/ml
4) t Benzene	7.888	191248	9.378 ng/ml
6) t Toluene	10.621	549547	28.383 ng/ml
7) t Ethylbenzene	13.058	169699	9.371 ng/ml
8) t m-Xylene	13.190	338032	18.963 ng/ml
9) t O-Xylene	13.917	329995	18.991 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	331840	19.317 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
Data File : FB027472.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2022 15:27
Operator : AJ/MA
Sample : BSF0621S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0621S1

Integration File: SAMPLE.e
Quant Time: Jun 22 04:27:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

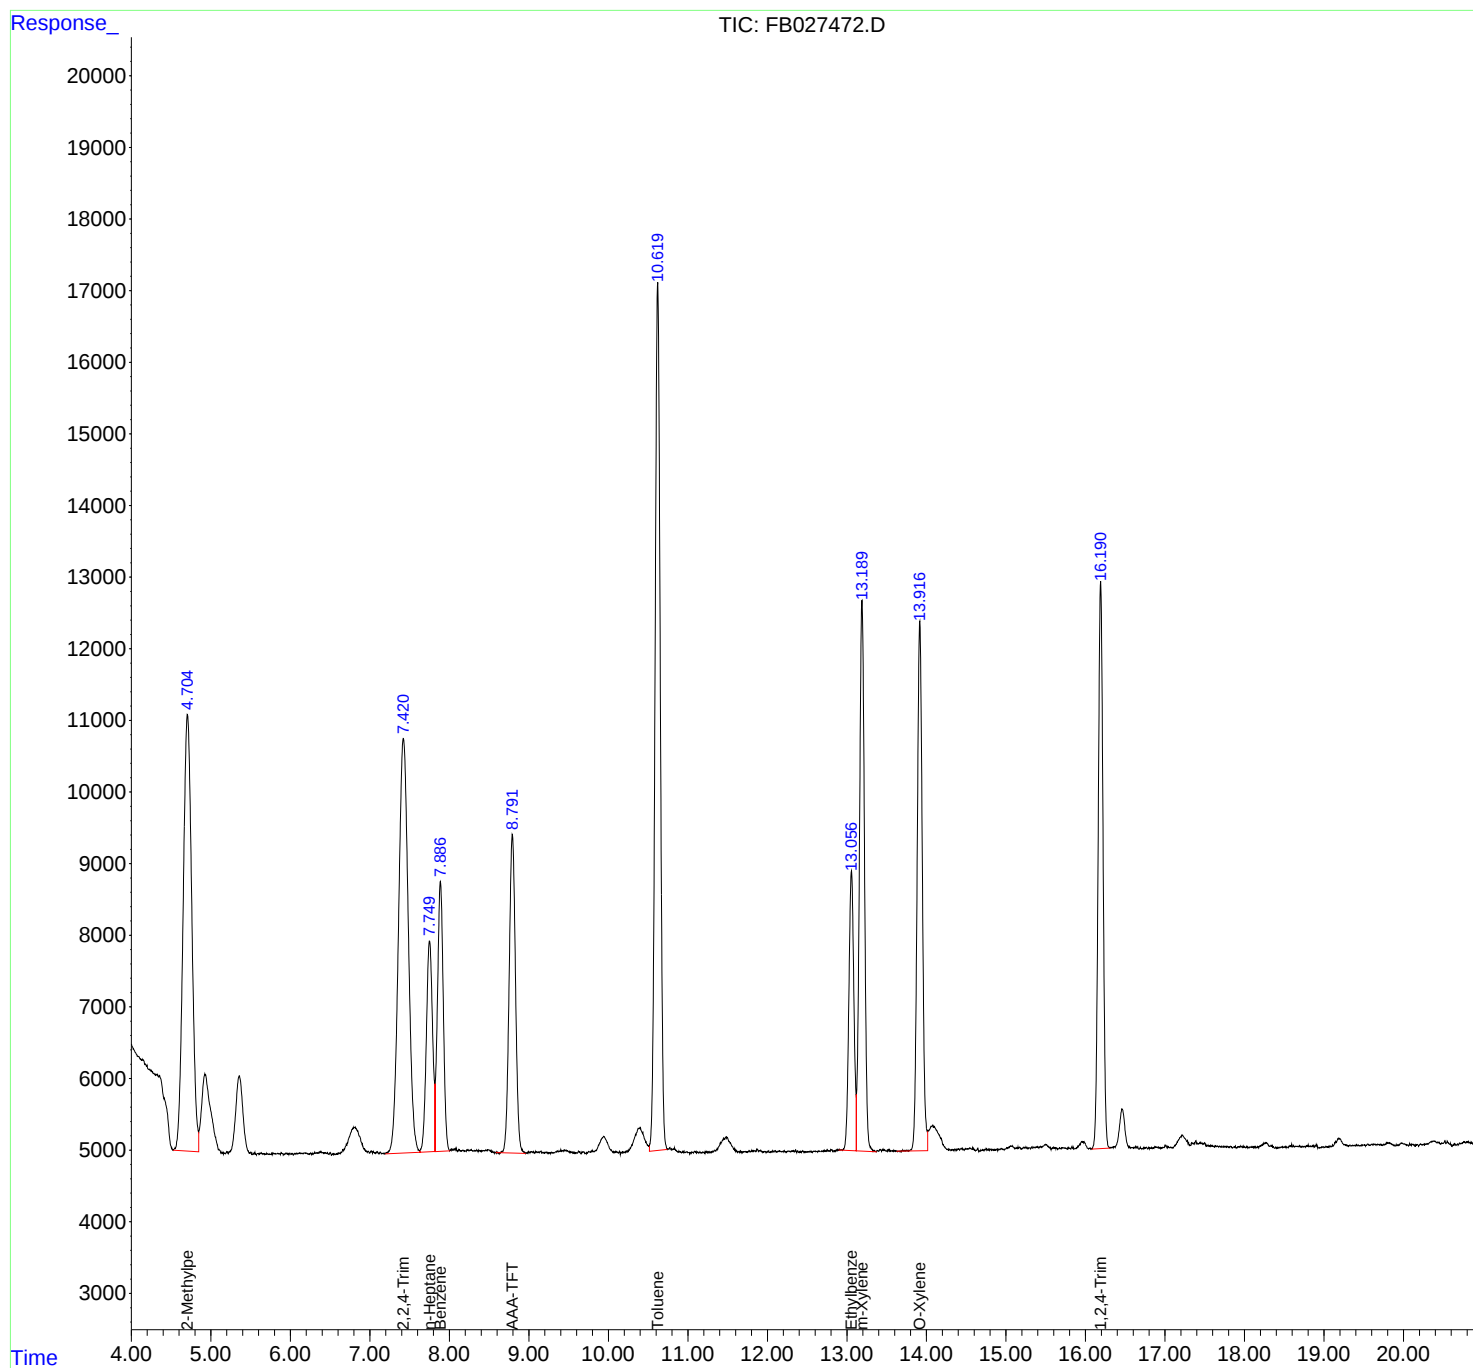


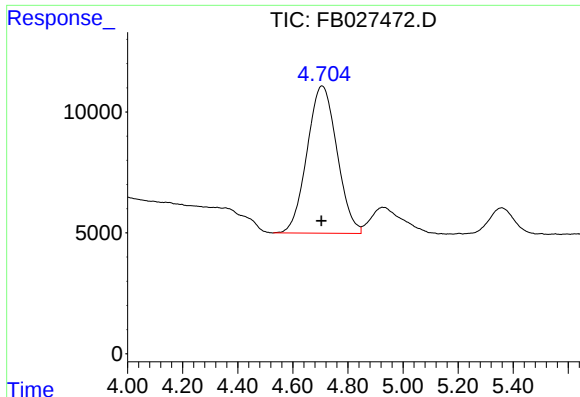

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.002 min
Response: 459787
Conc: 27.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S1

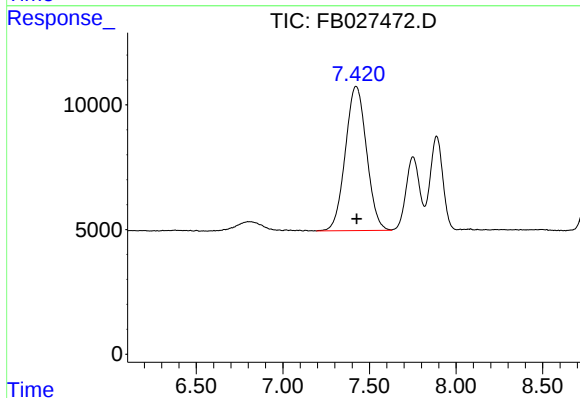


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: -0.004 min
Response: 492135
Conc: 28.03 ng/ml

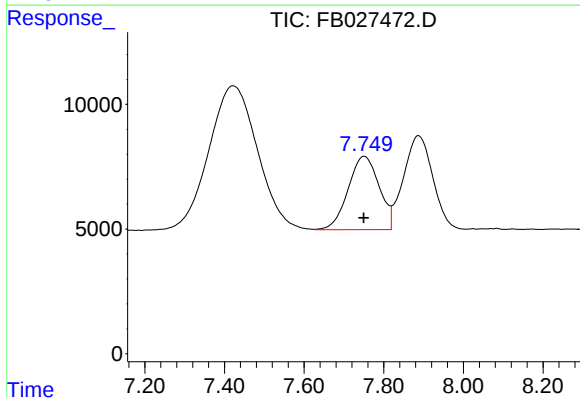


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.002 min
Response: 159263
Conc: 9.09 ng/ml

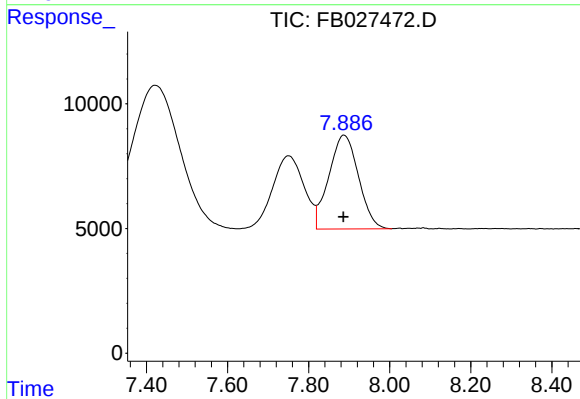

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 191248
Conc: 9.38 ng/ml

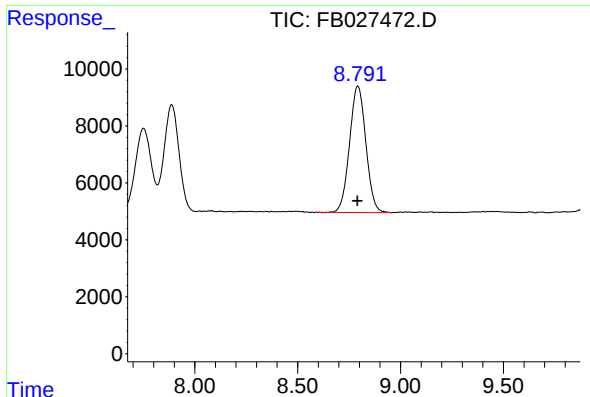

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 244876
Conc: 21.83 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S1

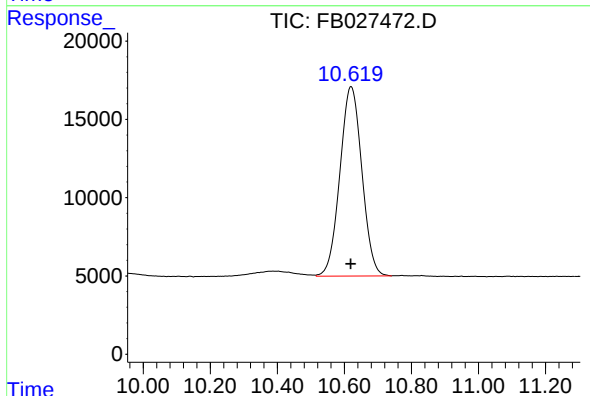


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.001 min
Response: 549547
Conc: 28.38 ng/ml

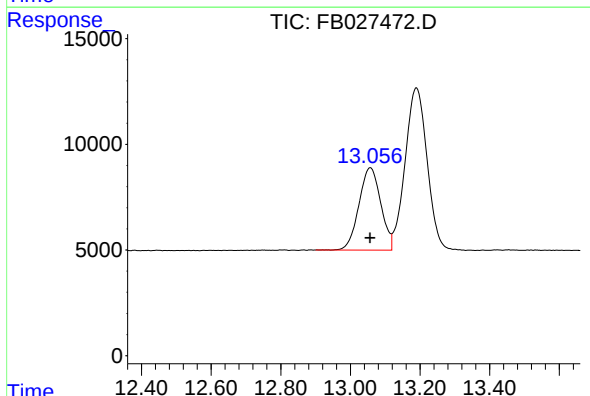


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.001 min
Response: 169699
Conc: 9.37 ng/ml

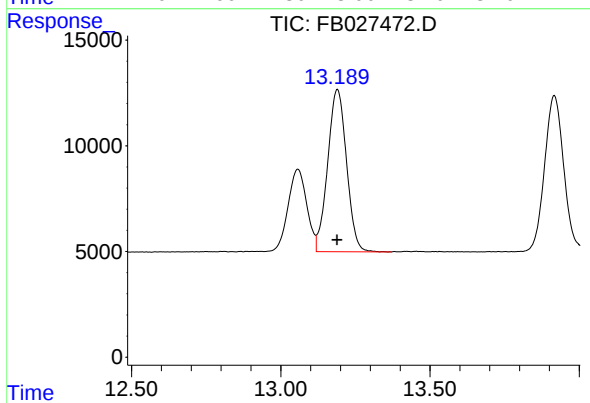

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 338032
Conc: 18.96 ng/ml

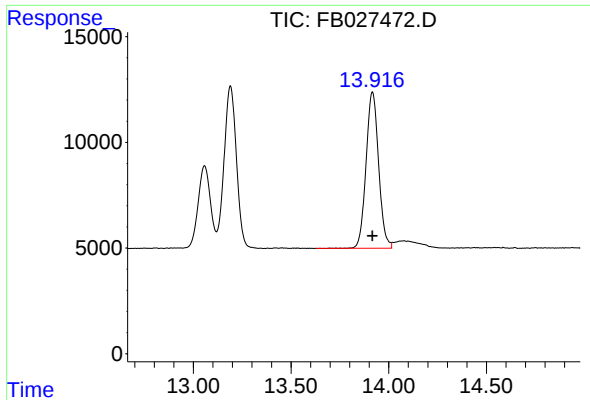

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 329995
Conc: 18.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S1

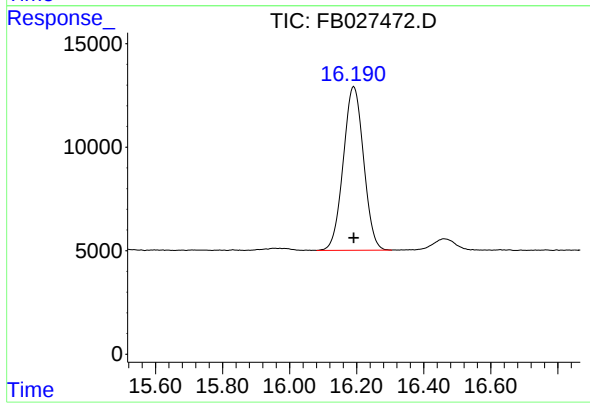

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 331840
Conc: 19.32 ng/ml