

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
 Data File : FB027481.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2022 20:57
 Operator : AJ/MA
 Sample : BSF0621S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0621S2

Integration File: SAMPLE.e
 Quant Time: Jun 22 04:28:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	235233	20.972 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	490058	29.088 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	532022	30.300 ng/ml
3) t n-Heptane	7.752	166817	9.522 ng/ml
4) t Benzene	7.888	211427	10.368 ng/ml
6) t Toluene	10.621	590535	30.500 ng/ml
7) t Ethylbenzene	13.058	193533	10.687 ng/ml
8) t m-Xylene	13.191	364868	20.468 ng/ml
9) t O-Xylene	13.918	357585	20.579 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	356862	20.774 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
Data File : FB027481.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2022 20:57
Operator : AJ/MA
Sample : BSF0621S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0621S2

Integration File: SAMPLE.e
Quant Time: Jun 22 04:28:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

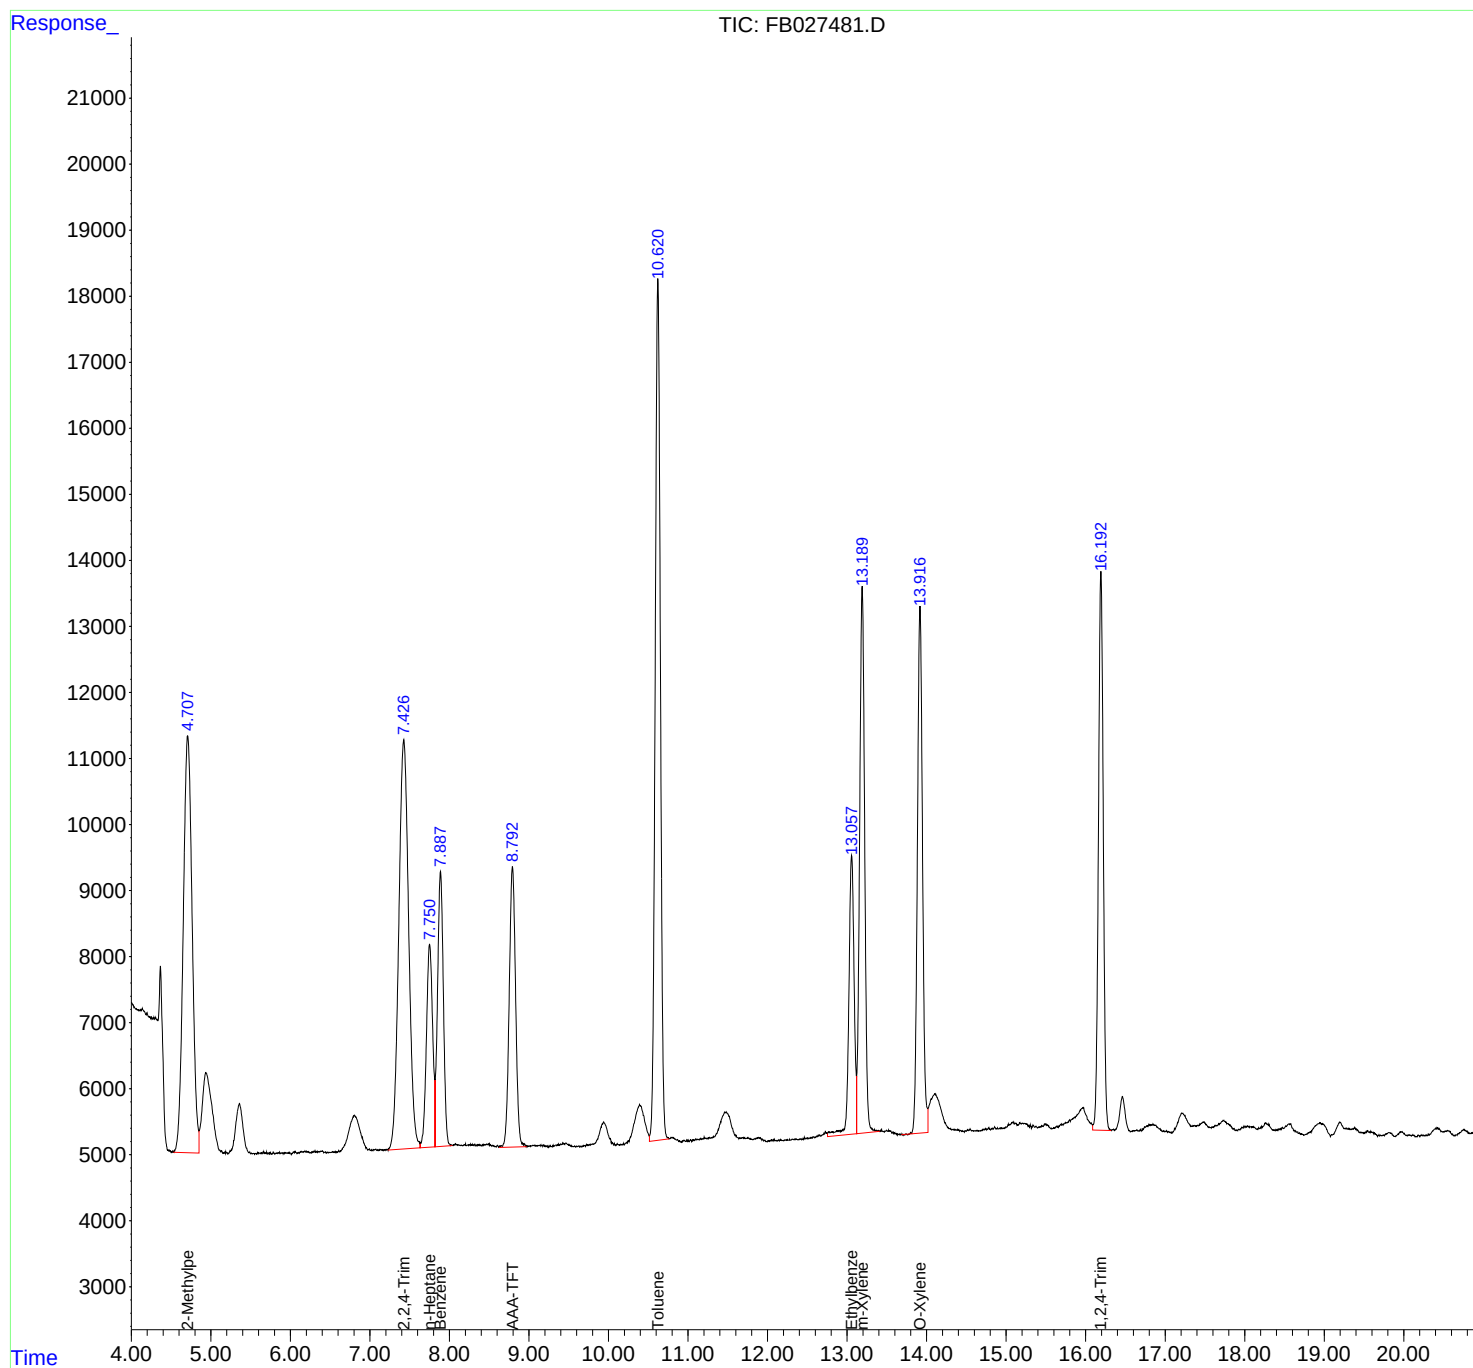


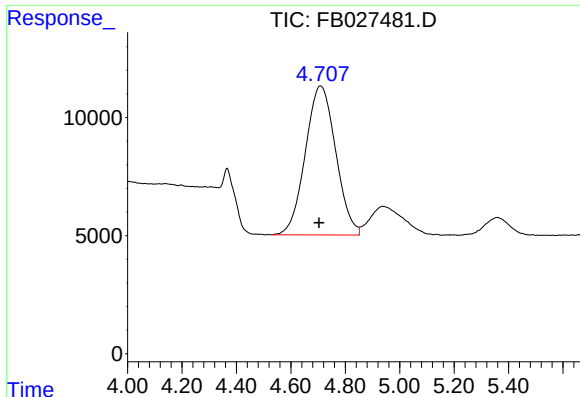

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.005 min
Response: 490058
Conc: 29.09 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S2

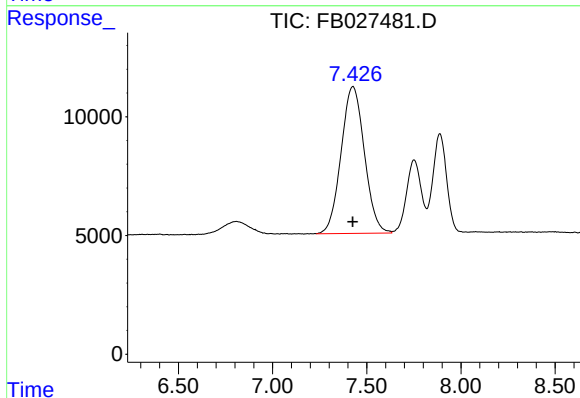


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.001 min
Response: 532022
Conc: 30.30 ng/ml

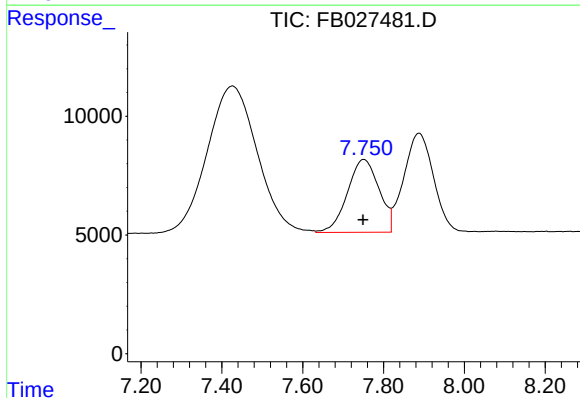


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.002 min
Response: 166817
Conc: 9.52 ng/ml

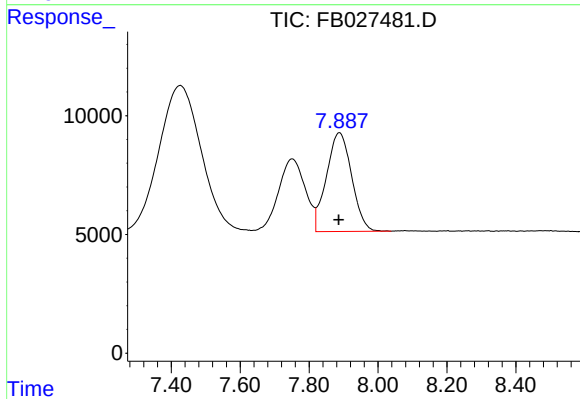

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.003 min
Response: 211427
Conc: 10.37 ng/ml

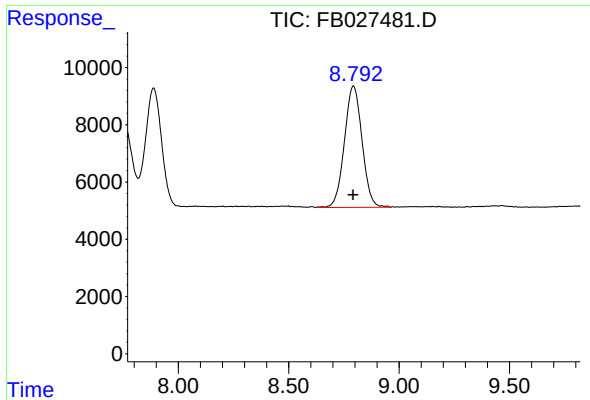

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.003 min
Response: 235233
Conc: 20.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S2

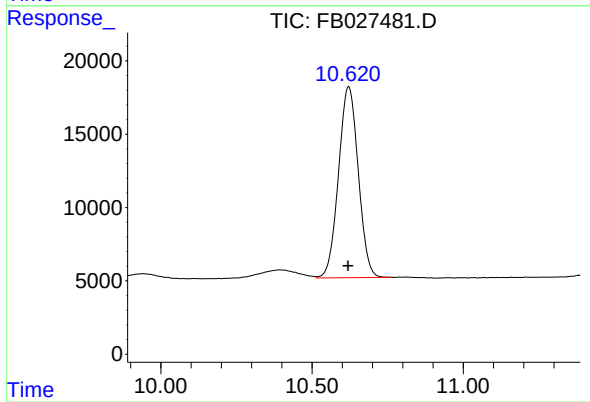


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 590535
Conc: 30.50 ng/ml

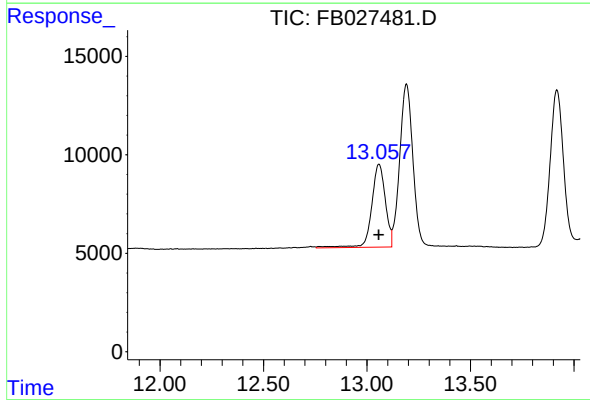


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 193533
Conc: 10.69 ng/ml

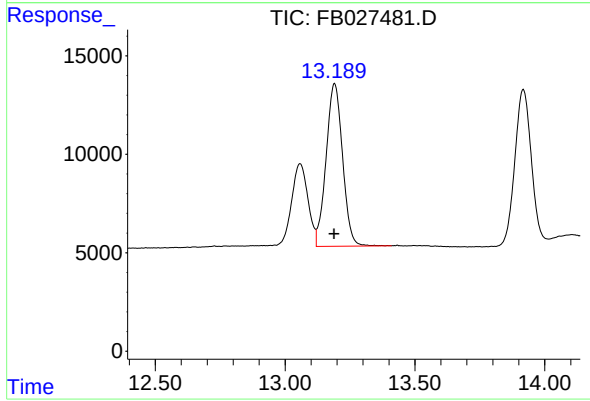

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 364868
Conc: 20.47 ng/ml

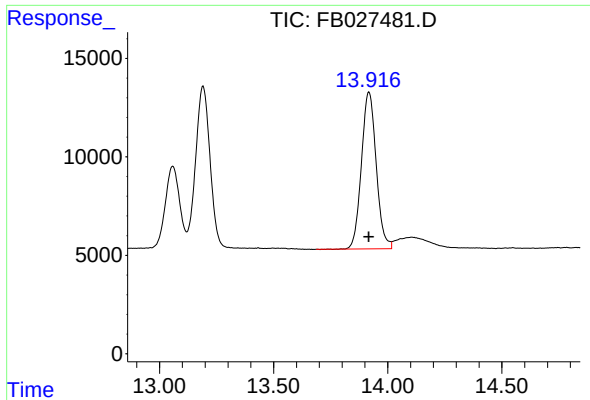

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 357585
Conc: 20.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S2

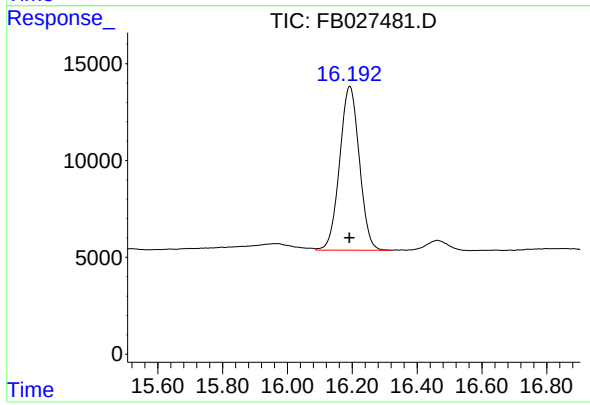

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.001 min
Response: 356862
Conc: 20.77 ng/ml