

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
 Data File : FB027487.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2022 1:13
 Operator : AJ/MA
 Sample : BSF0621S3
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0621S3

Integration File: SAMPLE.e
 Quant Time: Jun 22 04:29:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	204726	18.252 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	466783	27.707 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	523121	29.793 ng/ml
3) t n-Heptane	7.749	155681	8.887 ng/ml
4) t Benzene	7.887	195047	9.565 ng/ml
6) t Toluene	10.620	557564	28.797 ng/ml
7) t Ethylbenzene	13.056	174064	9.612 ng/ml
8) t m-Xylene	13.189	348761	19.565 ng/ml
9) t O-Xylene	13.915	342907	19.735 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	353529	20.580 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062122\
Data File : FB027487.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2022 1:13
Operator : AJ/MA
Sample : BSF0621S3
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0621S3

Integration File: SAMPLE.e
Quant Time: Jun 22 04:29:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

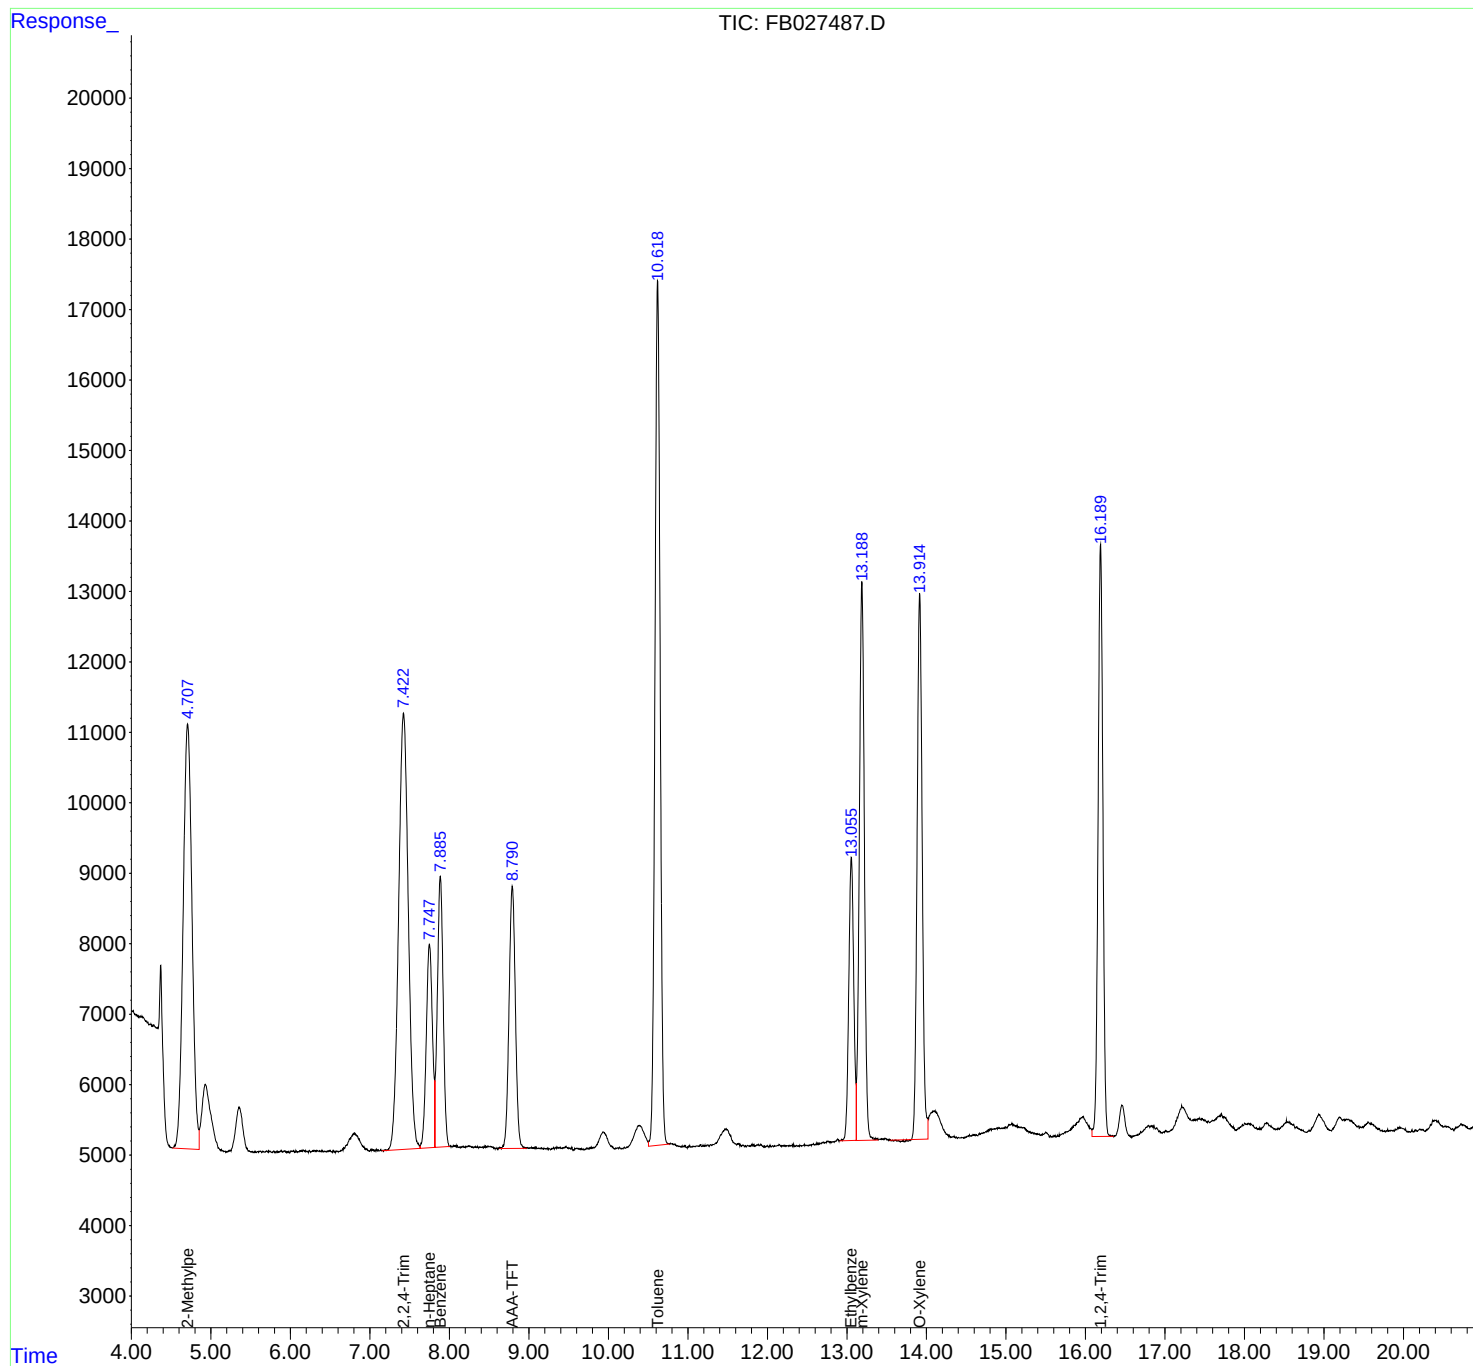


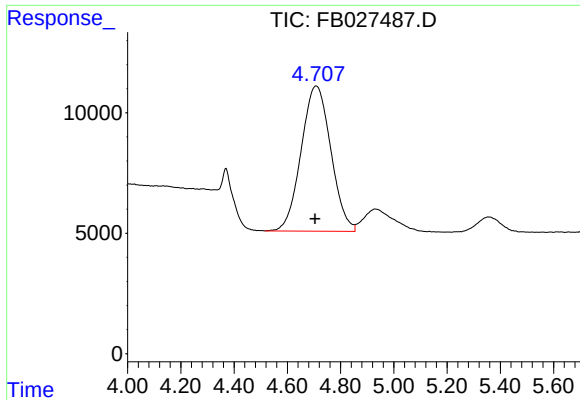

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.005 min
Response: 466783
Conc: 27.71 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S3

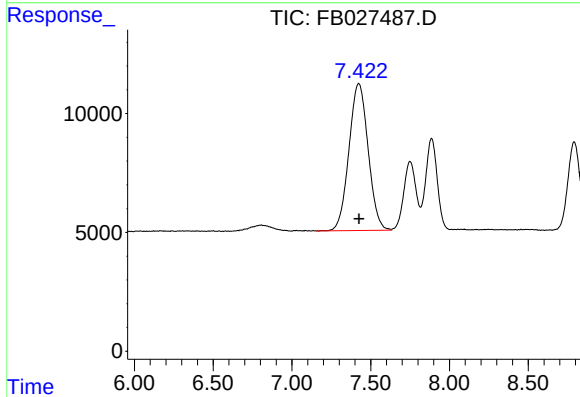


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.002 min
Response: 523121
Conc: 29.79 ng/ml

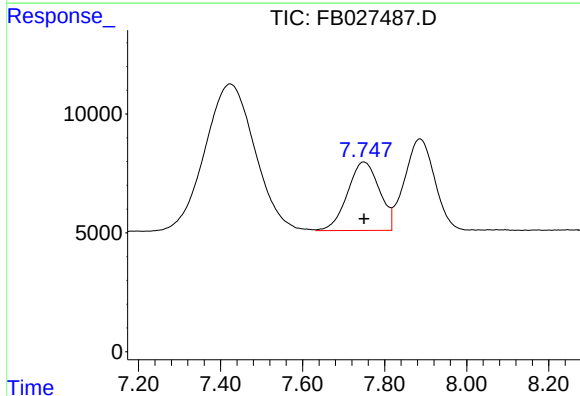


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 155681
Conc: 8.89 ng/ml

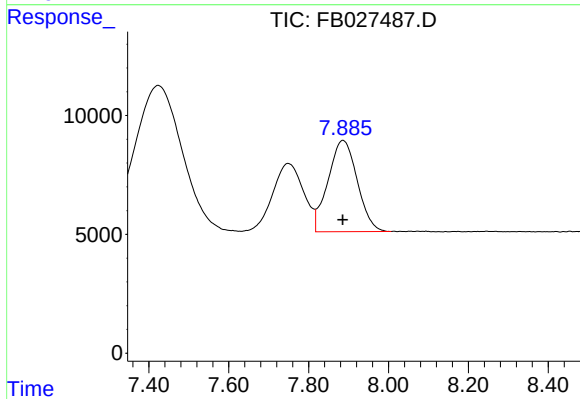

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 195047
Conc: 9.56 ng/ml

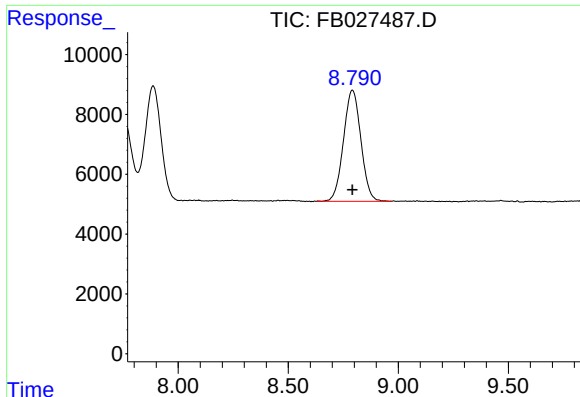

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 204726
Conc: 18.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S3

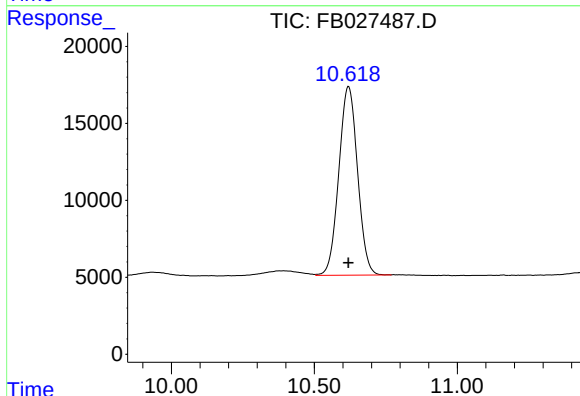


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 557564
Conc: 28.80 ng/ml

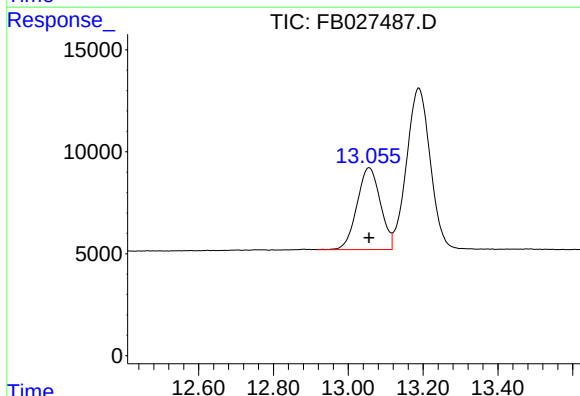


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 174064
Conc: 9.61 ng/ml

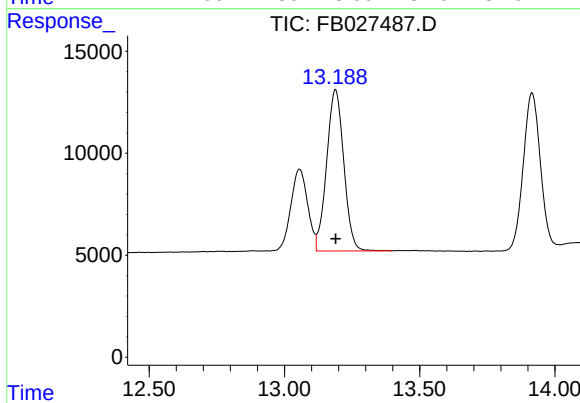

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 348761
Conc: 19.56 ng/ml

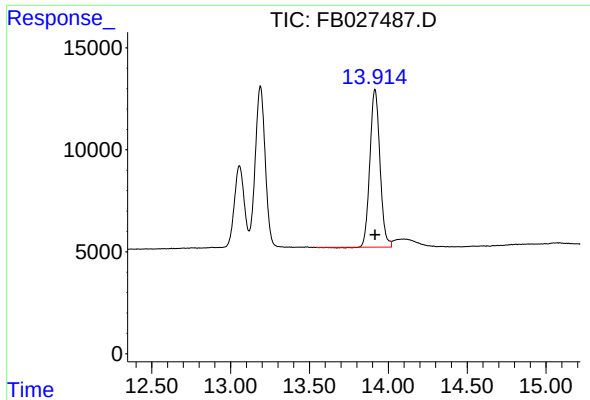

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.000 min
Response: 342907
Conc: 19.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S3

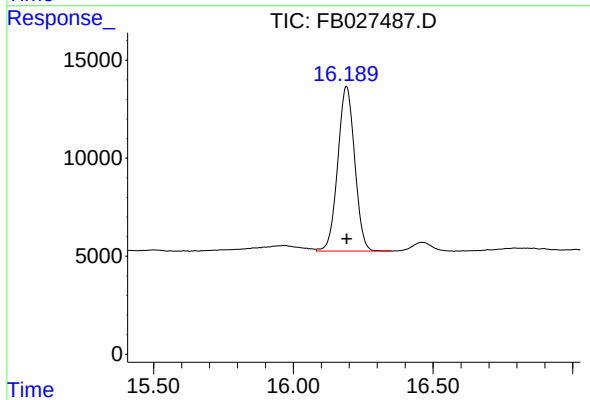

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.000 min
Response: 353529
Conc: 20.58 ng/ml