

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
 Data File : FB030098.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2023 9:54
 Operator : YP/AJ
 Sample : 03357-19
 Misc : 8.26G/5.00 ML DI WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 22 23:36:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.786	113659	8.170 ng/ml
Target Compounds				
3) t	n-Heptane	7.786	32155	1.661 ng/ml
6) t	Toluene	10.639	3788	0.175 ng/ml
7) t	Ethylbenzene	13.046	9636	0.477 ng/ml
8) t	m-Xylene	13.167	6621	0.329 ng/ml
9) t	O-Xylene	13.859	5469	0.281 ng/ml
10) t	1,2,4-Trimethylbenzene	16.129	12668	0.676 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030098.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2023 9:54
Operator : YP/AJ
Sample : 03357-19
Misc : 8.26G/5.00 ML DI WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 22 23:36:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

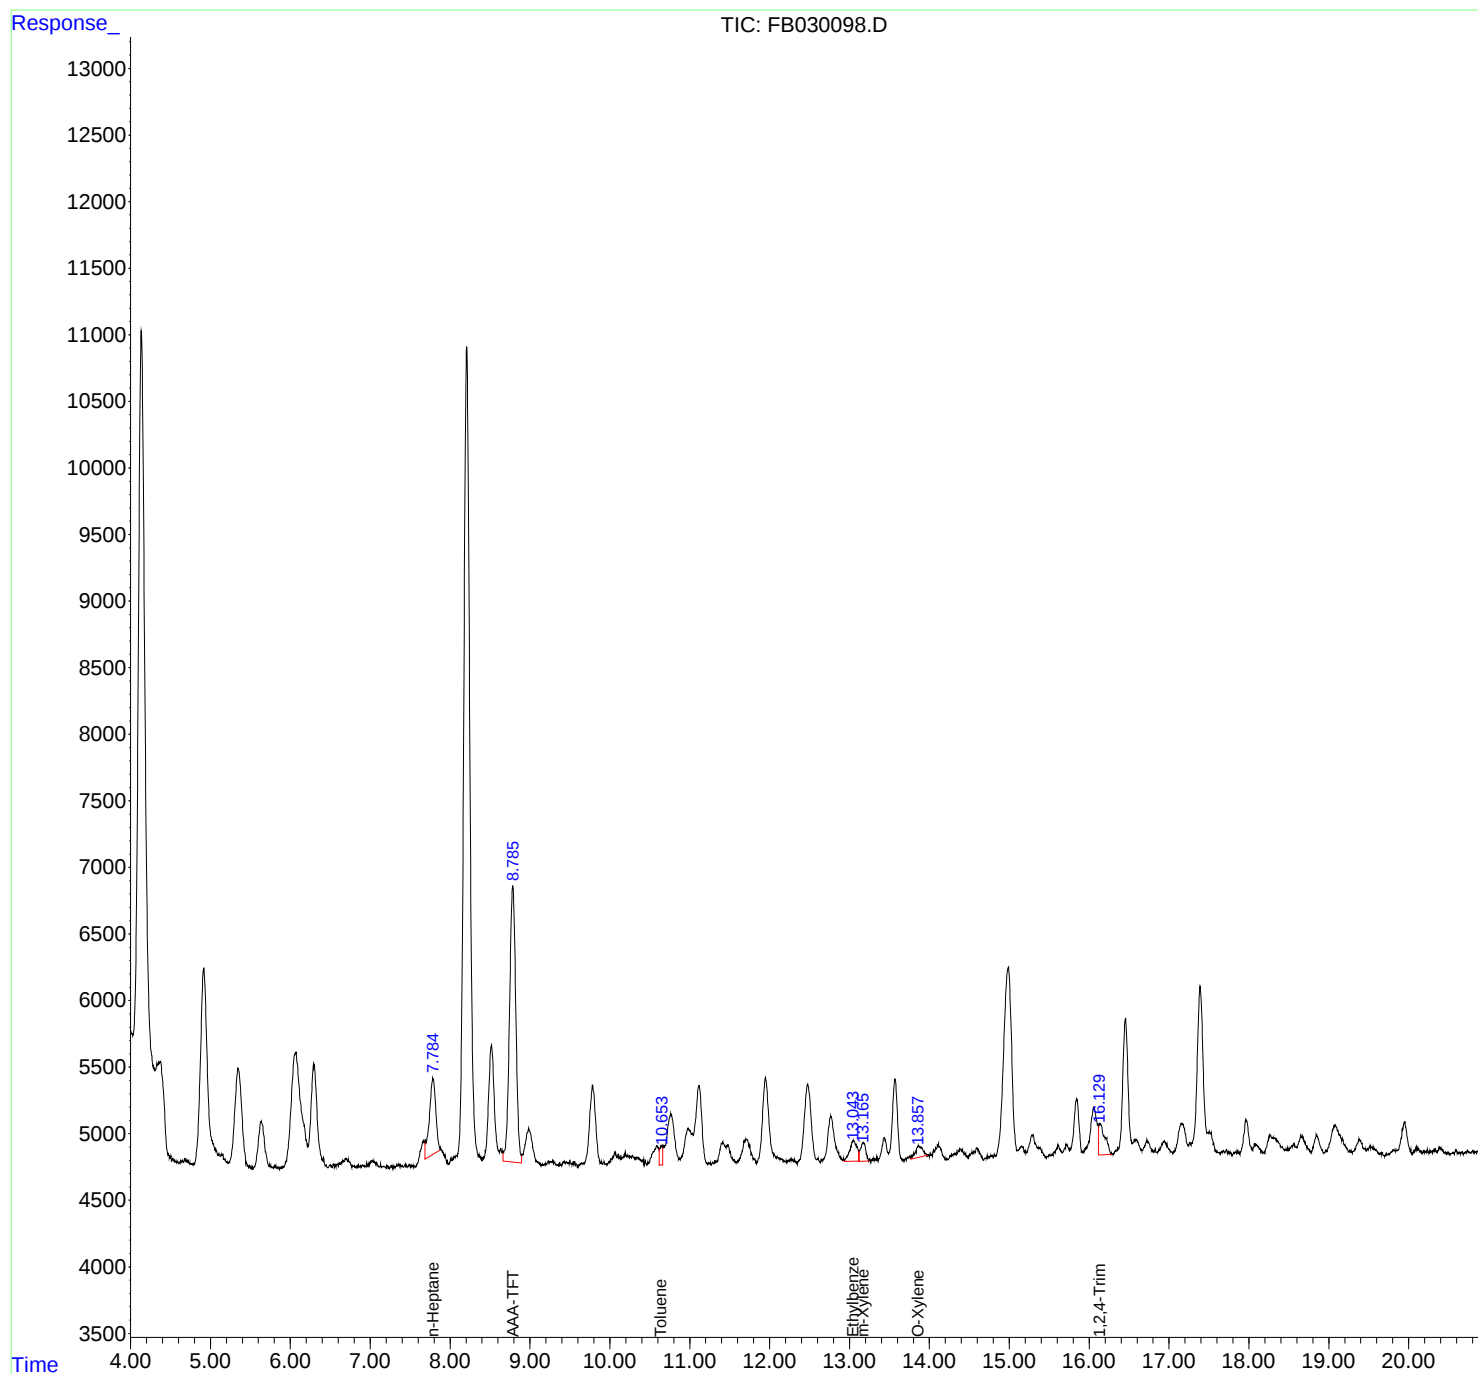


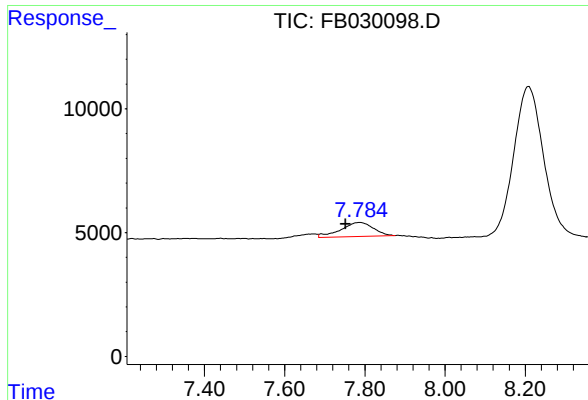

#3 n-Heptane


R.T.: 7.786 min
Delta R.T.: 0.034 min
Response: 32155
Conc: 1.66 ng/ml

Instrument :
FID_B
ClientSampleId :

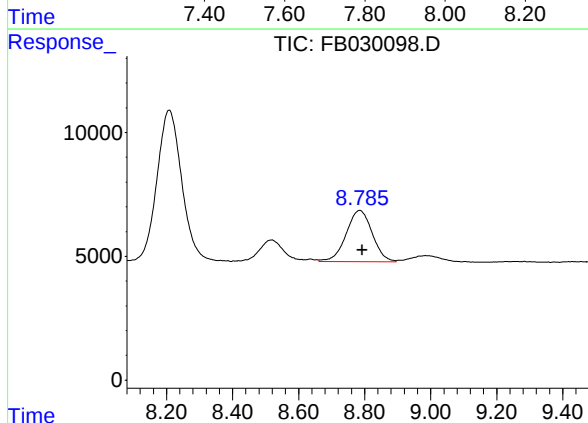


#5 AAA-TFT

R.T.: 8.786 min
Delta R.T.: -0.007 min
Response: 113659
Conc: 8.17 ng/ml

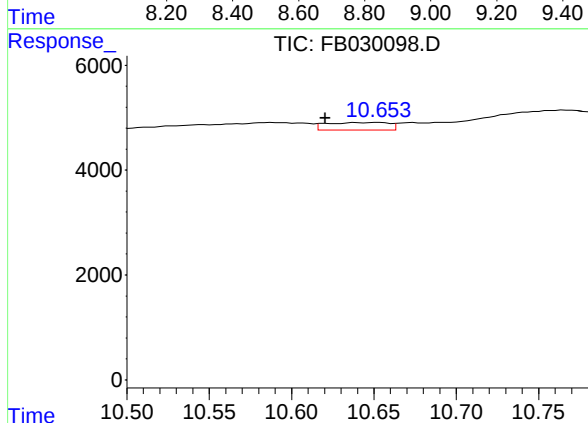


#6 Toluene

R.T.: 10.639 min
Delta R.T.: 0.019 min
Response: 3788
Conc: 0.17 ng/ml

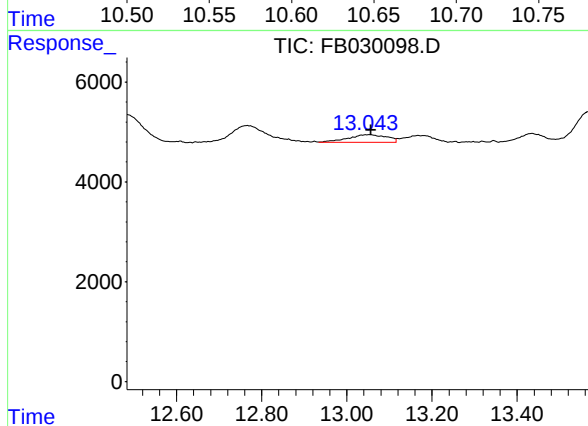

#7 Ethylbenzene


R.T.: 13.046 min
Delta R.T.: -0.011 min
Response: 9636
Conc: 0.48 ng/ml

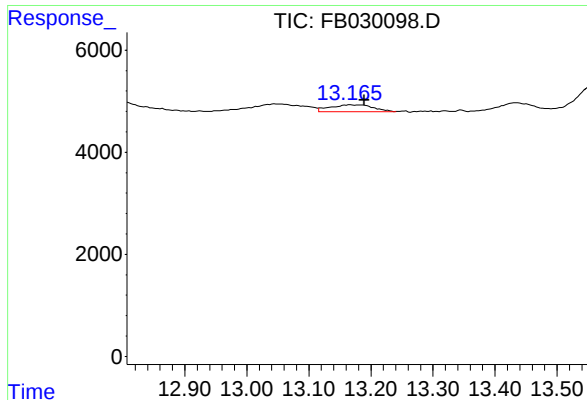

#8 m-Xylene


R.T.: 13.167 min
Delta R.T.: -0.022 min
Response: 6621
Conc: 0.33 ng/ml

Instrument :
FID_B
ClientSampleId :

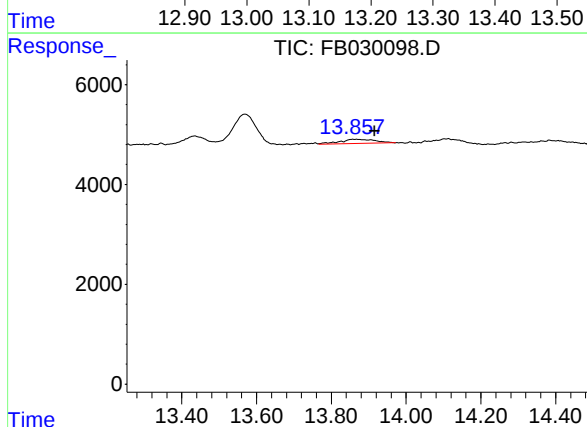

#9 O-Xylene

R.T.: 13.859 min
Delta R.T.: -0.058 min
Response: 5469
Conc: 0.28 ng/ml

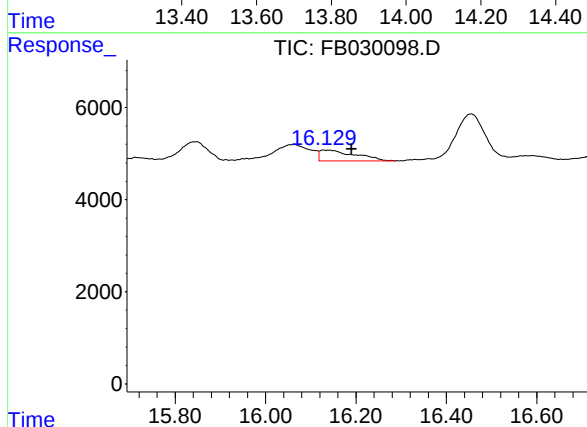

#10 1,2,4-Trimethylbenzene

R.T.: 16.129 min
Delta R.T.: -0.061 min
Response: 12668
Conc: 0.68 ng/ml