

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
 Data File : FB030100.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2023 11:10
 Operator : YP/AJ
 Sample : 03357-04
 Misc : 6.66G/5.00 ML DI WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 22 23:36:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.784	163890	11.780 ng/ml
Target Compounds				
6) t	Toluene	10.611	56087	2.584 ng/ml
7) t	Ethylbenzene	13.045	111894	5.534 ng/ml
8) t	m-Xylene	13.179	283073	14.076 ng/ml
9) t	O-Xylene	13.907	188291	9.661 ng/ml
10) t	1,2,4-Trimethylbenzene	16.183	251632	13.434 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030100.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2023 11:10
Operator : YP/AJ
Sample : 03357-04
Misc : 6.66G/5.00 ML DI WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 22 23:36:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

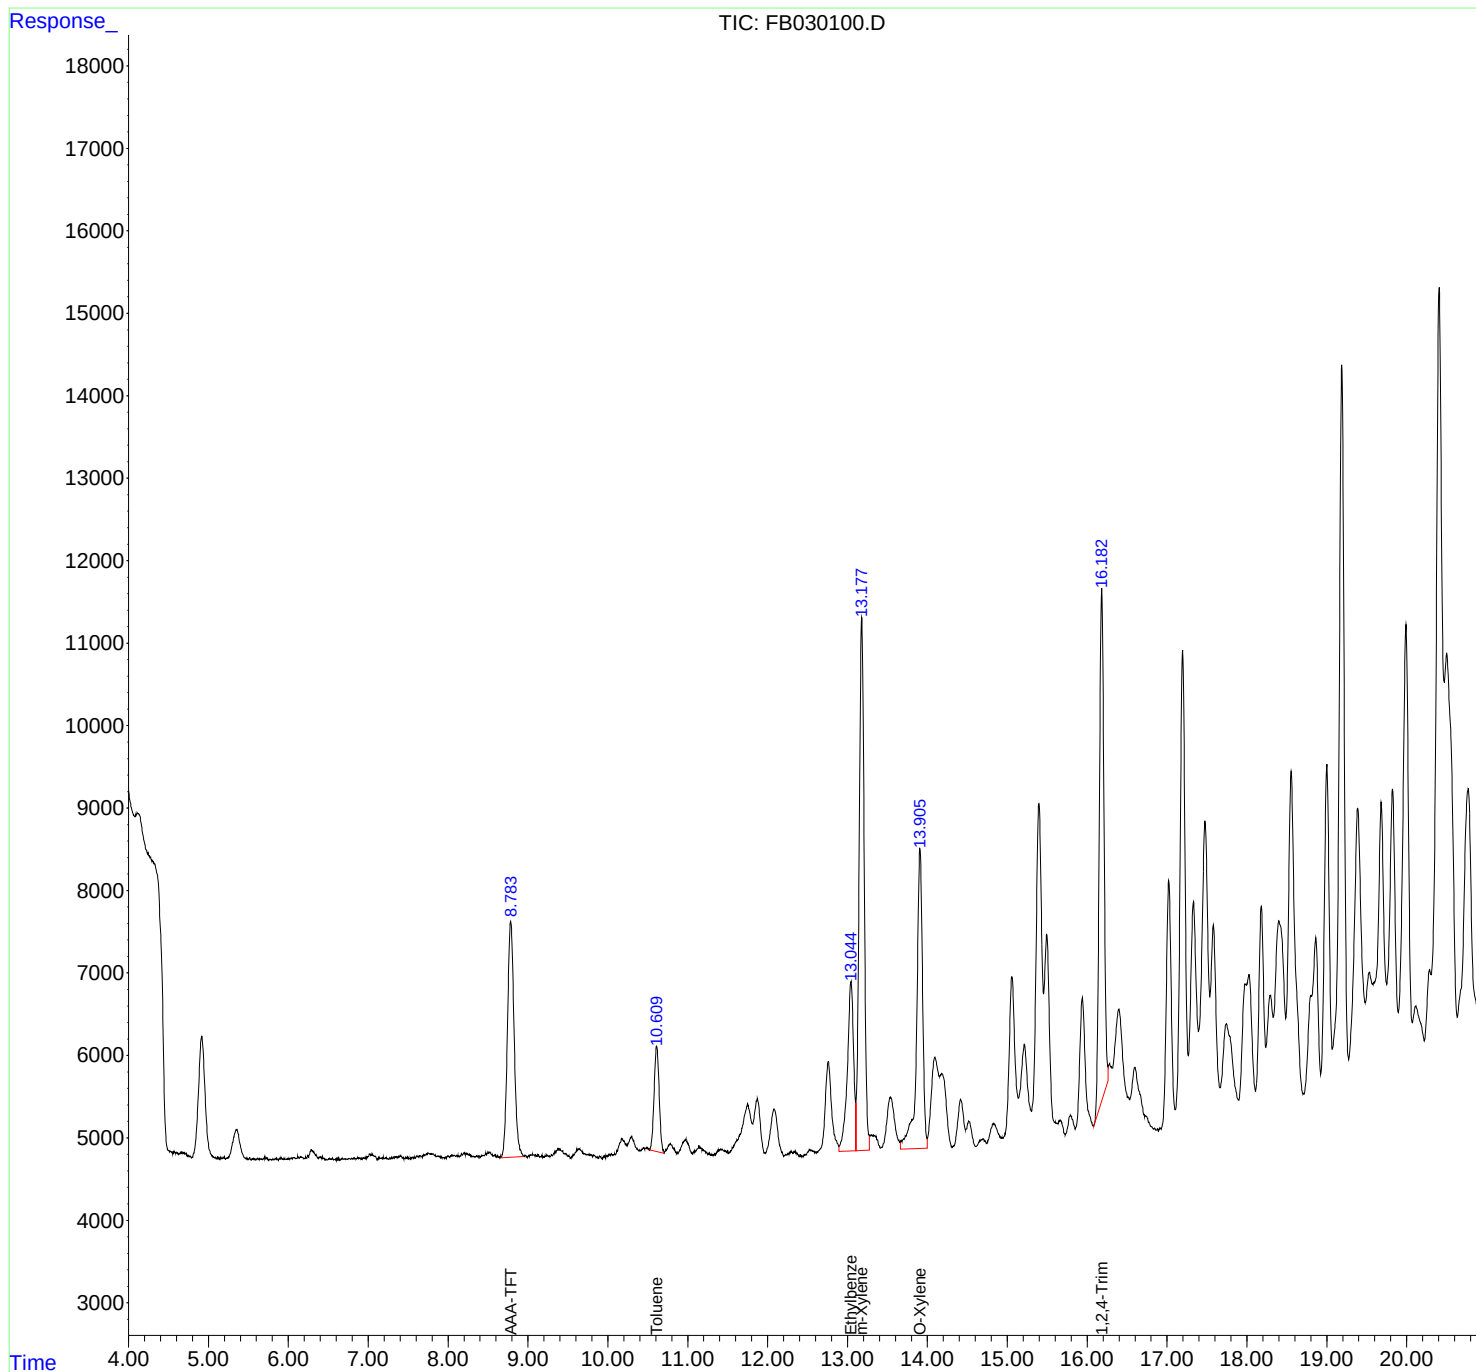


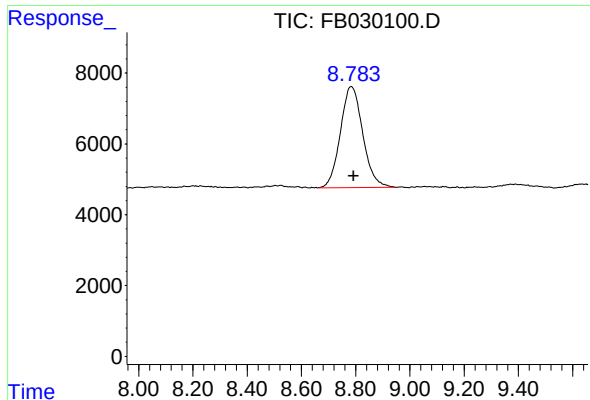

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: -0.008 min
Response: 163890
Conc: 11.78 ng/ml

Instrument :
FID_B
ClientSampleId :

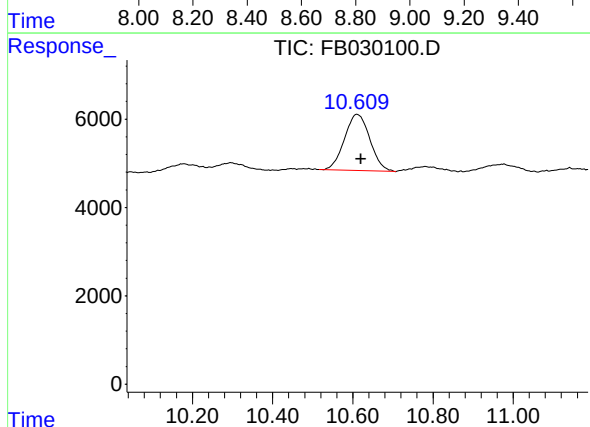


#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.010 min
Response: 56087
Conc: 2.58 ng/ml

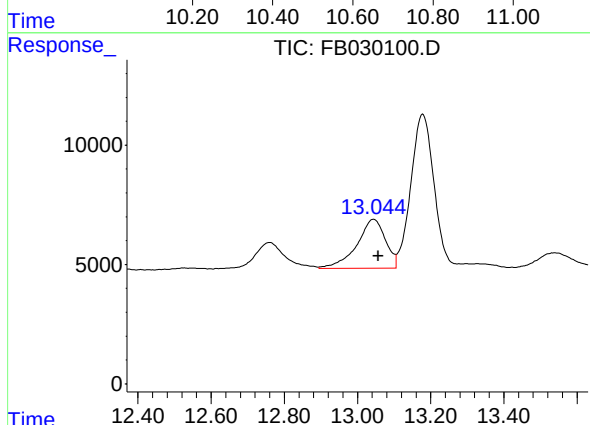


#7 Ethylbenzene

R.T.: 13.045 min
Delta R.T.: -0.011 min
Response: 111894
Conc: 5.53 ng/ml

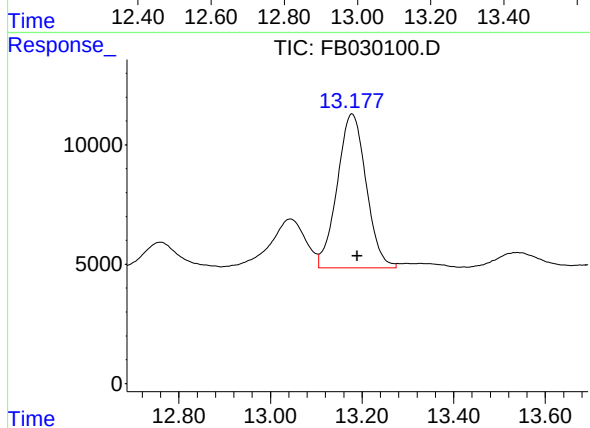

#8 m-Xylene


R.T.: 13.179 min
Delta R.T.: -0.010 min
Response: 283073
Conc: 14.08 ng/ml

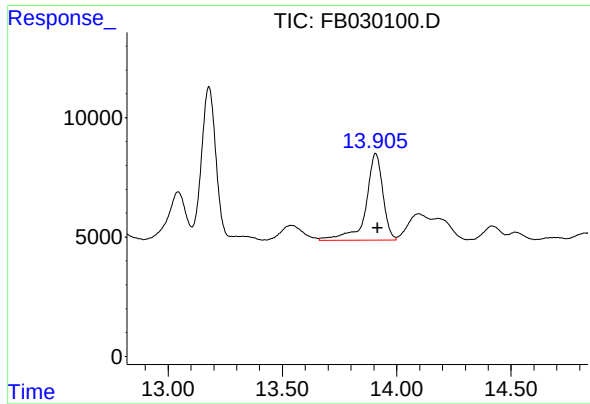

#9 O-Xylene

R.T.: 13.907 min
Delta R.T.: -0.009 min
Response: 188291
Conc: 9.66 ng/ml

Instrument :
FID_B
ClientSampleId :

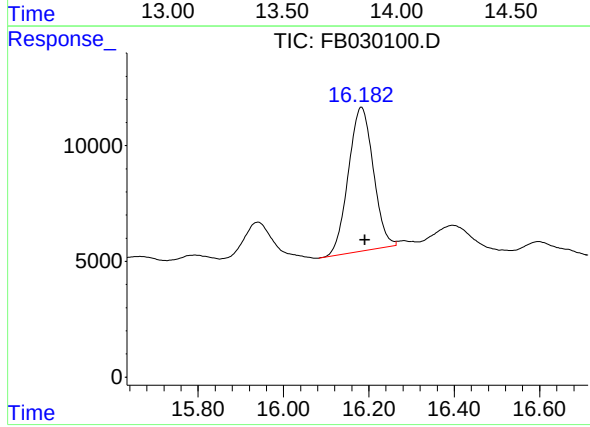

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.008 min
Response: 251632
Conc: 13.43 ng/ml