

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
 Data File : FB030104.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2023 13:42
 Operator : YP/AJ
 Sample : 03357-19 50X
 Misc : 7.54G/5.00 ML MEOH
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 22 23:37:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.785	337357	24.248 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	10185	0.539 ng/ml
3) t n-Heptane	7.750	3673	0.190 ng/ml
6) t Toluene	10.611	5780	0.266 ng/ml
8) t m-Xylene	13.181	12871	0.640 ng/ml
9) t O-Xylene	13.912	6885	0.353 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030104.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2023 13:42
Operator : YP/AJ
Sample : 03357-19 50X
Misc : 7.54G/5.00 ML MEOH
ALS Vial : 46 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 22 23:37:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

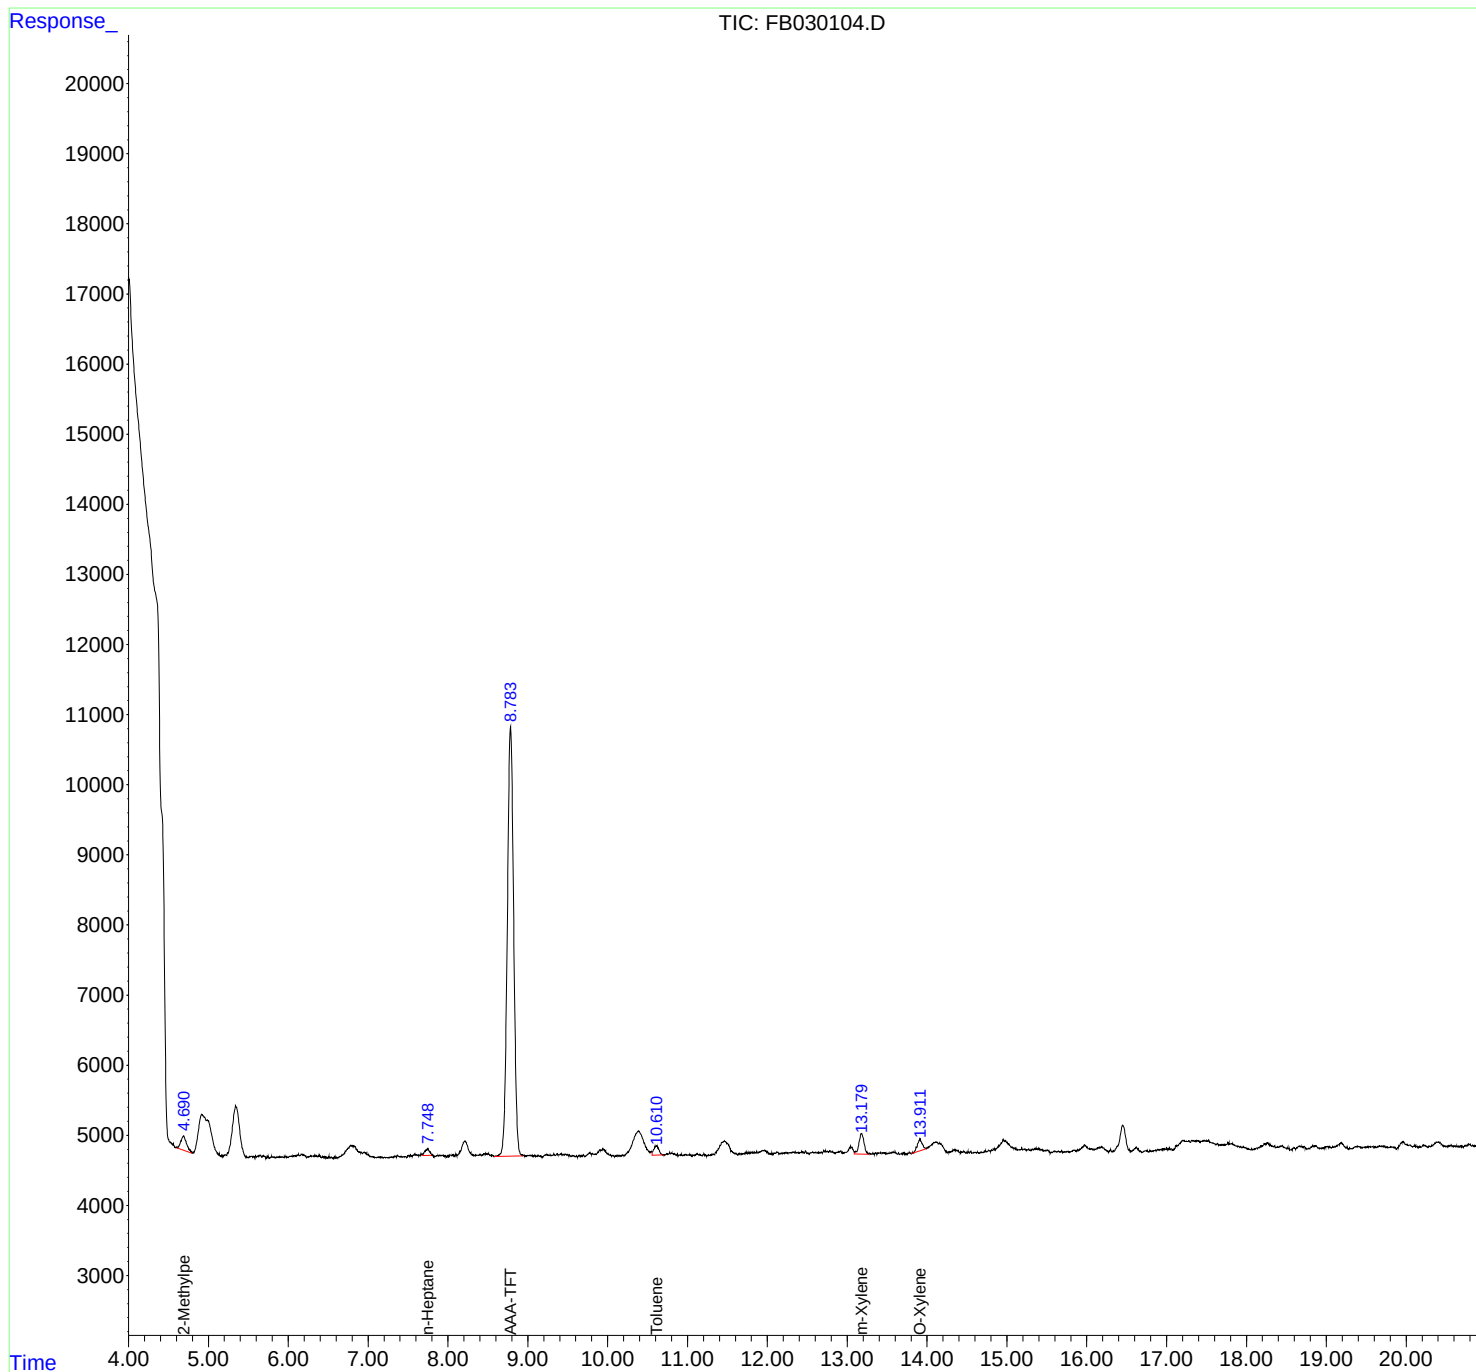

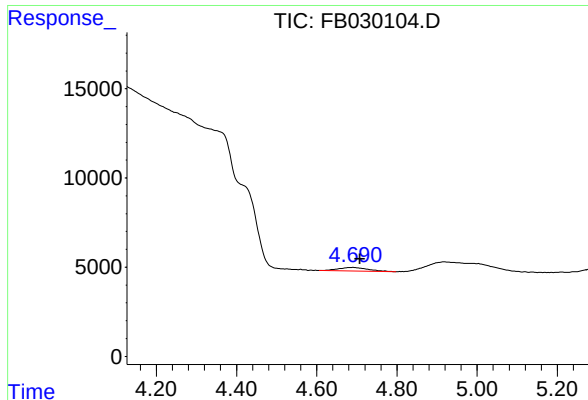


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: -0.016 min
Response: 10185
Conc: 0.54 ng/ml

Instrument :


FID_B

ClientSampleId :

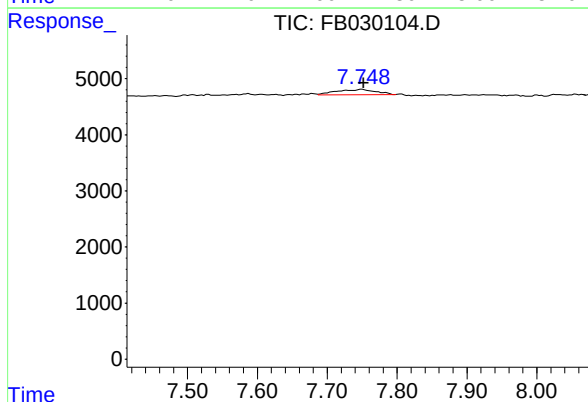


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.002 min
Response: 3673
Conc: 0.19 ng/ml

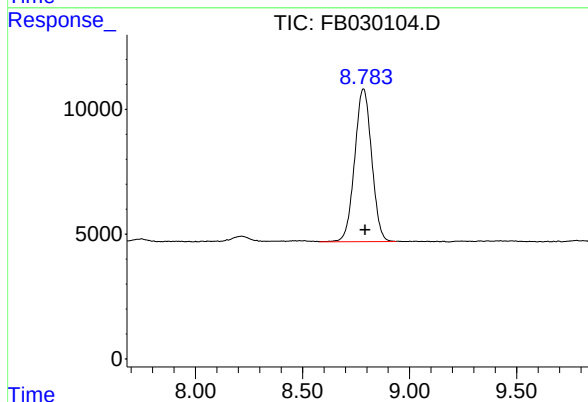


#5 AAA-TFT

R.T.: 8.785 min
Delta R.T.: -0.008 min
Response: 337357
Conc: 24.25 ng/ml

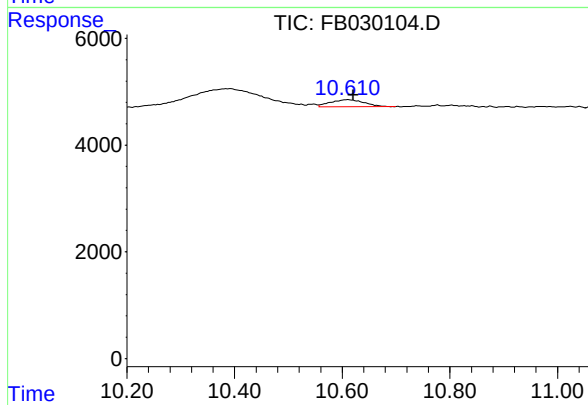

#6 Toluene


R.T.: 10.611 min
Delta R.T.: -0.009 min
Response: 5780
Conc: 0.27 ng/ml

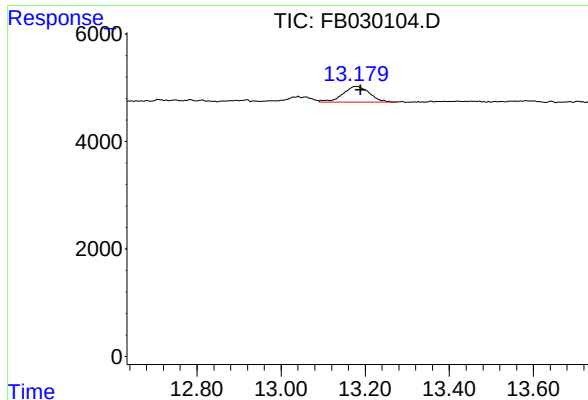

#8 m-Xylene

R.T.: 13.181 min
Delta R.T.: -0.008 min
Response: 12871
Conc: 0.64 ng/ml

Instrument :
FID_B
ClientSampleId :

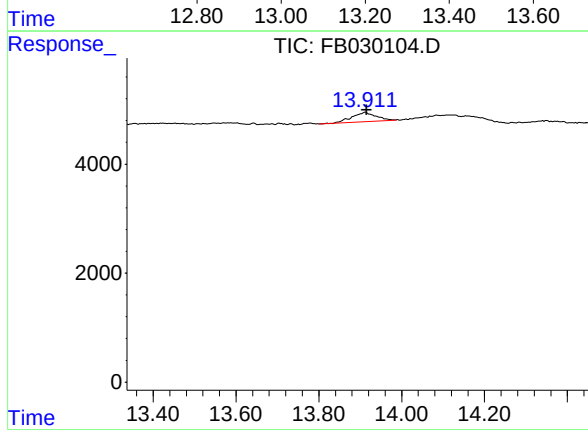

#9 o-Xylene

R.T.: 13.912 min
Delta R.T.: -0.004 min
Response: 6885
Conc: 0.35 ng/ml