

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
 Data File : FB030066.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2023 11:10
 Operator : YP/AJ
 Sample : BSF0621S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0621S1

Integration File: Calibration.e
 Quant Time: Jun 21 23:24:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.785	231778	16.660 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	569756	30.156 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	583654	30.932 ng/ml
3) t n-Heptane	7.743	199440	10.303 ng/ml
4) t Benzene	7.880	232991	10.409 ng/ml
6) t Toluene	10.612	677562	31.220 ng/ml
7) t Ethylbenzene	13.048	211556	10.463 ng/ml
8) t m-Xylene	13.181	421178	20.943 ng/ml
9) t O-Xylene	13.907	402073	20.629 ng/ml
10) t 1,2,4-Trimethylbenzene	16.182	398072	21.253 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030066.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2023 11:10
Operator : YP/AJ
Sample : BSF0621S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0621S1

Integration File: Calibration.e
Quant Time: Jun 21 23:24:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

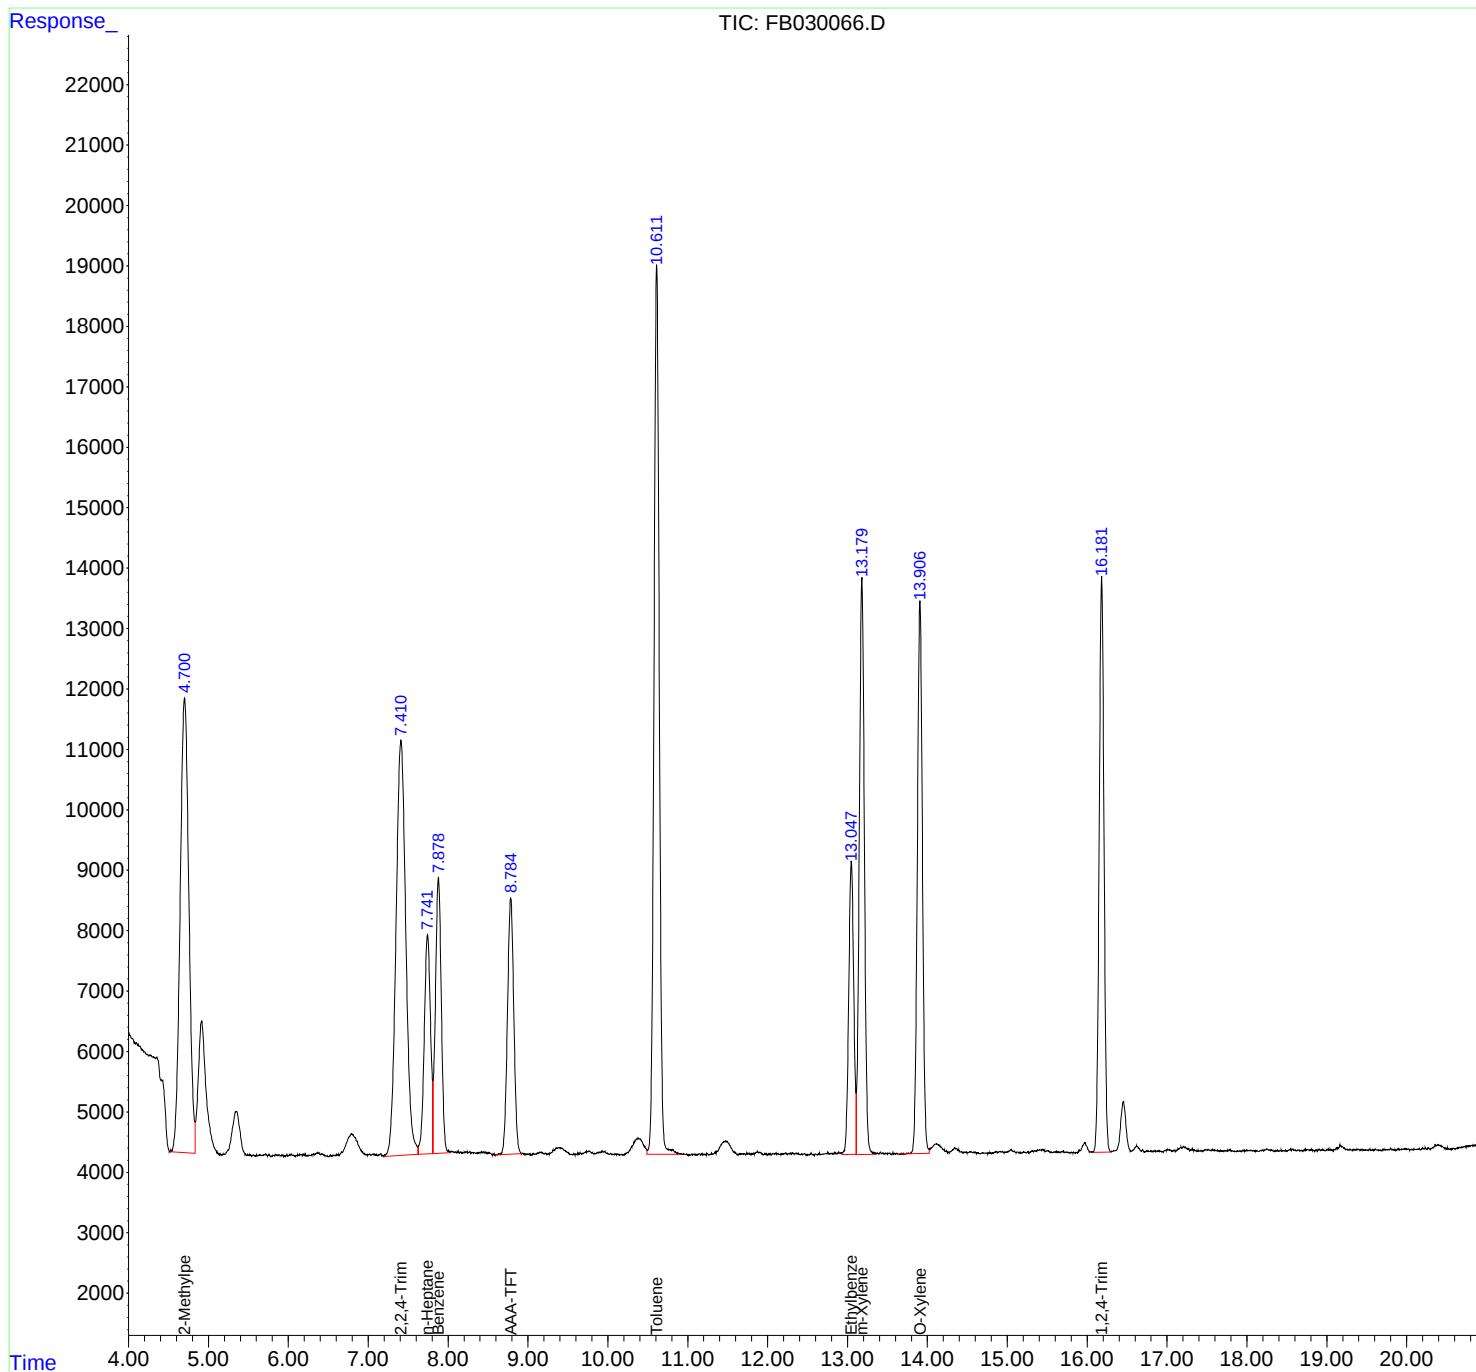


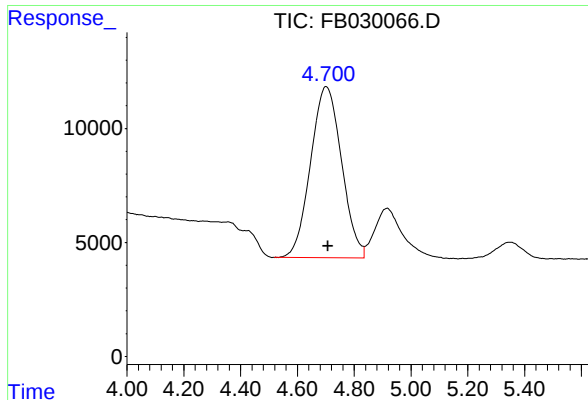

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.007 min
Response: 569756
Conc: 30.16 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S1

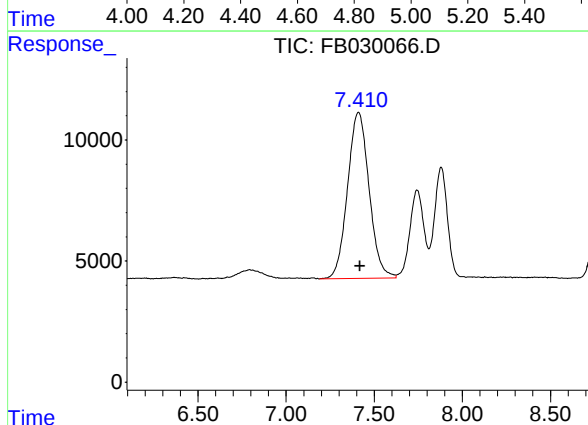


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.007 min
Response: 583654
Conc: 30.93 ng/ml

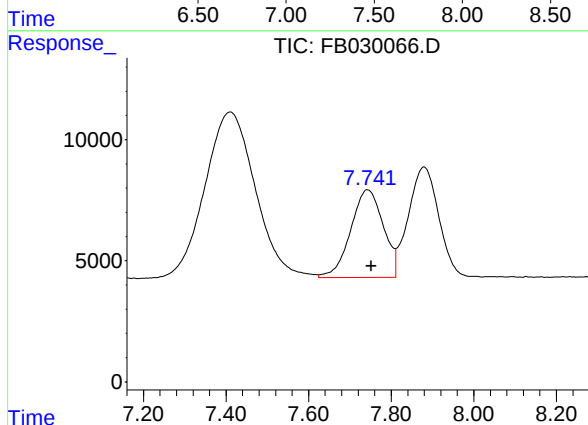


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.009 min
Response: 199440
Conc: 10.30 ng/ml

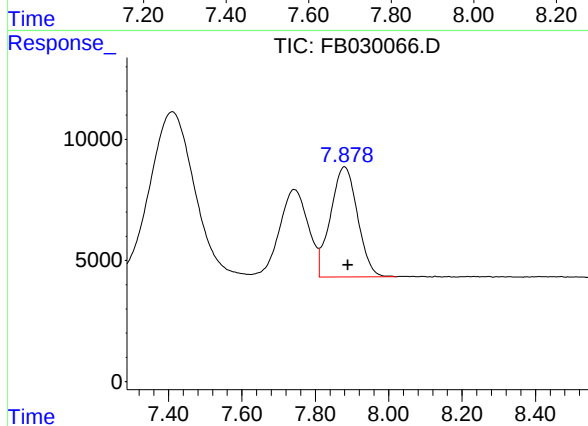

#4 Benzene


R.T.: 7.880 min
Delta R.T.: -0.009 min
Response: 232991
Conc: 10.41 ng/ml

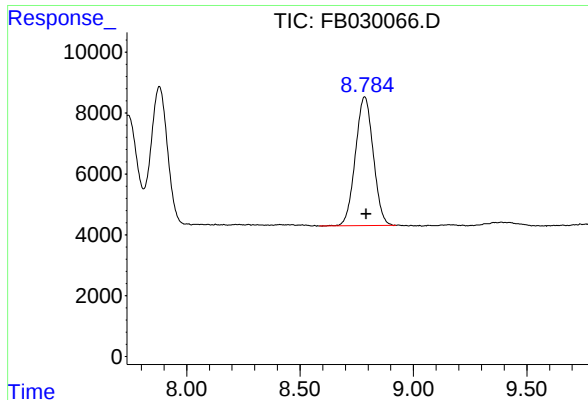

#5 AAA-TFT


R.T.: 8.785 min
Delta R.T.: -0.007 min
Response: 231778
Conc: 16.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S1

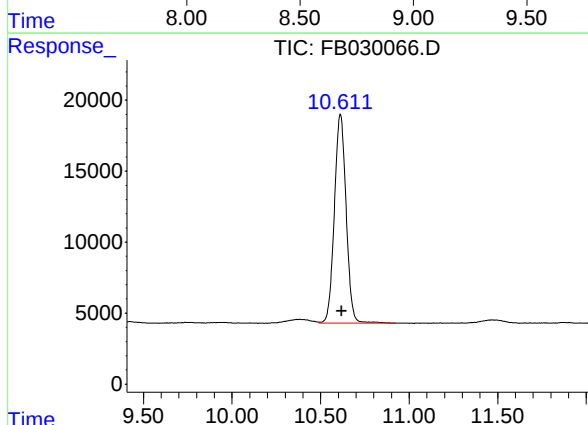


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.008 min
Response: 677562
Conc: 31.22 ng/ml

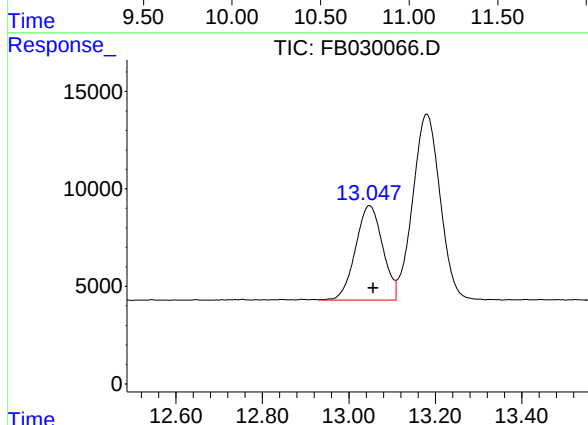


#7 Ethylbenzene

R.T.: 13.048 min
Delta R.T.: -0.008 min
Response: 211556
Conc: 10.46 ng/ml

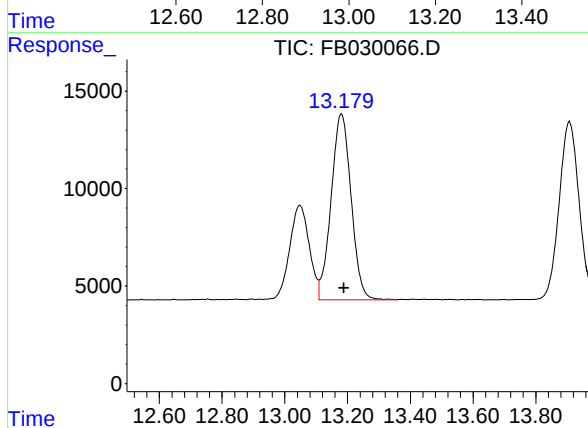

#8 m-Xylene


R.T.: 13.181 min
Delta R.T.: -0.008 min
Response: 421178
Conc: 20.94 ng/ml

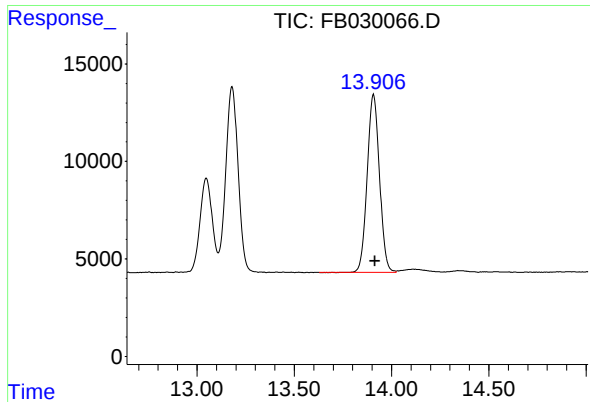

#9 O-Xylene

R.T.: 13.907 min
Delta R.T.: -0.009 min
Response: 402073
Conc: 20.63 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S1

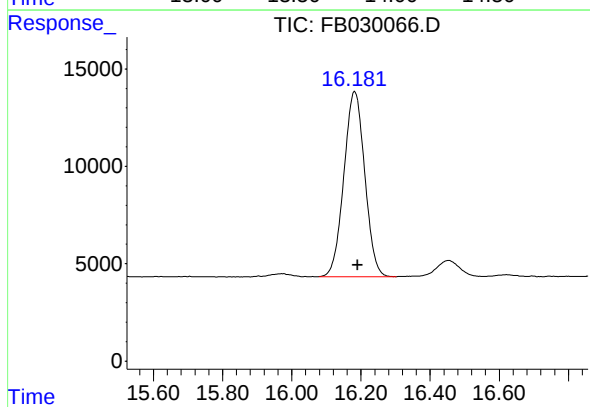

#10 1,2,4-Trimethylbenzene

R.T.: 16.182 min
Delta R.T.: -0.008 min
Response: 398072
Conc: 21.25 ng/ml