

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
 Data File : FB030070.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2023 13:42
 Operator : YP/AJ
 Sample : 03352-01MS 50X
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-3-062023MS

Integration File: Calibration.e
 Quant Time: Jun 21 23:24:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	296675	21.324 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.696	507588	26.865 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	531213	28.152 ng/ml
3) t n-Heptane	7.740	193221	9.982 ng/ml
4) t Benzene	7.877	243673	10.886 ng/ml
6) t Toluene	10.612	698763	32.196 ng/ml
7) t Ethylbenzene	13.049	216417	10.703 ng/ml
8) t m-Xylene	13.182	424595	21.113 ng/ml
9) t O-Xylene	13.909	405229	20.791 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	368087	19.652 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030070.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2023 13:42
Operator : YP/AJ
Sample : 03352-01MS 50X
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-3-062023MS

Integration File: Calibration.e
Quant Time: Jun 21 23:24:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

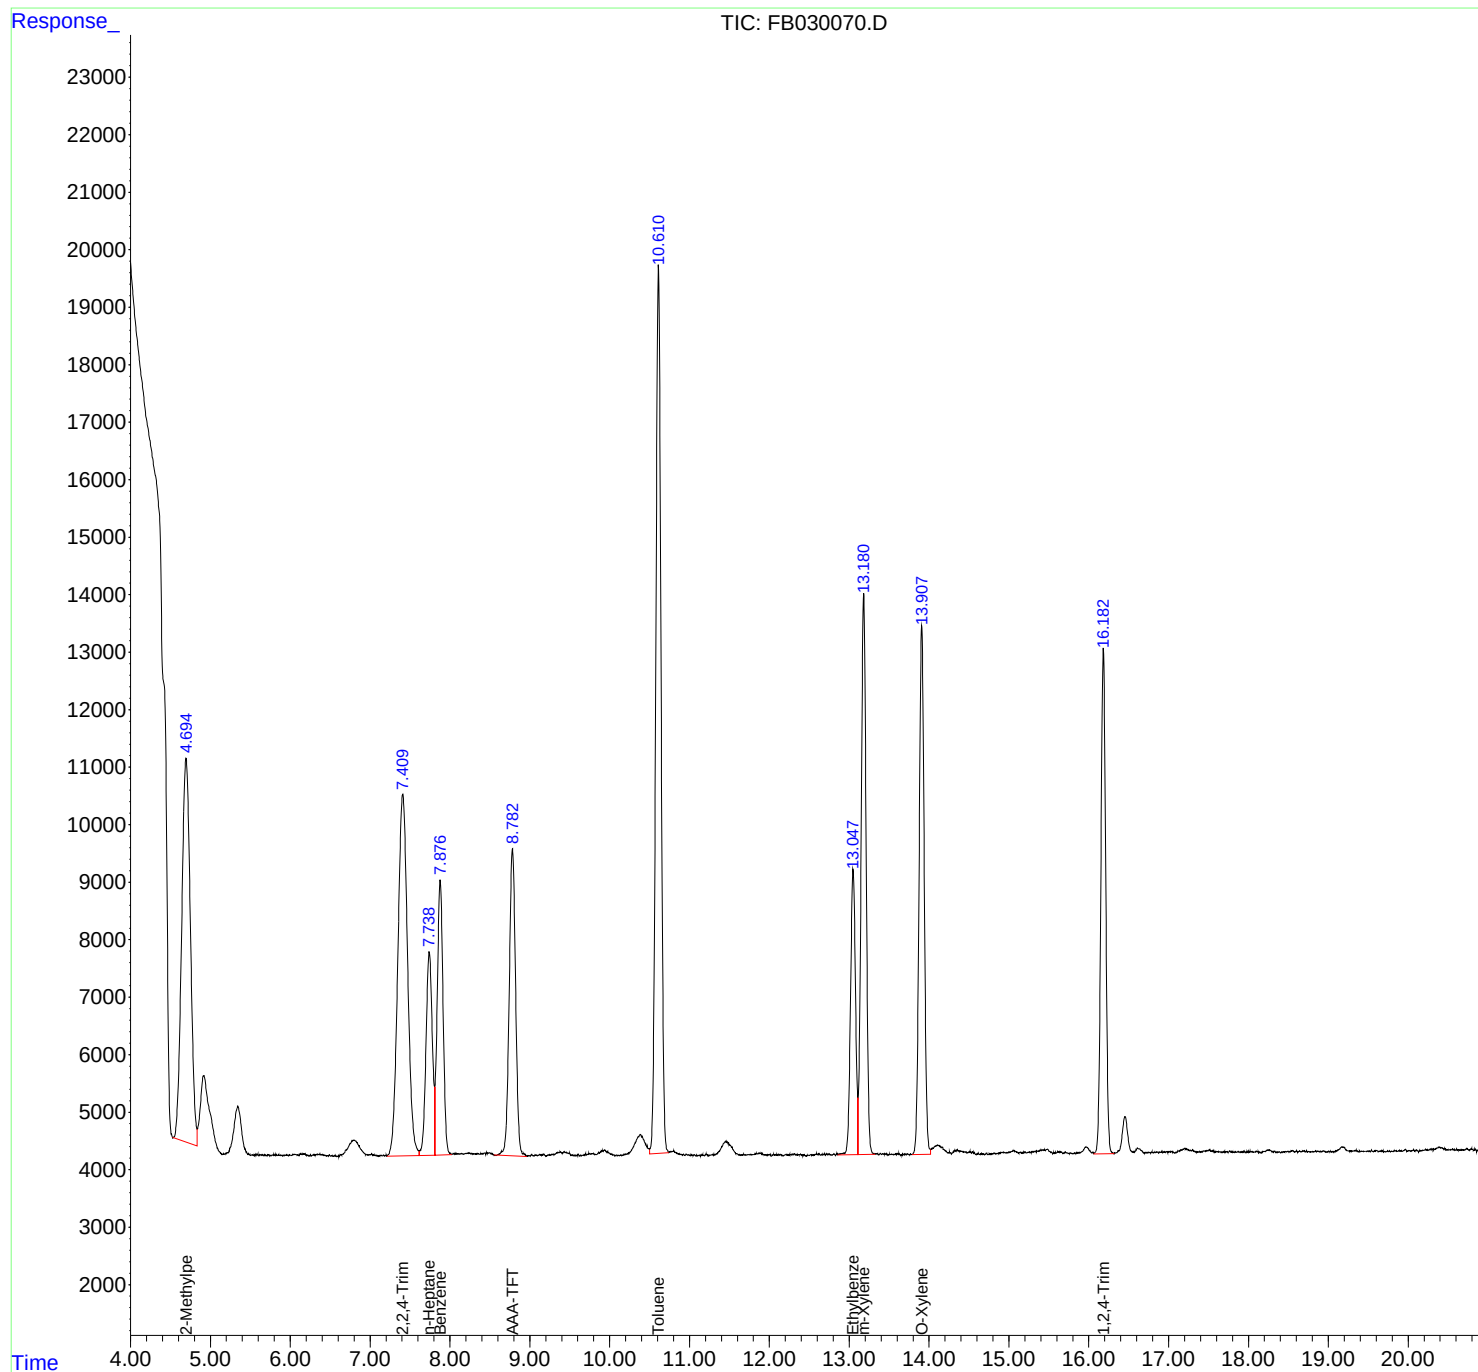


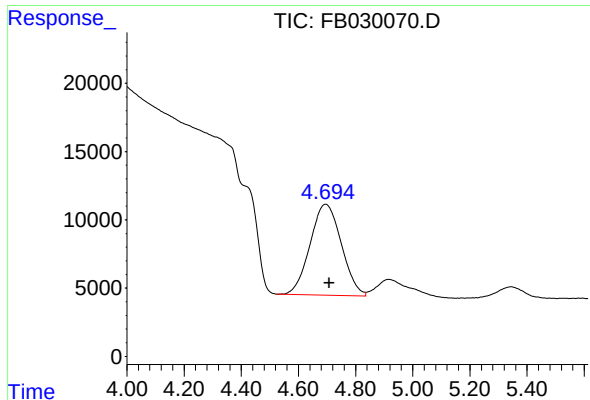

#1 2-Methylpentane


R.T.: 4.696 min
Delta R.T.: -0.012 min
Response: 507588
Conc: 26.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-3-062023MS

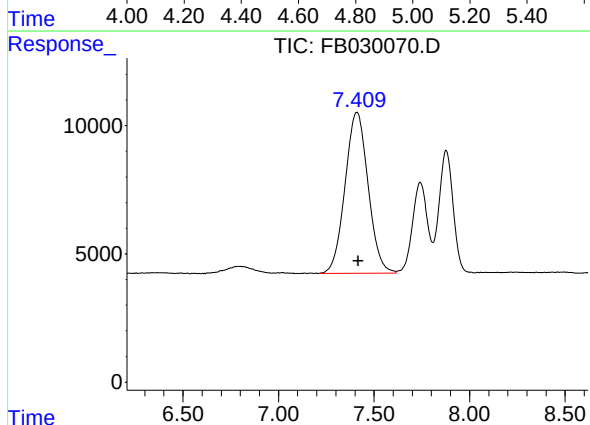


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.009 min
Response: 531213
Conc: 28.15 ng/ml

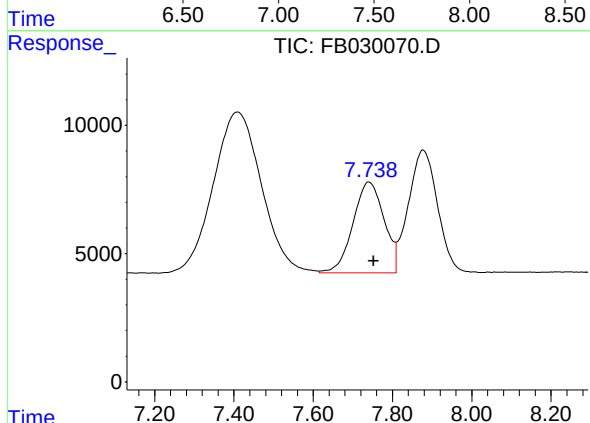


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.012 min
Response: 193221
Conc: 9.98 ng/ml

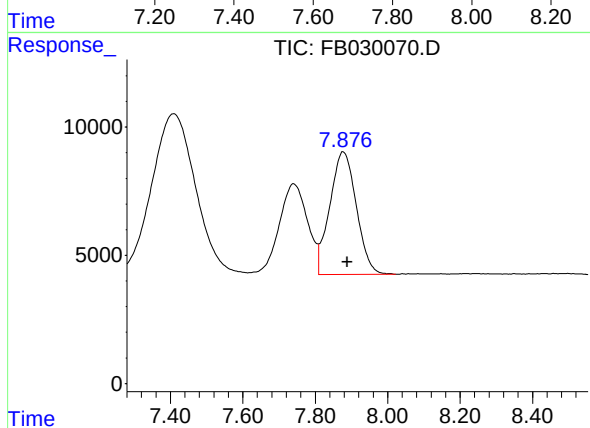

#4 Benzene


R.T.: 7.877 min
Delta R.T.: -0.011 min
Response: 243673
Conc: 10.89 ng/ml

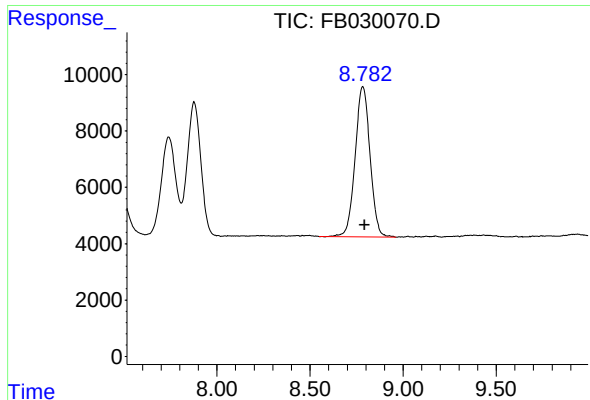

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: -0.009 min
Response: 296675
Conc: 21.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-3-062023MS

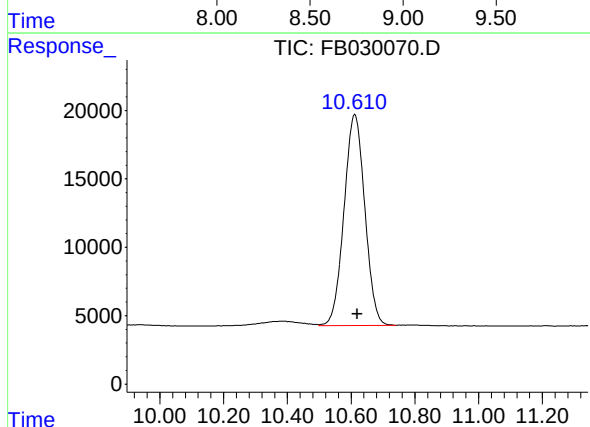


#6 Toluene

R.T.: 10.612 min
Delta R.T.: -0.009 min
Response: 698763
Conc: 32.20 ng/ml

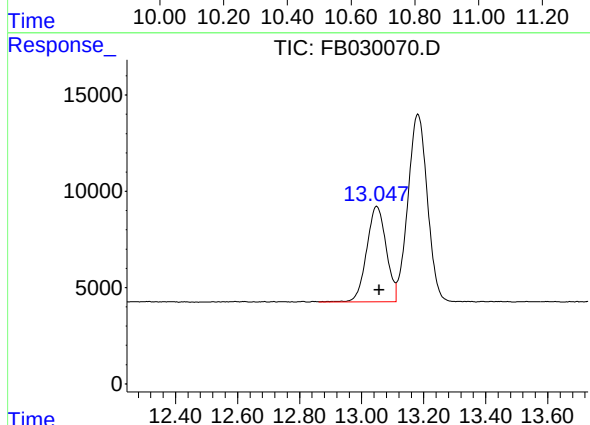


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.008 min
Response: 216417
Conc: 10.70 ng/ml

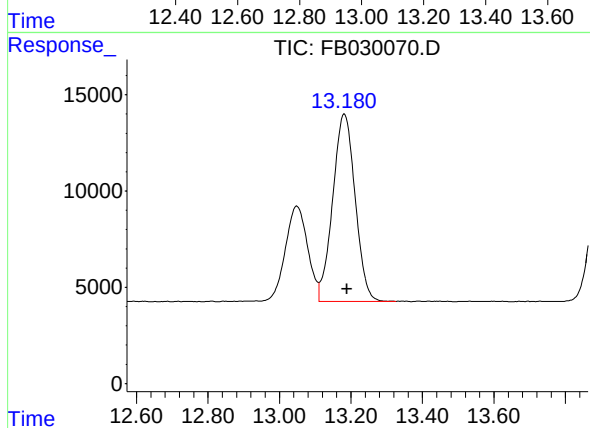

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: -0.007 min
Response: 424595
Conc: 21.11 ng/ml

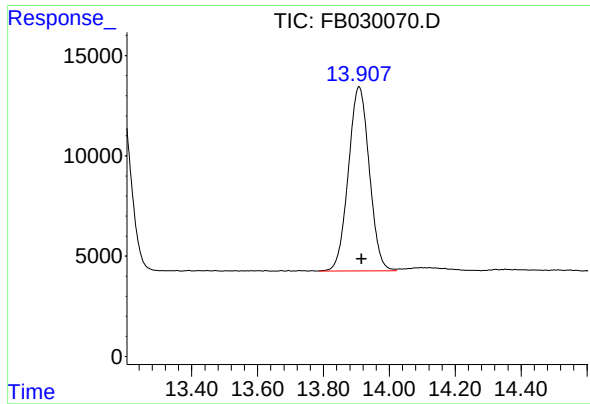

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: -0.007 min
Response: 405229
Conc: 20.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-3-062023MS

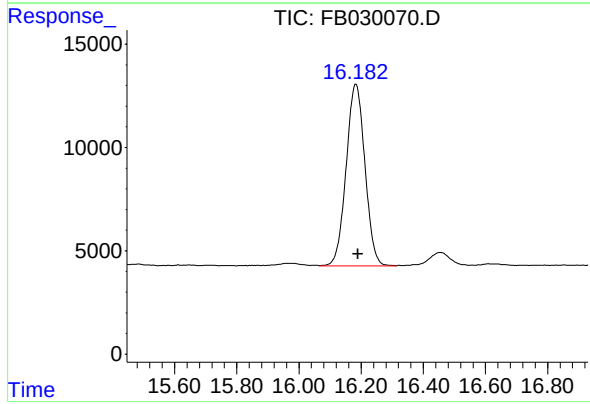

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.007 min
Response: 368087
Conc: 19.65 ng/ml