

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB062123\  
Data File : FB030076.D  
Signal(s) : FID2B.CH  
Acq On : 21 Jun 2023 18:48  
Operator : YP/AJ  
Sample : 03357-19  
Misc : 7.54G/5.00 ML DI WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
WC-SCAN-04-G

Integration File: Calibration.e  
Quant Time: Jun 21 23:25:22 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB060323.M  
Quant Title :  
QLast Update : Mon Jun 05 04:33:00 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units  |
|-----------------------------|-------|----------|-------------|
| -----                       |       |          |             |
| System Monitoring Compounds |       |          |             |
| 5) s AAA-TFT                | 8.790 | 11176    | 0.803 ng/ml |
| Target Compounds            |       |          |             |
| -----                       |       |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB062123\  
Data File : FB030076.D  
Signal(s) : FID2B.CH  
Acq On : 21 Jun 2023 18:48  
Operator : YP/AJ  
Sample : 03357-19  
Misc : 7.54G/5.00 ML DI WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
WC-SCAN-04-G

Integration File: Calibration.e  
Quant Time: Jun 21 23:25:22 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB060323.M  
Quant Title :  
QLast Update : Mon Jun 05 04:33:00 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

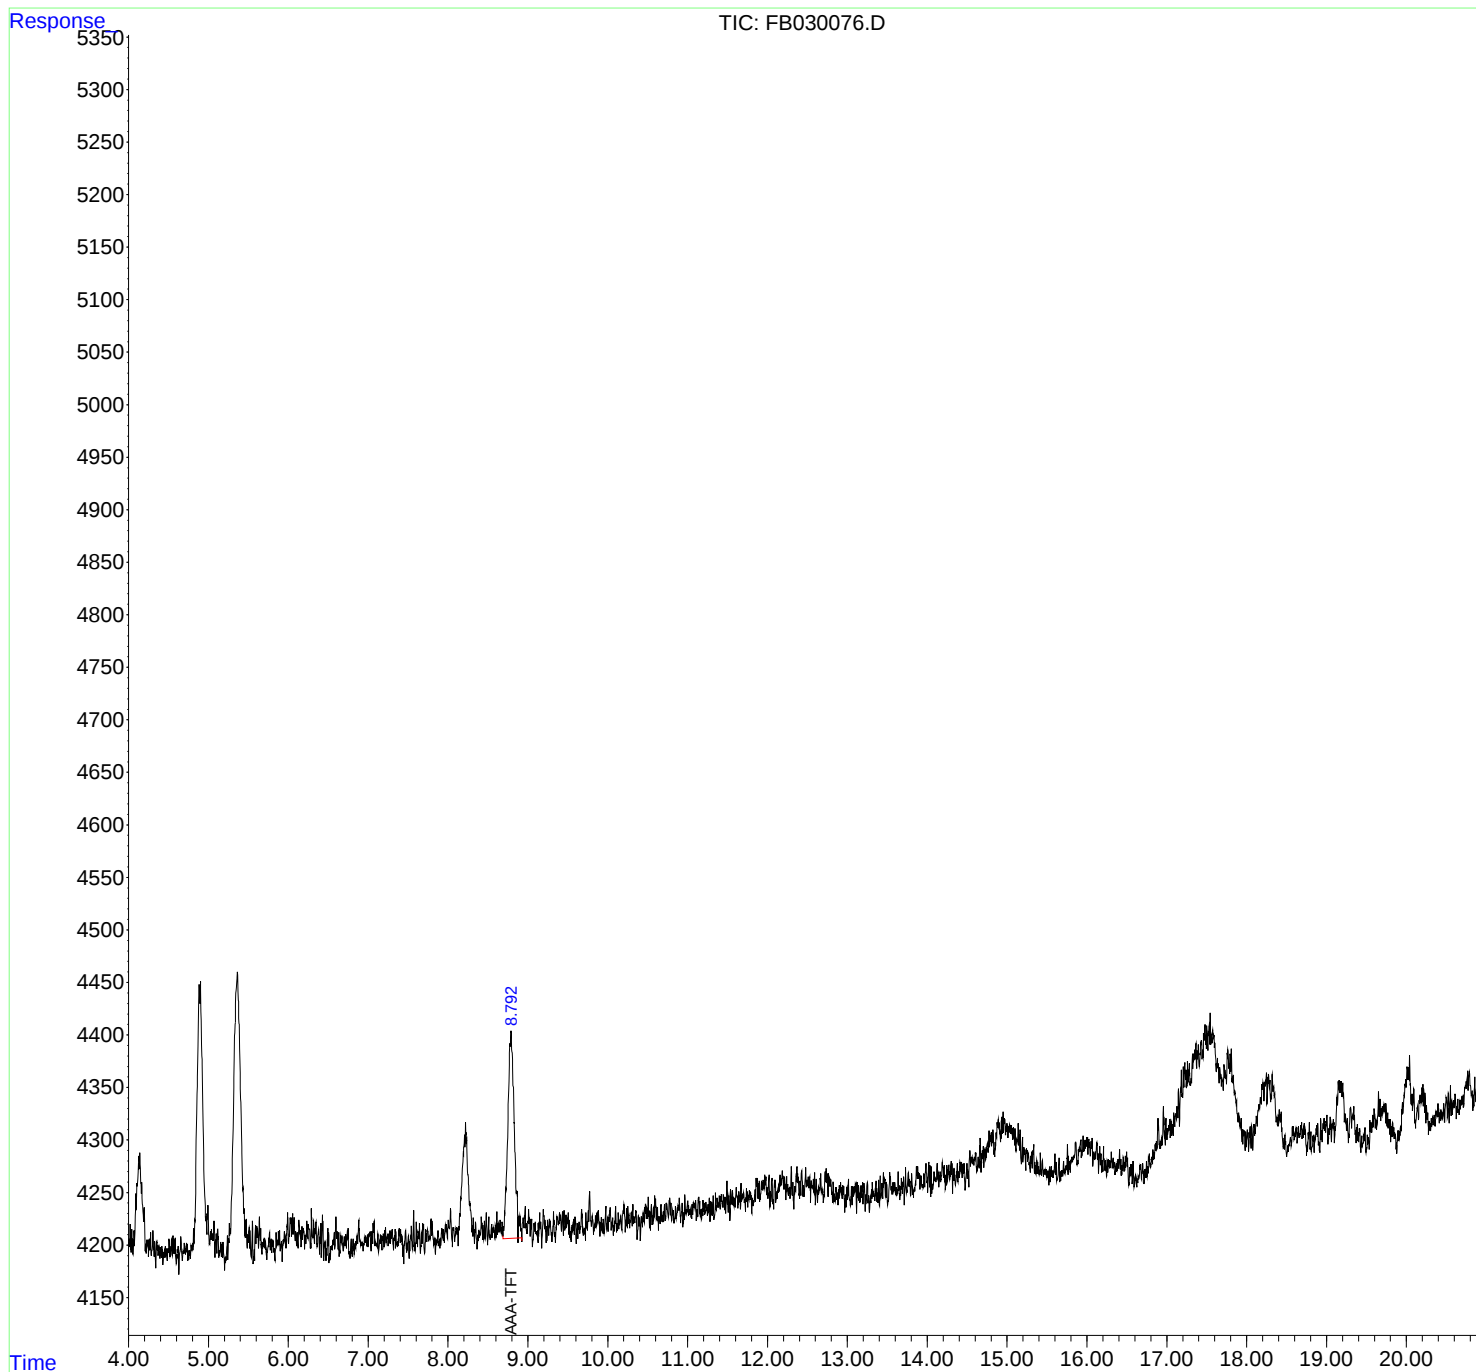

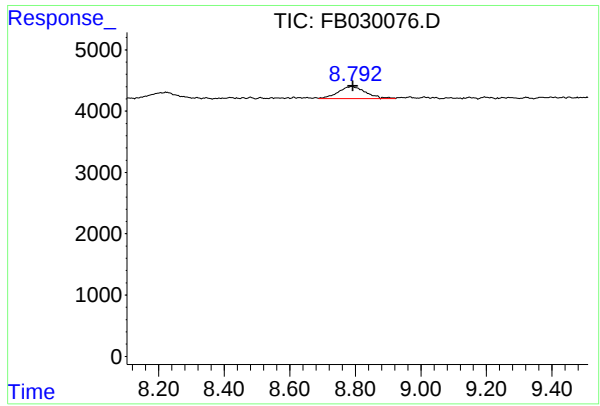

#5 AAA-TFT

R.T.: 8.790 min  
Delta R.T.: -0.003 min  
Response: 11176  
Conc: 0.80 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
WC-SCAN-04-G