

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
 Data File : FB030082.D
 Signal(s) : FID2B.CH
 Acq On : 21 Jun 2023 22:37
 Operator : YP/AJ
 Sample : BSF0621S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0621S2

Integration File: Calibration.e
 Quant Time: Jun 21 23:25:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	281874	20.260 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	588325	31.138 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	588961	31.213 ng/ml
3) t n-Heptane	7.746	202072	10.439 ng/ml
4) t Benzene	7.882	237440	10.608 ng/ml
6) t Toluene	10.614	705891	32.525 ng/ml
7) t Ethylbenzene	13.050	219919	10.876 ng/ml
8) t m-Xylene	13.182	433796	21.571 ng/ml
9) t O-Xylene	13.909	411604	21.118 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	401274	21.424 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030082.D
Signal(s) : FID2B.CH
Acq On : 21 Jun 2023 22:37
Operator : YP/AJ
Sample : BSF0621S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0621S2

Integration File: Calibration.e
Quant Time: Jun 21 23:25:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

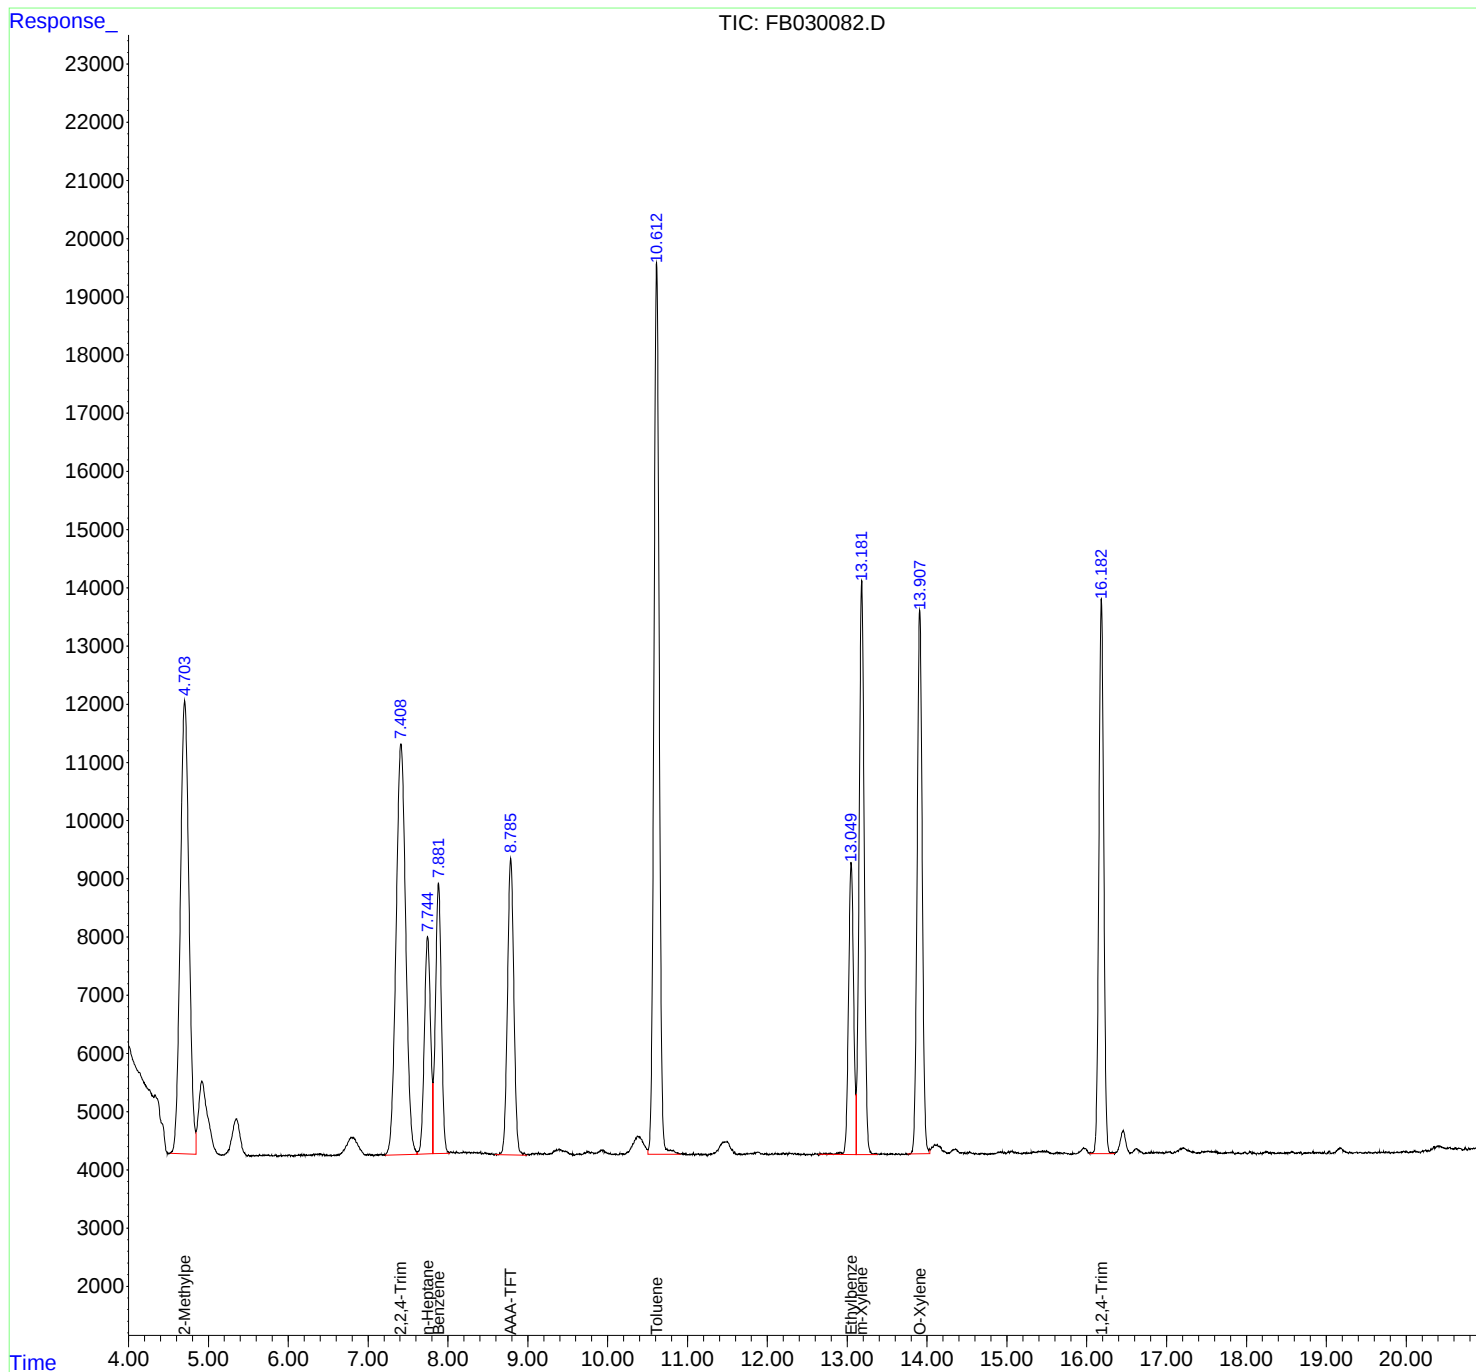


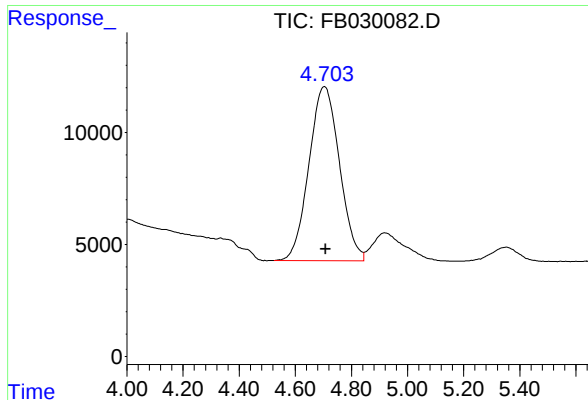

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.004 min
Response: 588325
Conc: 31.14 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S2

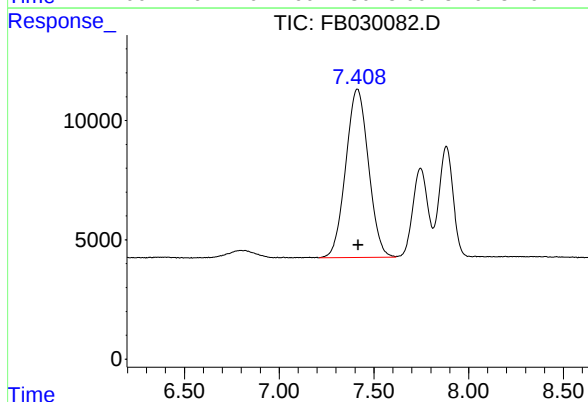


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.008 min
Response: 588961
Conc: 31.21 ng/ml

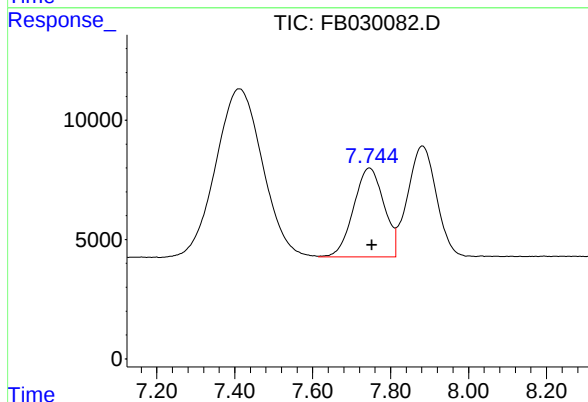


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.006 min
Response: 202072
Conc: 10.44 ng/ml

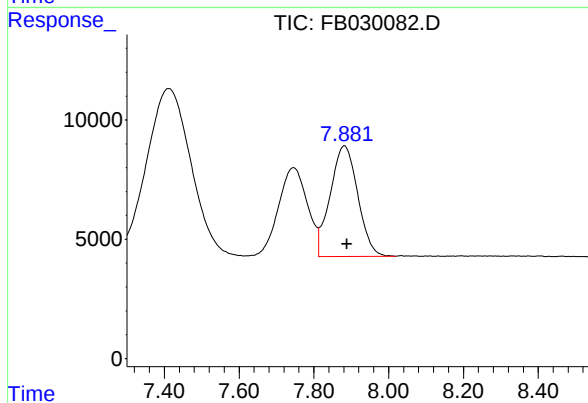

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.006 min
Response: 237440
Conc: 10.61 ng/ml

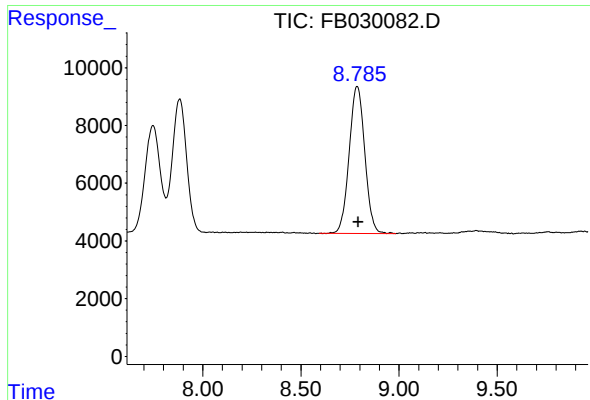

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.006 min
Response: 281874
Conc: 20.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S2

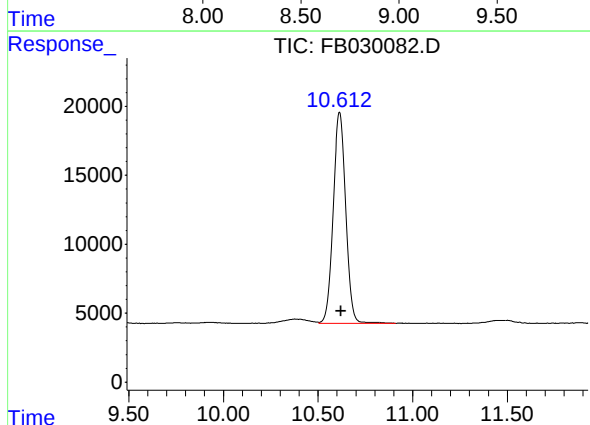


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.006 min
Response: 705891
Conc: 32.52 ng/ml

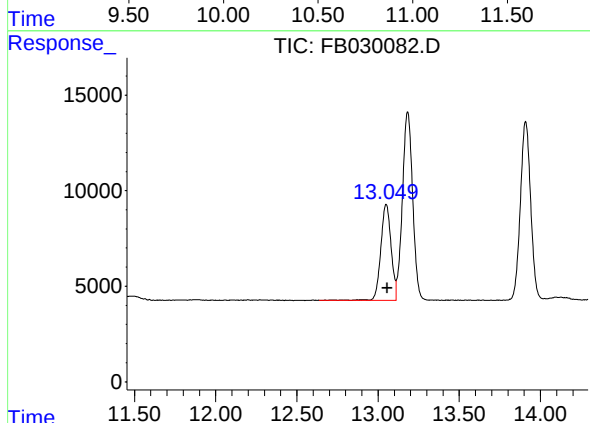


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: -0.007 min
Response: 219919
Conc: 10.88 ng/ml

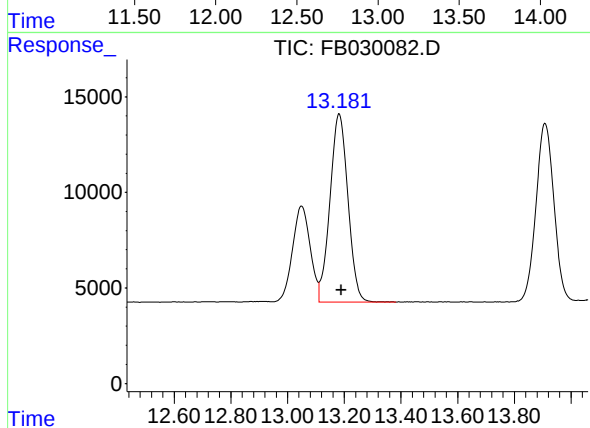

#8 m-Xylene


R.T.: 13.182 min
Delta R.T.: -0.007 min
Response: 433796
Conc: 21.57 ng/ml

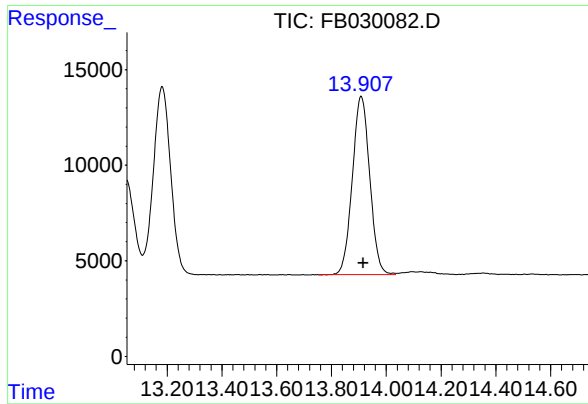

#9 O-Xylene

R.T.: 13.909 min
Delta R.T.: -0.007 min
Response: 411604
Conc: 21.12 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S2

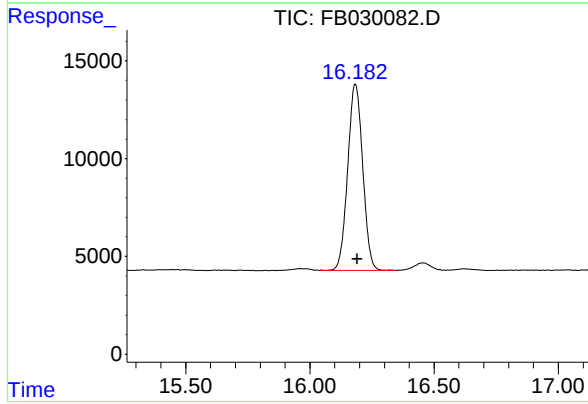

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.007 min
Response: 401274
Conc: 21.42 ng/ml