

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030091.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2023 4:54
Operator : YP/AJ
Sample : 03355-12
Misc : 5.09G/5.00 ML DI WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-06-COMP

Integration File: Calibration.e
Quant Time: Jun 22 05:53:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030091.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2023 4:54
Operator : YP/AJ
Sample : 03355-12
Misc : 5.09G/5.00 ML DI WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-06-COMP

Integration File: Calibration.e
Quant Time: Jun 22 05:53:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

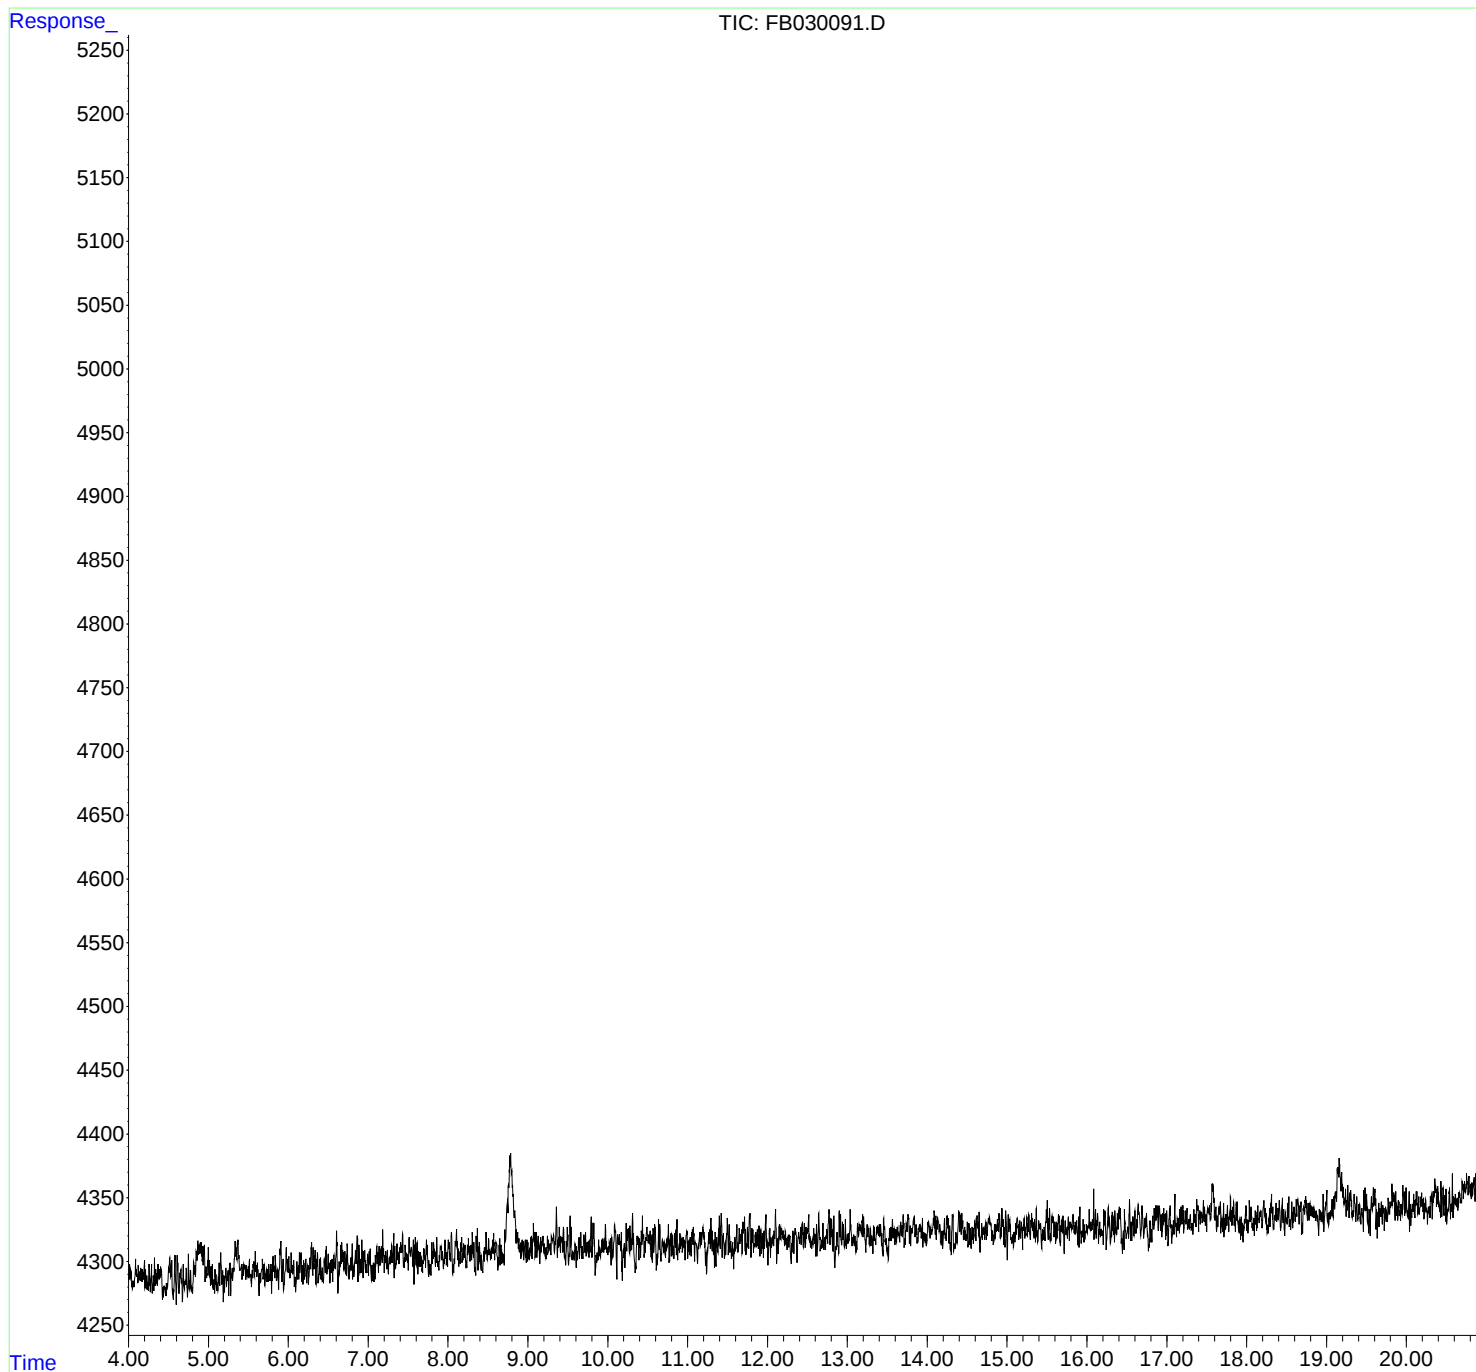

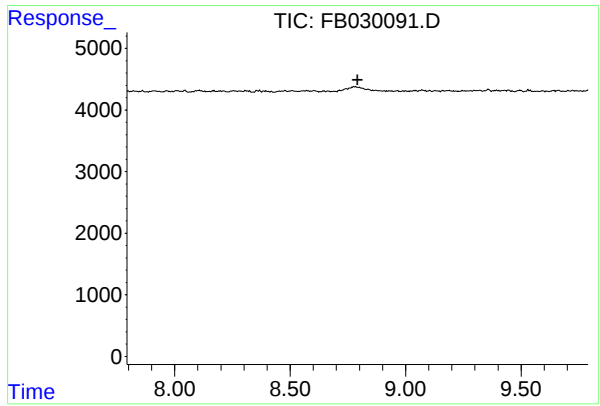

#5 AAA-TFT

R.T.: 0.000 min
Exp R.T.: 8.793 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :
SB-06-COMP