

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
 Data File : FB030093.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2023 6:09
 Operator : YP/AJ
 Sample : BSF0621S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0621S3

Integration File: Calibration.e
 Quant Time: Jun 22 07:12:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.784	218617	15.714 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.703	535654	28.351 ng/ml
2) t	2,2,4-Trimethylpentane	7.408	537109	28.465 ng/ml
3) t	n-Heptane	7.743	185134	9.564 ng/ml
4) t	Benzene	7.880	217488	9.716 ng/ml
6) t	Toluene	10.611	629978	29.027 ng/ml
7) t	Ethylbenzene	13.046	198545	9.819 ng/ml
8) t	m-Xylene	13.179	394639	19.624 ng/ml
9) t	O-Xylene	13.906	377374	19.362 ng/ml
10) t	1,2,4-Trimethylbenzene	16.181	372334	19.879 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030093.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2023 6:09
Operator : YP/AJ
Sample : BSF0621S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0621S3

Integration File: Calibration.e
Quant Time: Jun 22 07:12:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

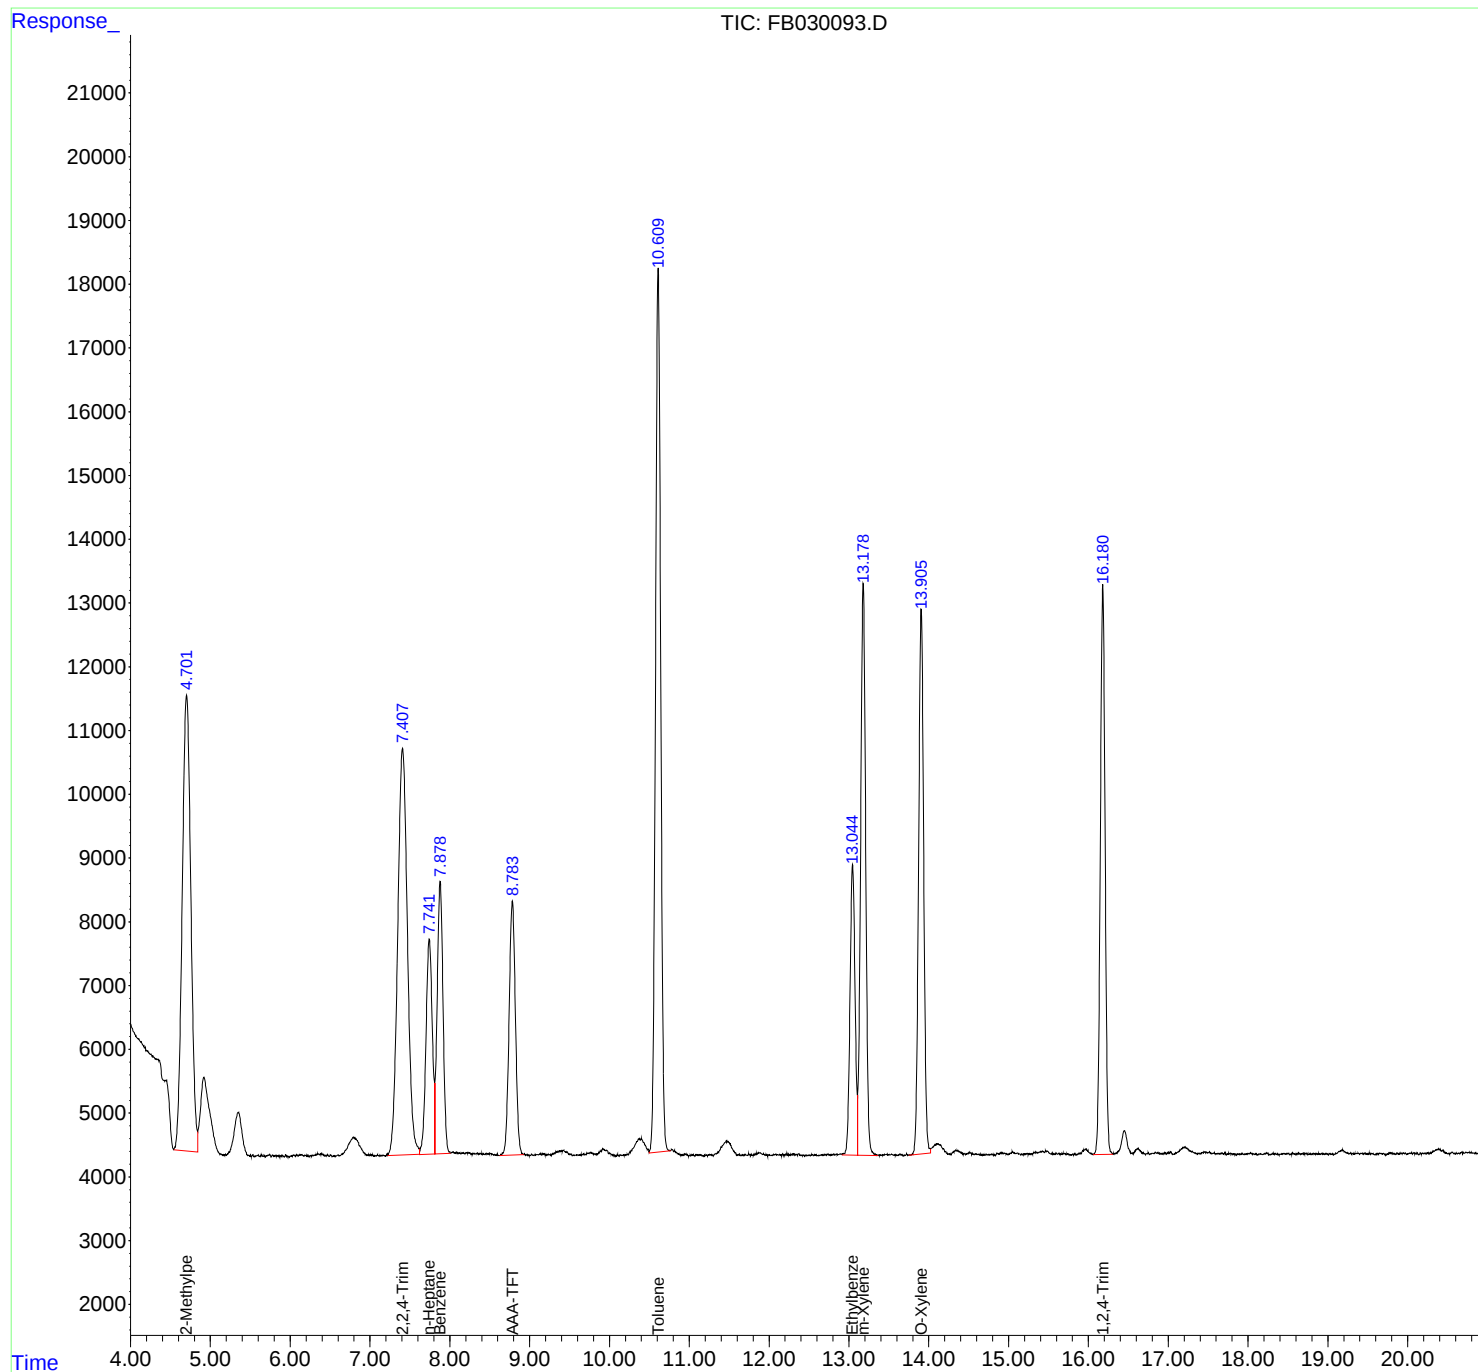


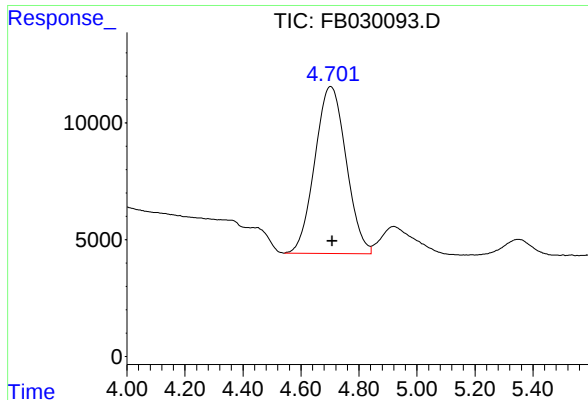

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.005 min
Response: 535654
Conc: 28.35 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S3

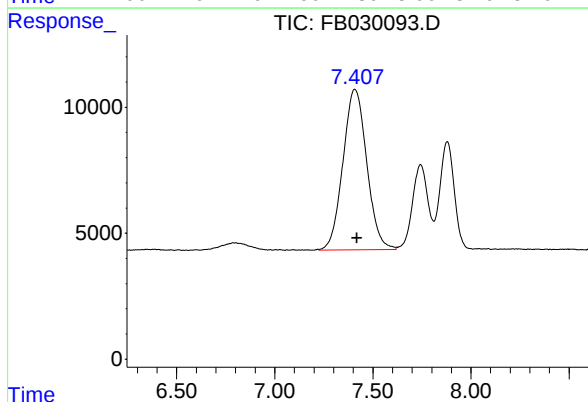


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: -0.011 min
Response: 537109
Conc: 28.46 ng/ml

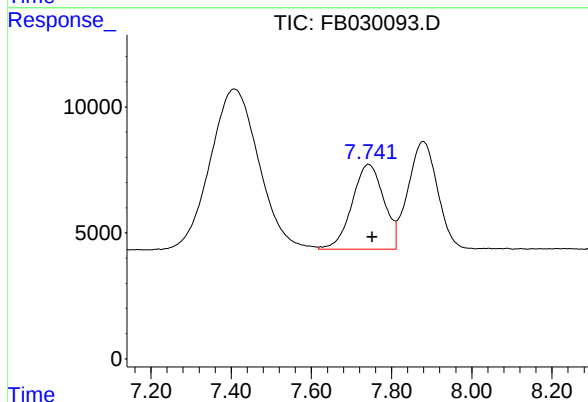


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.009 min
Response: 185134
Conc: 9.56 ng/ml

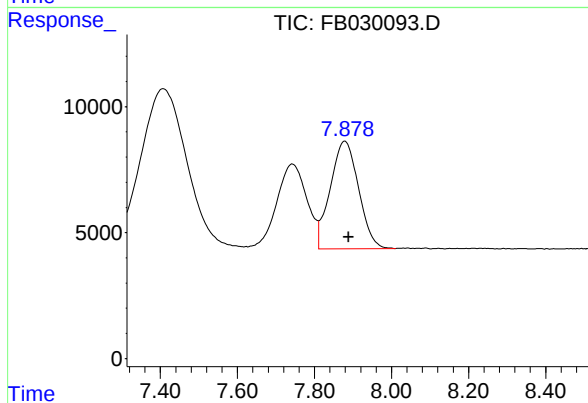

#4 Benzene


R.T.: 7.880 min
Delta R.T.: -0.009 min
Response: 217488
Conc: 9.72 ng/ml

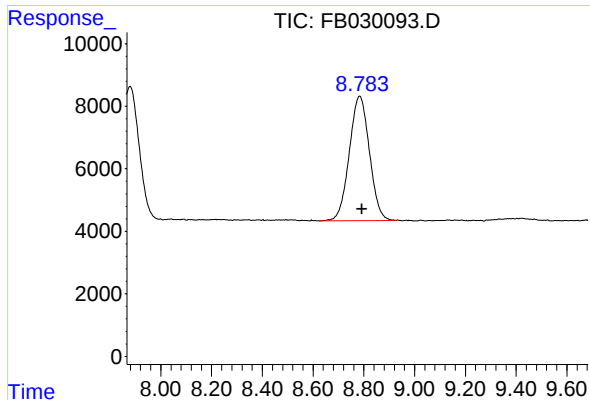

#5 AAA-TFT


R.T.: 8.784 min
Delta R.T.: -0.008 min
Response: 218617
Conc: 15.71 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S3

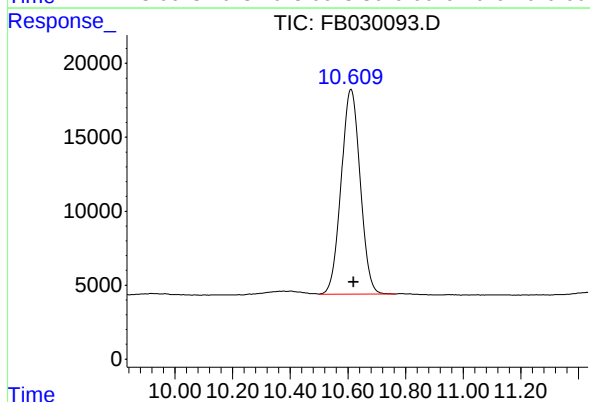


#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.010 min
Response: 629978
Conc: 29.03 ng/ml

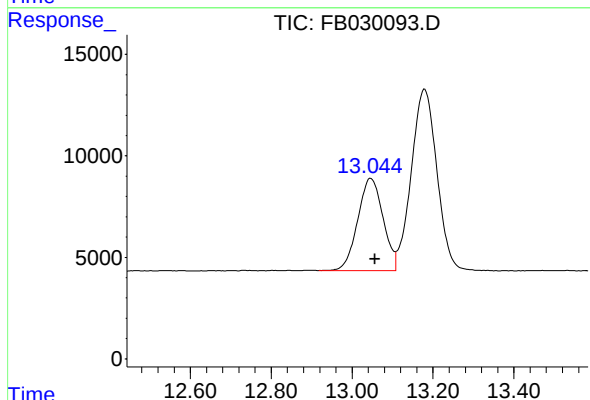


#7 Ethylbenzene

R.T.: 13.046 min
Delta R.T.: -0.011 min
Response: 198545
Conc: 9.82 ng/ml

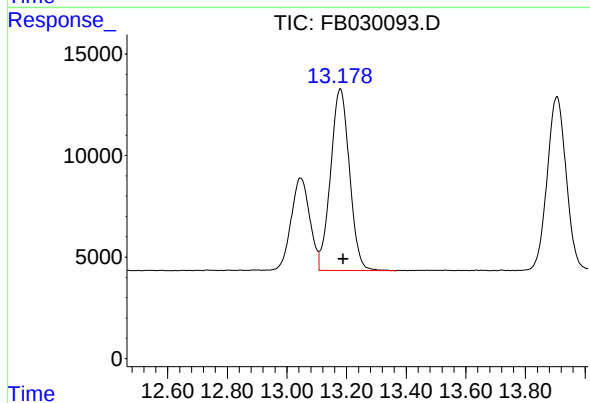

#8 m-Xylene


R.T.: 13.179 min
Delta R.T.: -0.010 min
Response: 394639
Conc: 19.62 ng/ml

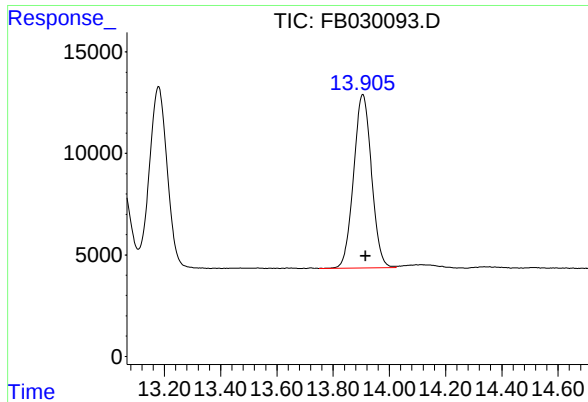

#9 O-Xylene

R.T.: 13.906 min
Delta R.T.: -0.010 min
Response: 377374
Conc: 19.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S3

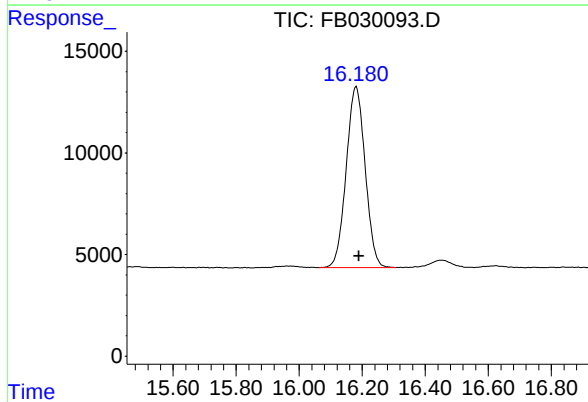

#10 1,2,4-Trimethylbenzene

R.T.: 16.181 min
Delta R.T.: -0.010 min
Response: 372334
Conc: 19.88 ng/ml