

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB062123\  
Data File : FB030099.D  
Signal(s) : FID2B.CH  
Acq On : 22 Jun 2023 10:32  
Operator : YP/AJ  
Sample : 03357-14  
Misc : 7.14G/5.00 ML DI WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
WC-SCAN-03-G

Integration File: Calibration.e  
Quant Time: Jun 22 23:36:50 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB060323.M  
Quant Title :  
QLast Update : Mon Jun 05 04:33:00 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 5) s AAA-TFT                | 8.784 | 150704   | 10.832 ng/ml |
| Target Compounds            |       |          |              |
| -----                       |       |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB062123\  
Data File : FB030099.D  
Signal(s) : FID2B.CH  
Acq On : 22 Jun 2023 10:32  
Operator : YP/AJ  
Sample : 03357-14  
Misc : 7.14G/5.00 ML DI WATER  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
WC-SCAN-03-G

Integration File: Calibration.e  
Quant Time: Jun 22 23:36:50 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB060323.M  
Quant Title :  
QLast Update : Mon Jun 05 04:33:00 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

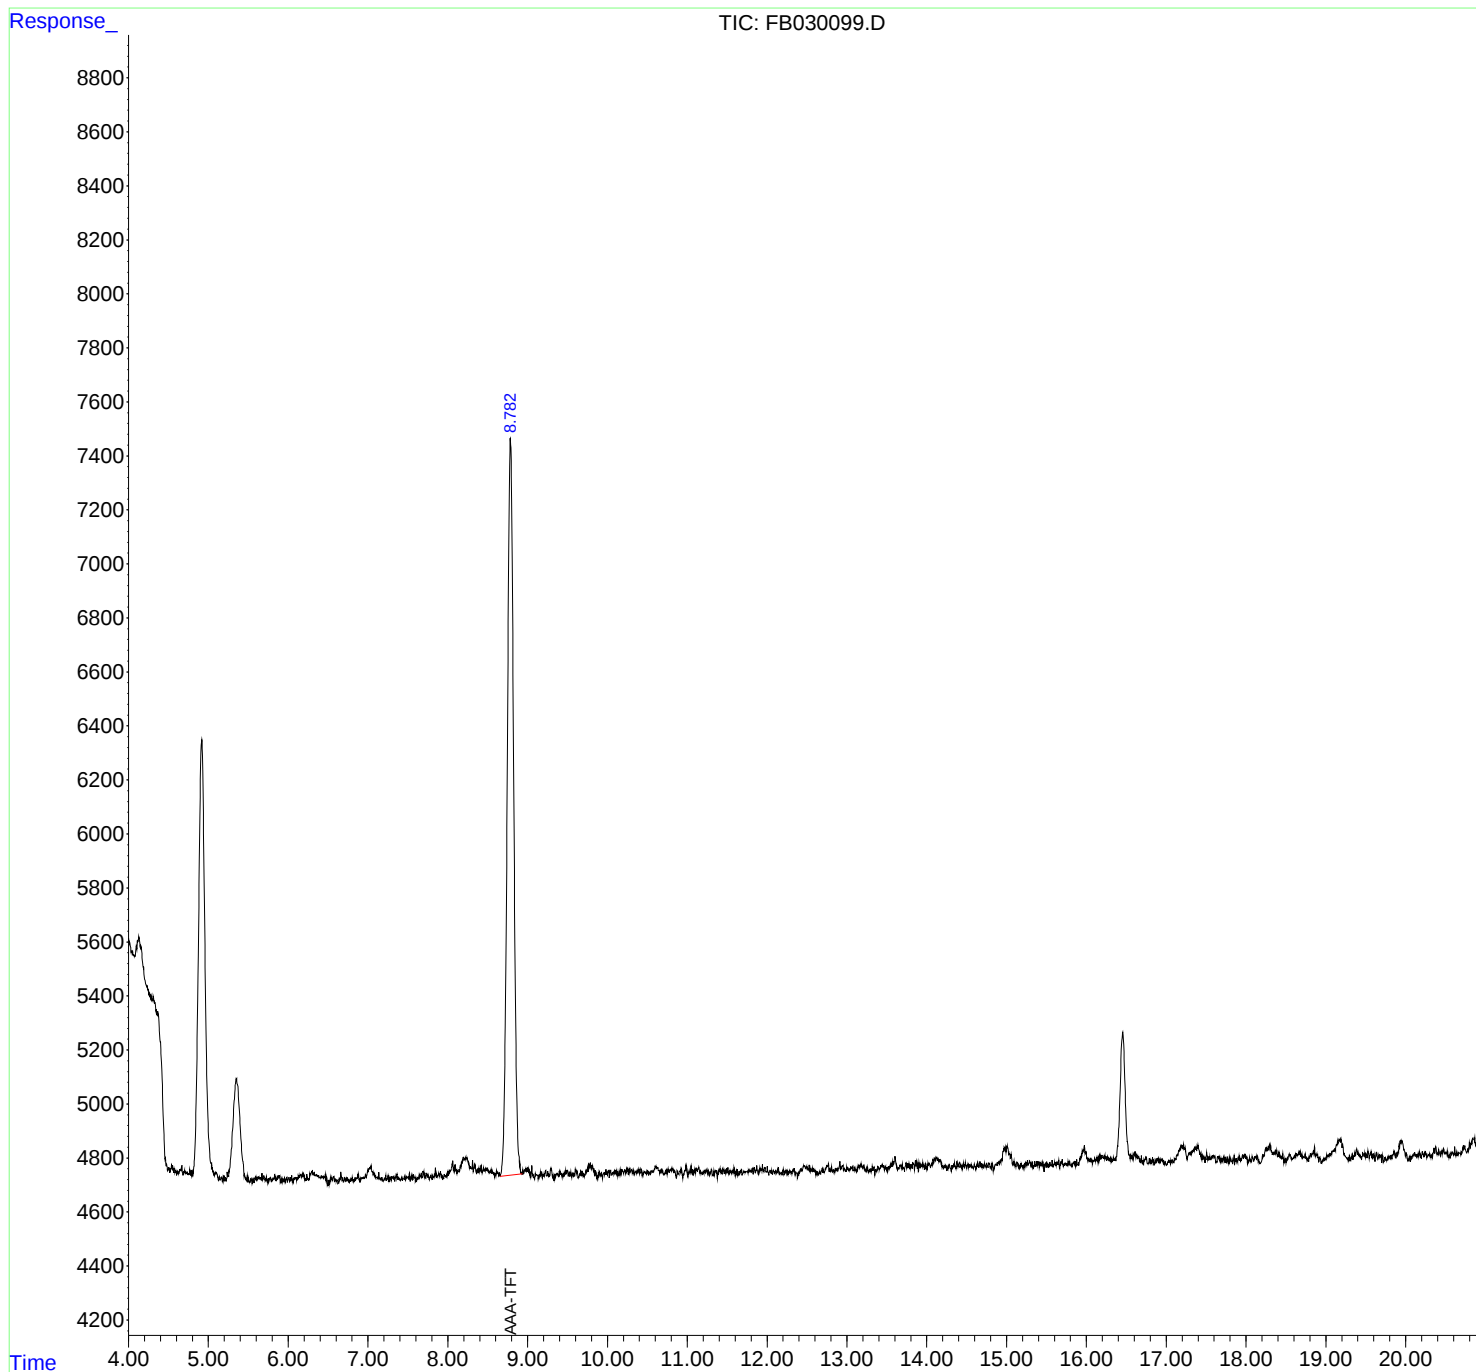

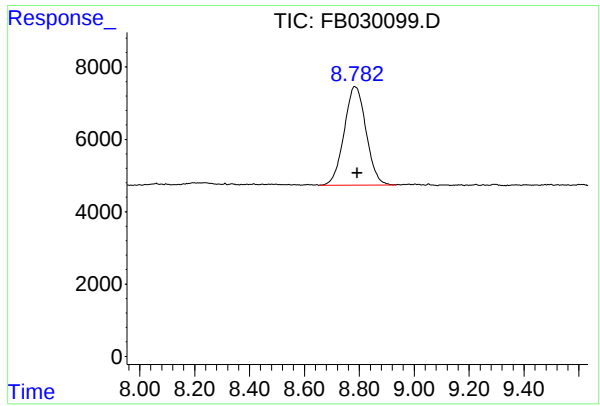

#5 AAA-TFT

R.T.: 8.784 min  
Delta R.T.: -0.009 min  
Response: 150704  
Conc: 10.83 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
WC-SCAN-03-G