

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
 Data File : FB030113.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2023 19:32
 Operator : YP/AJ
 Sample : BSF0621S4
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0621S4

Integration File: Calibration.e
 Quant Time: Jun 22 23:37:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
 Quant Title :
 QLast Update : Mon Jun 05 04:33:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	279122	20.063 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	546485	28.924 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	581421	30.813 ng/ml
3) t n-Heptane	7.748	188096	9.717 ng/ml
4) t Benzene	7.884	228608	10.213 ng/ml
6) t Toluene	10.616	649362	29.920 ng/ml
7) t Ethylbenzene	13.052	205012	10.139 ng/ml
8) t m-Xylene	13.185	407703	20.273 ng/ml
9) t O-Xylene	13.912	394532	20.242 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	375471	20.046 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062123\
Data File : FB030113.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2023 19:32
Operator : YP/AJ
Sample : BSF0621S4
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0621S4

Integration File: Calibration.e
Quant Time: Jun 22 23:37:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060323.M
Quant Title :
QLast Update : Mon Jun 05 04:33:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

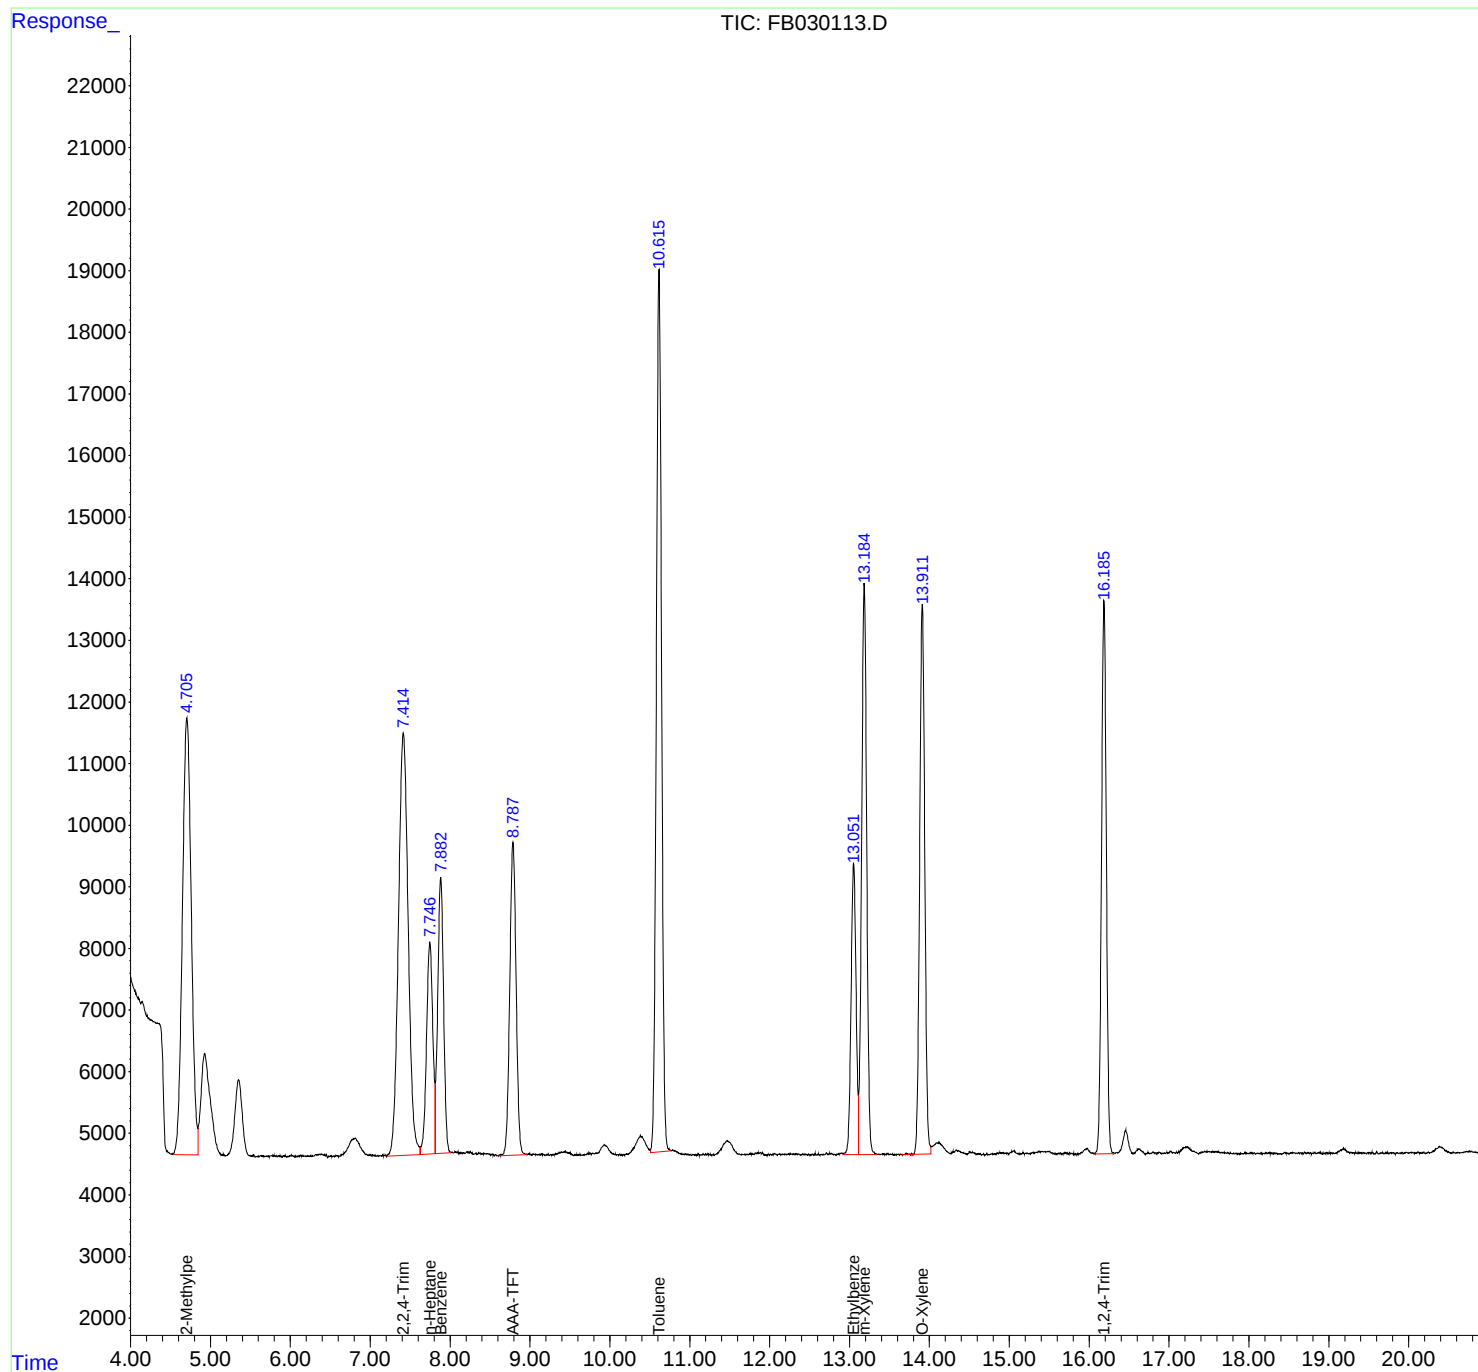


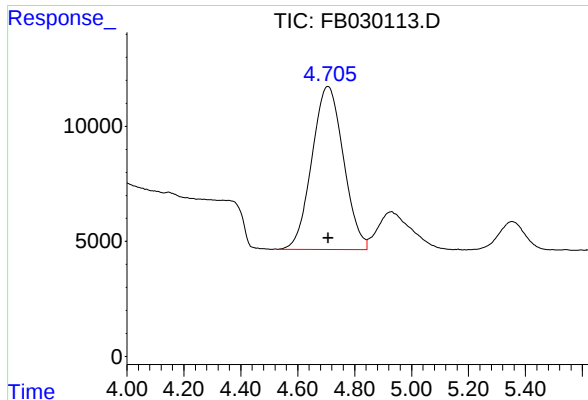

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.002 min
Response: 546485
Conc: 28.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S4

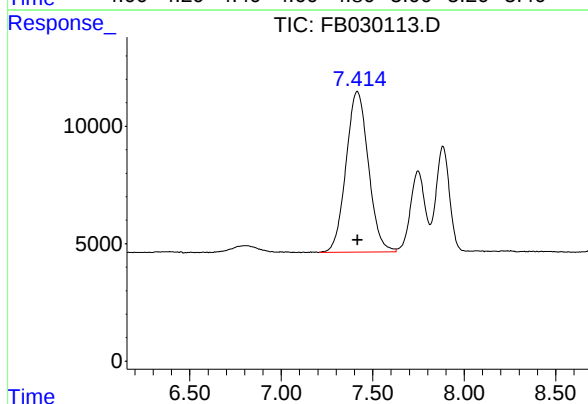


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 581421
Conc: 30.81 ng/ml

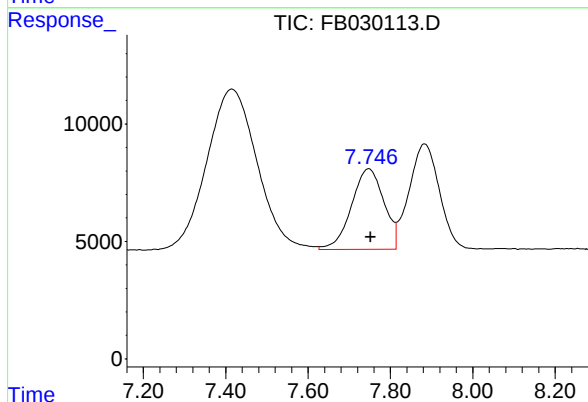


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.004 min
Response: 188096
Conc: 9.72 ng/ml

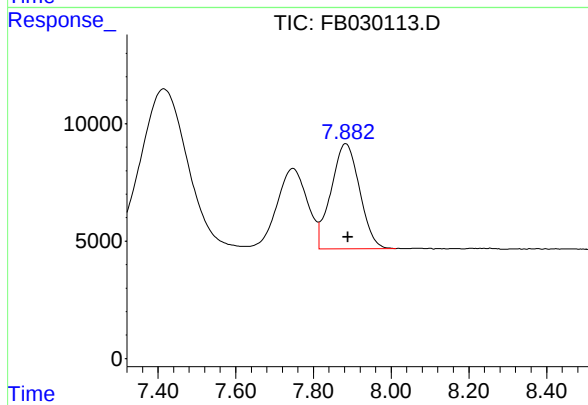

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.005 min
Response: 228608
Conc: 10.21 ng/ml

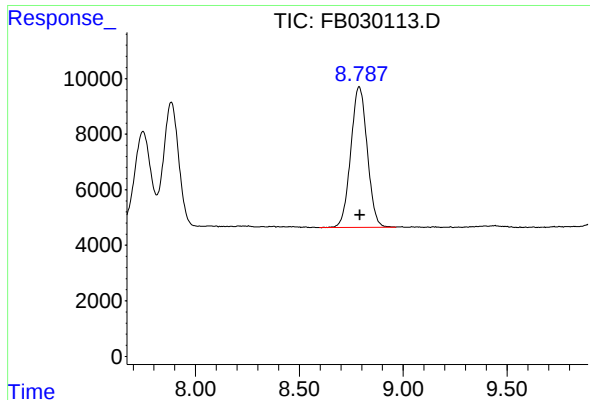

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.005 min
Response: 279122
Conc: 20.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S4

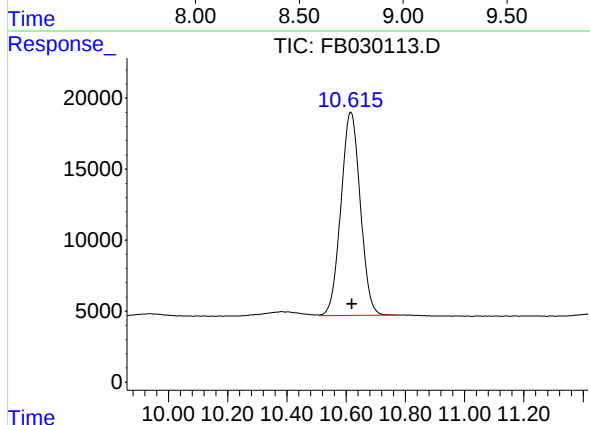


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 649362
Conc: 29.92 ng/ml

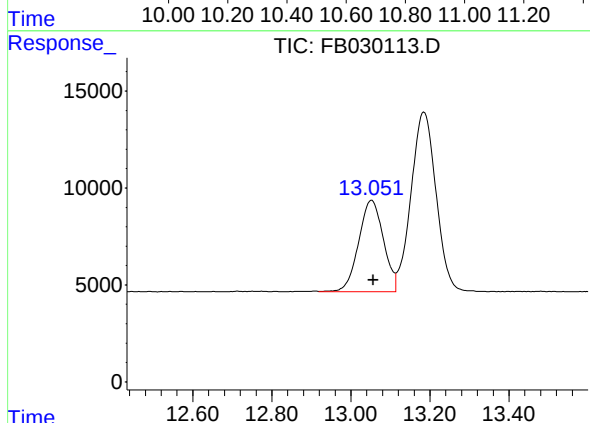


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.004 min
Response: 205012
Conc: 10.14 ng/ml

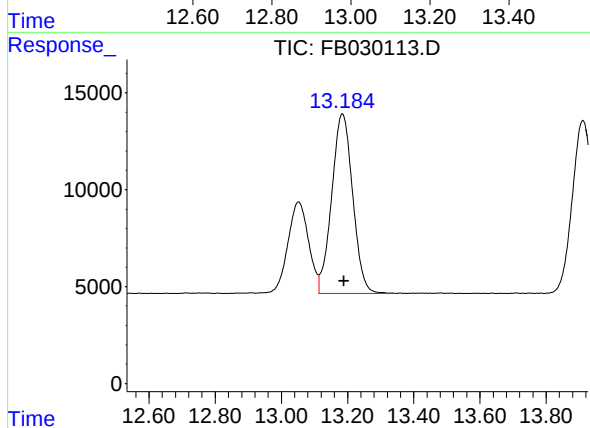

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.004 min
Response: 407703
Conc: 20.27 ng/ml

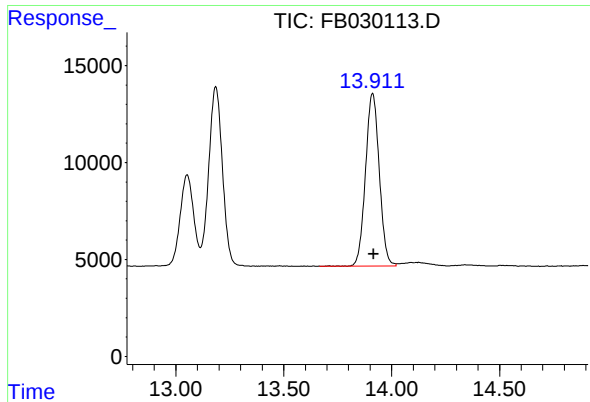

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.004 min
Response: 394532
Conc: 20.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0621S4

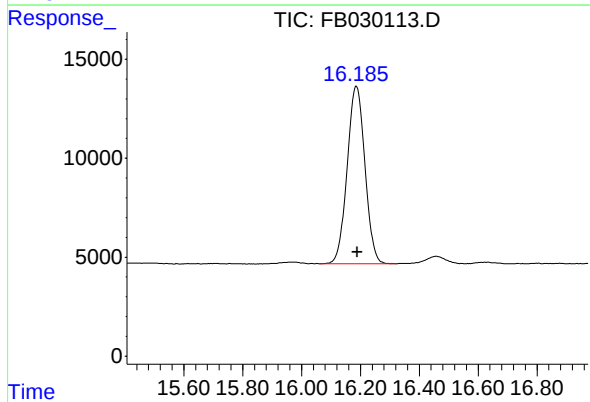

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: -0.004 min
Response: 375471
Conc: 20.05 ng/ml