

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
Data File : FB027496.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2022 17:42
Operator : AJ/MA
Sample : N3431-11MSD
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 23 07:27:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
1) t 2-Methylpentane	4.711	187673	11.140 ng/ml
2) t 2,2,4-Trimethylpentane	7.468	672884	38.323 ng/ml
3) t n-Heptane	7.818	1885569	107.631 ng/ml
4) t Benzene	7.818	1885569	92.464 ng/ml
6) t Toluene	10.618	339845	17.552 ng/ml
7) t Ethylbenzene	13.023	8796260	485.729 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
Data File : FB027496.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2022 17:42
Operator : AJ/MA
Sample : N3431-11MSD
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 23 07:27:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

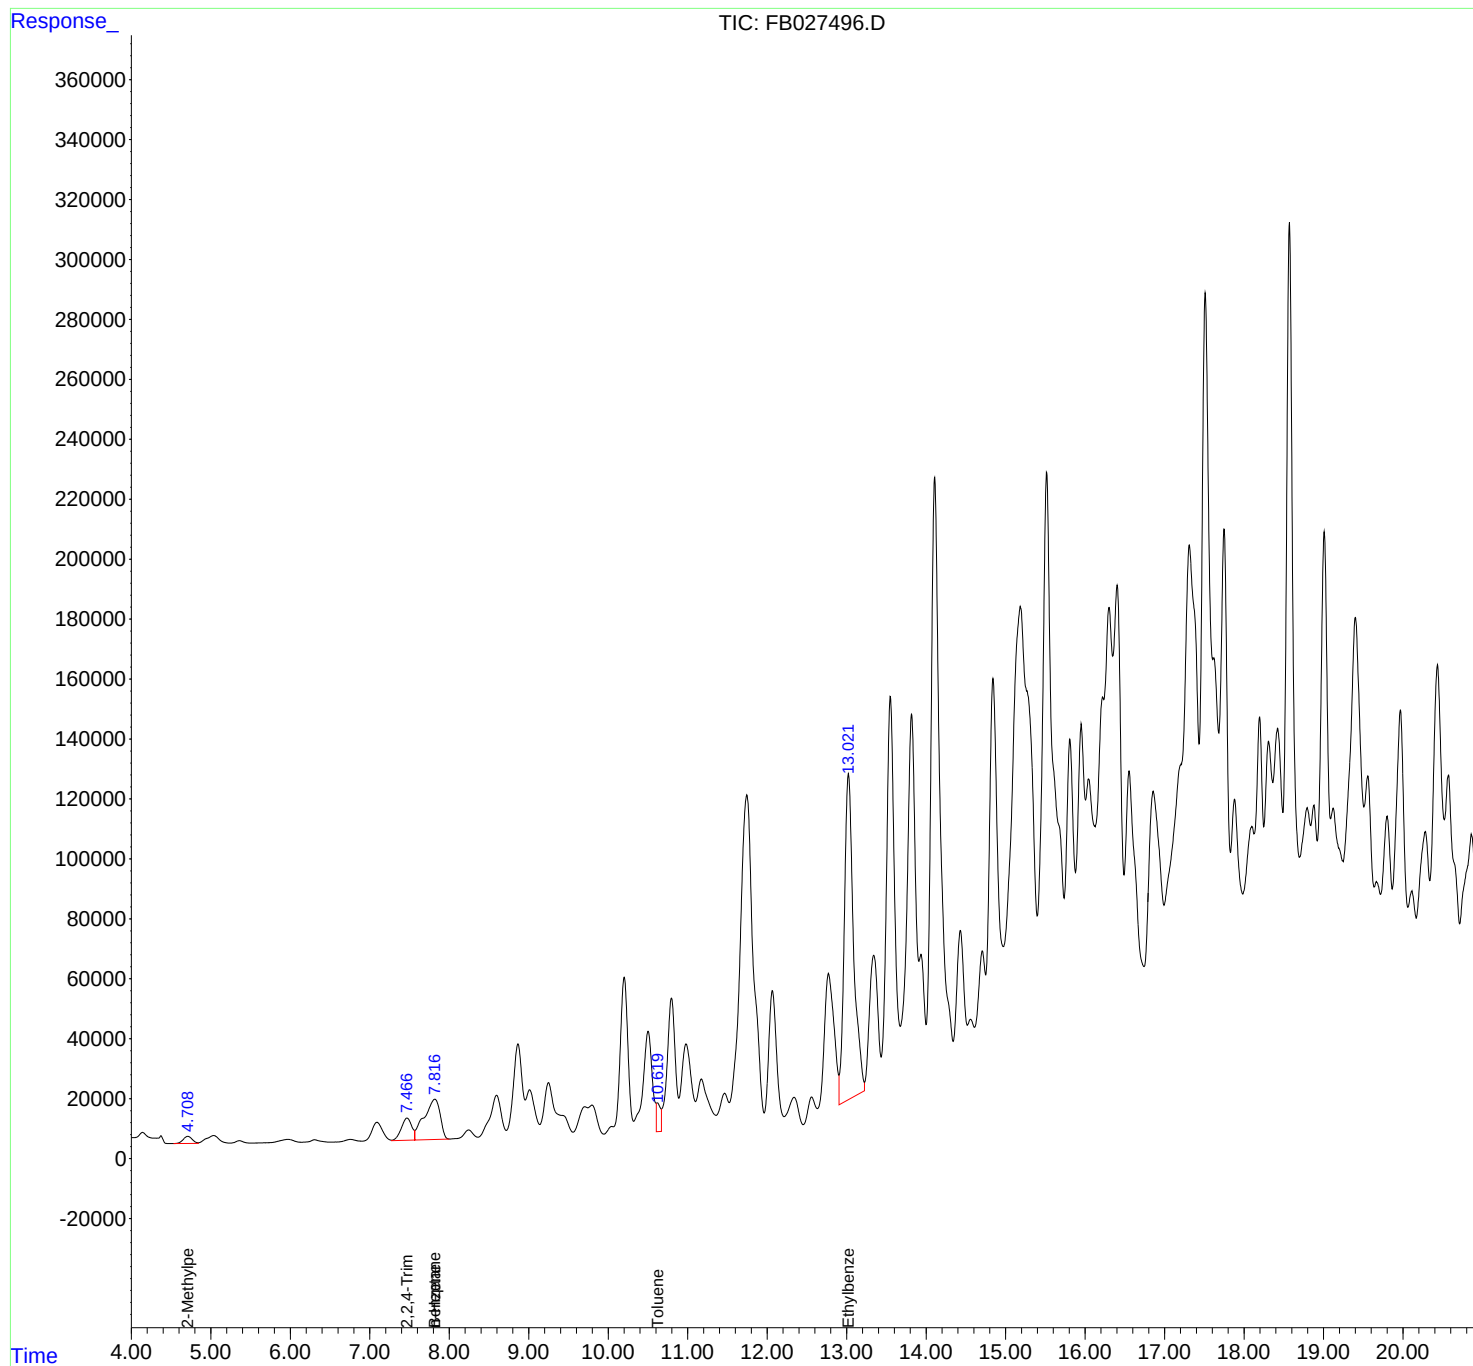


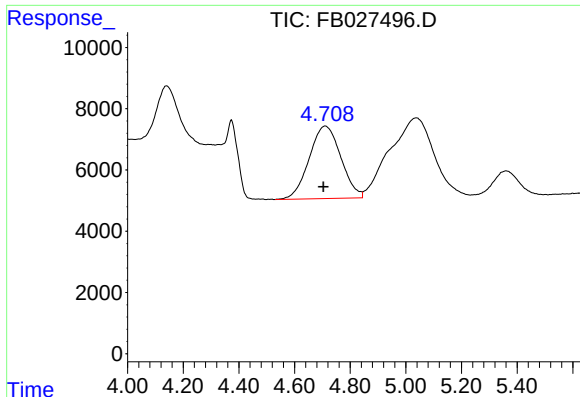

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.007 min
Response: 187673
Conc: 11.14 ng/ml

Instrument :
FID_B
ClientSampleId :

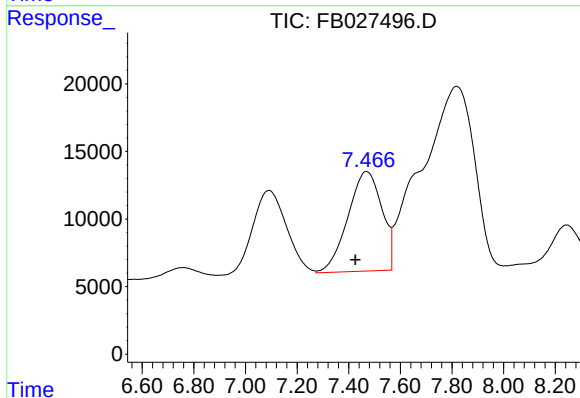


#2 2,2,4-Trimethylpentane

R.T.: 7.468 min
Delta R.T.: 0.042 min
Response: 672884
Conc: 38.32 ng/ml

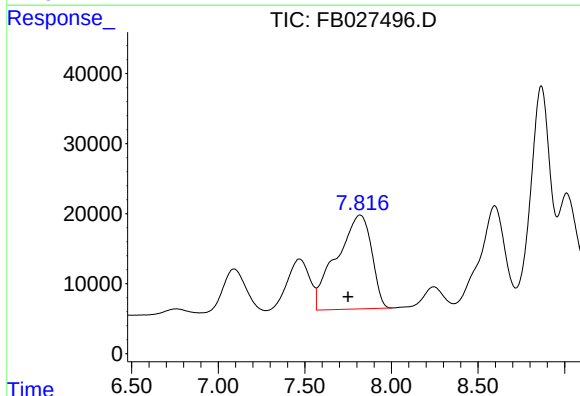


#3 n-Heptane

R.T.: 7.818 min
Delta R.T.: 0.068 min
Response: 1885569
Conc: 107.63 ng/ml

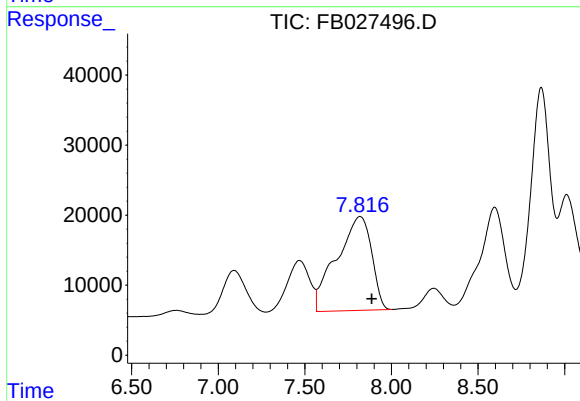

#4 Benzene


R.T.: 7.818 min
Delta R.T.: -0.068 min
Response: 1885569
Conc: 92.46 ng/ml

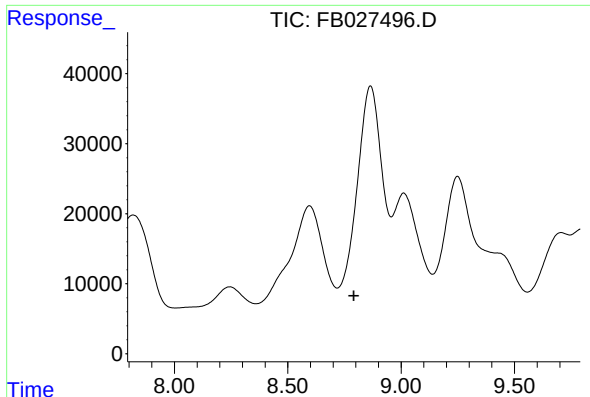

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :

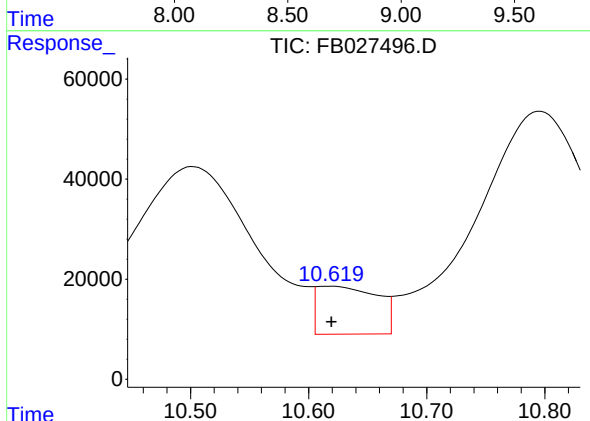

#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.002 min
Response: 339845
Conc: 17.55 ng/ml

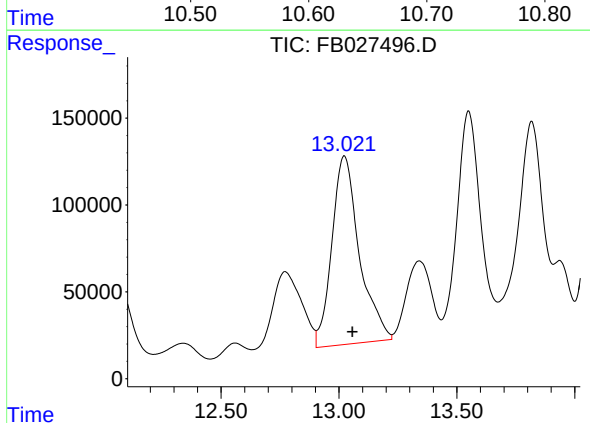

#7 Ethylbenzene

R.T.: 13.023 min
Delta R.T.: -0.033 min
Response: 8796260
Conc: 485.73 ng/ml