

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB062222\  
 Data File : FB027499.D  
 Signal(s) : FID2B.CH  
 Acq On : 22 Jun 2022 19:32  
 Operator : AJ/MA  
 Sample : N3431-23  
 Misc : 5.00G/5.00 ML DI WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Jun 23 07:29:10 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB061022.M  
 Quant Title :  
 QLast Update : Mon Jun 13 09:22:45 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

#### System Monitoring Compounds

##### Target Compounds

|      |                 |        |                           |
|------|-----------------|--------|---------------------------|
| 1) t | 2-Methylpentane | 4.732  | 41276895 2450.064 ng/ml   |
| 4) t | Benzene         | 7.854  | 684746824 33578.395 ng/ml |
| 6) t | Toluene         | 10.600 | 626579613 32361.222 ng/ml |
| 8) t | m-Xylene        | 13.129 | 774361528 43439.803 ng/ml |
| 9) t | O-Xylene        | 13.944 | 415294505 23900.488 ng/ml |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB062222\  
Data File : FB027499.D  
Signal(s) : FID2B.CH  
Acq On : 22 Jun 2022 19:32  
Operator : AJ/MA  
Sample : N3431-23  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Jun 23 07:29:10 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB061022.M  
Quant Title :  
QLast Update : Mon Jun 13 09:22:45 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

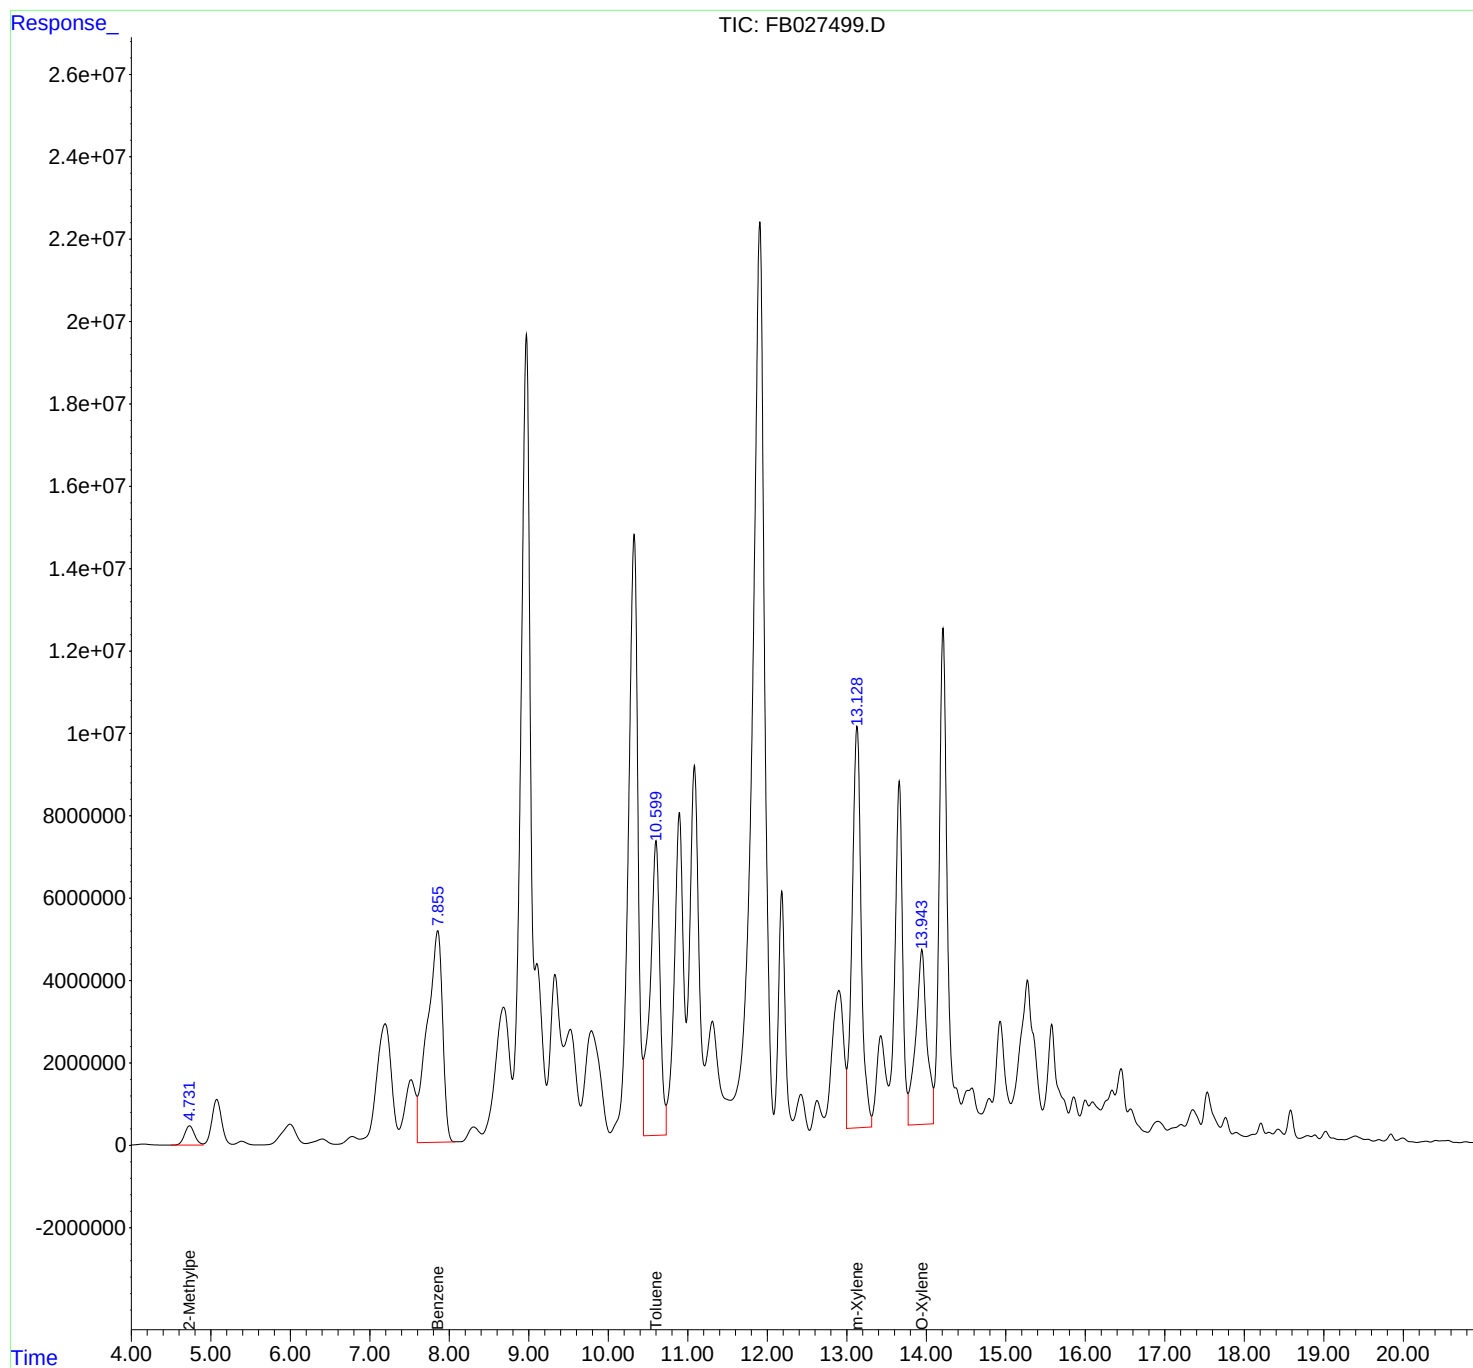


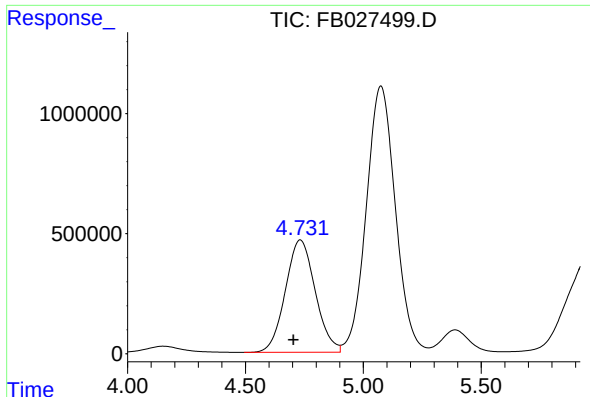

#1 2-Methylpentane


R.T.: 4.732 min  
Delta R.T.: 0.028 min  
Response: 41276895  
Conc: 2450.06 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

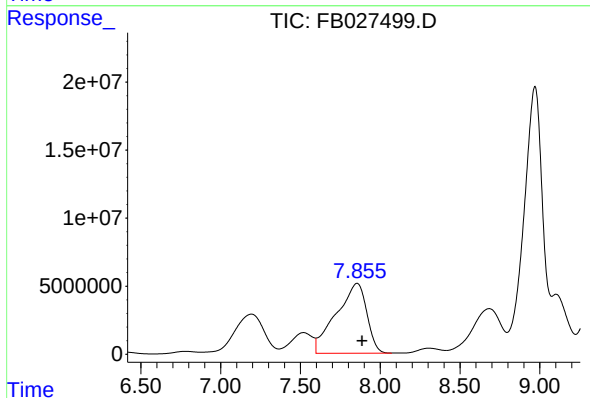


#4 Benzene

R.T.: 7.854 min  
Delta R.T.: -0.032 min  
Response: 684746824  
Conc: 33578.40 ng/ml

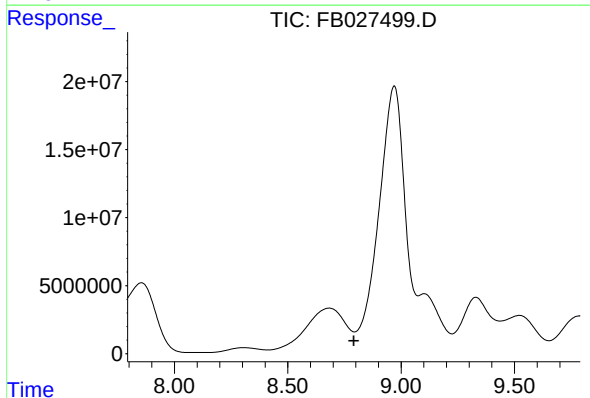


#5 AAA-TFT

R.T.: 0.000 min  
Exp R.T. : 8.791 min  
Response: 0  
Conc: N.D.

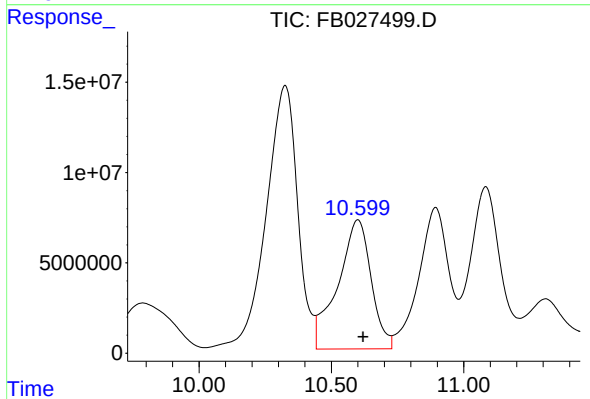

#6 Toluene


R.T.: 10.600 min  
Delta R.T.: -0.020 min  
Response: 626579613  
Conc: 32361.22 ng/ml

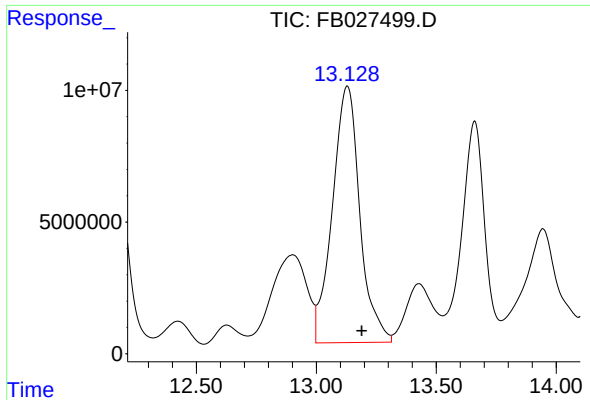

#8 m-Xylene

R.T.: 13.129 min  
Delta R.T.: -0.060 min  
Response: 774361528  
Conc: 43439.80 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

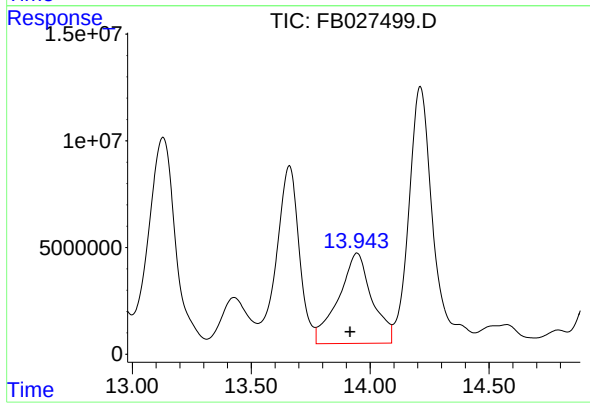

#9 o-Xylene

R.T.: 13.944 min  
Delta R.T.: 0.028 min  
Response: 415294505  
Conc: 23900.49 ng/ml