

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
Data File : FB027504.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2022 23:11
Operator : AJ/MA
Sample : N3431-23
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 23 07:31:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.846	46042	4.105 ng/ml
Target Compounds			
7) t Ethylbenzene	13.111	67181	3.710 ng/ml
8) t m-Xylene	13.227	129163	7.246 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
Data File : FB027504.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2022 23:11
Operator : AJ/MA
Sample : N3431-23
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 23 07:31:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

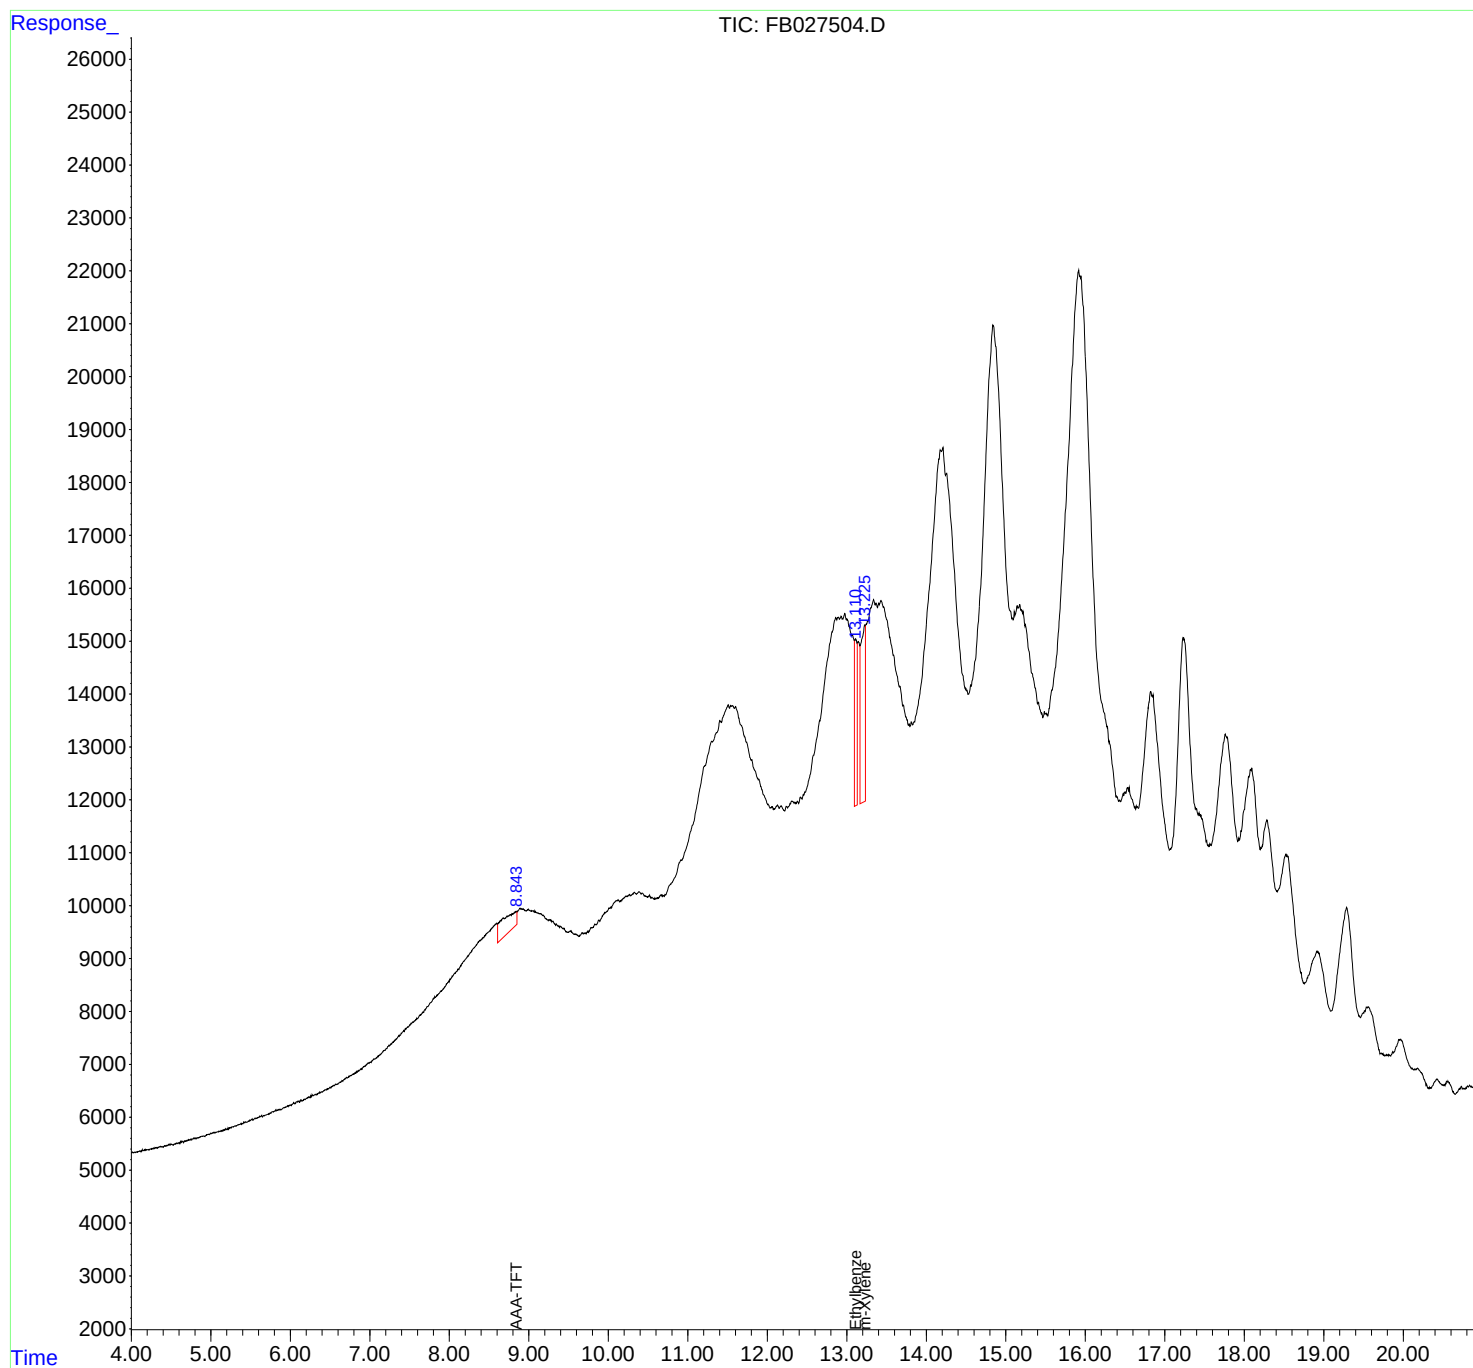


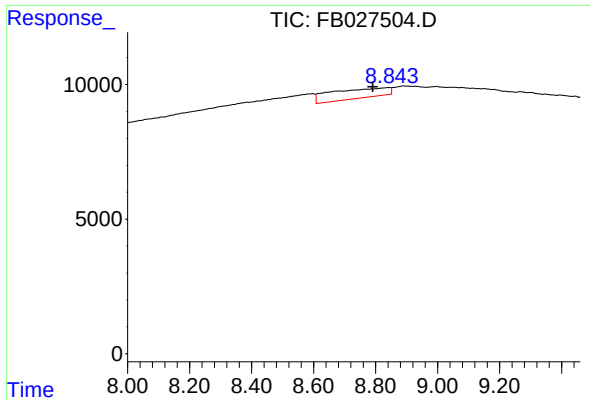

#5 AAA-TFT


R.T.: 8.846 min
Delta R.T.: 0.055 min
Response: 46042
Conc: 4.10 ng/ml

Instrument :
FID_B
ClientSampleId :

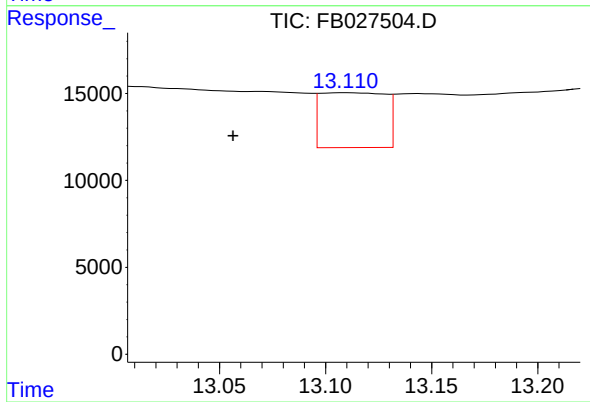

#7 Ethylbenzene

R.T.: 13.111 min
Delta R.T.: 0.055 min
Response: 67181
Conc: 3.71 ng/ml

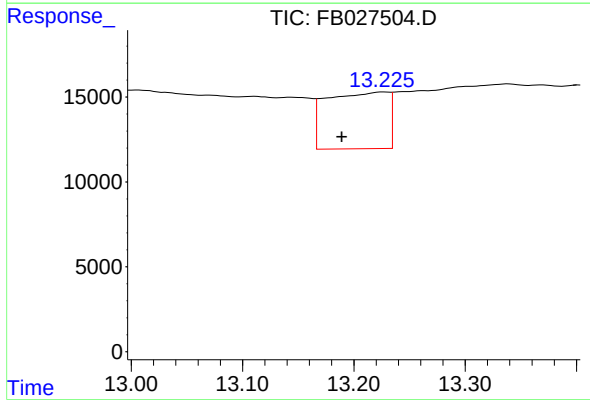

#8 m-Xylene

R.T.: 13.227 min
Delta R.T.: 0.038 min
Response: 129163
Conc: 7.25 ng/ml