

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
 Data File : FB027511.D
 Signal(s) : FID2B.CH
 Acq On : 23 Jun 2022 3:26
 Operator : AJ/MA
 Sample : BSF0622S3
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 23 07:34:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	276089	24.614 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	430421	25.548 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	471502	26.853 ng/ml
3) t n-Heptane	7.752	143438	8.188 ng/ml
4) t Benzene	7.888	177884	8.723 ng/ml
6) t Toluene	10.621	489947	25.304 ng/ml
7) t Ethylbenzene	13.056	605041	33.410 ng/ml
8) t m-Xylene	13.190	436187	24.469 ng/ml
9) t O-Xylene	13.917	436475	25.119 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	419861	24.441 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
Data File : FB027511.D
Signal(s) : FID2B.CH
Acq On : 23 Jun 2022 3:26
Operator : AJ/MA
Sample : BSF0622S3
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 23 07:34:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

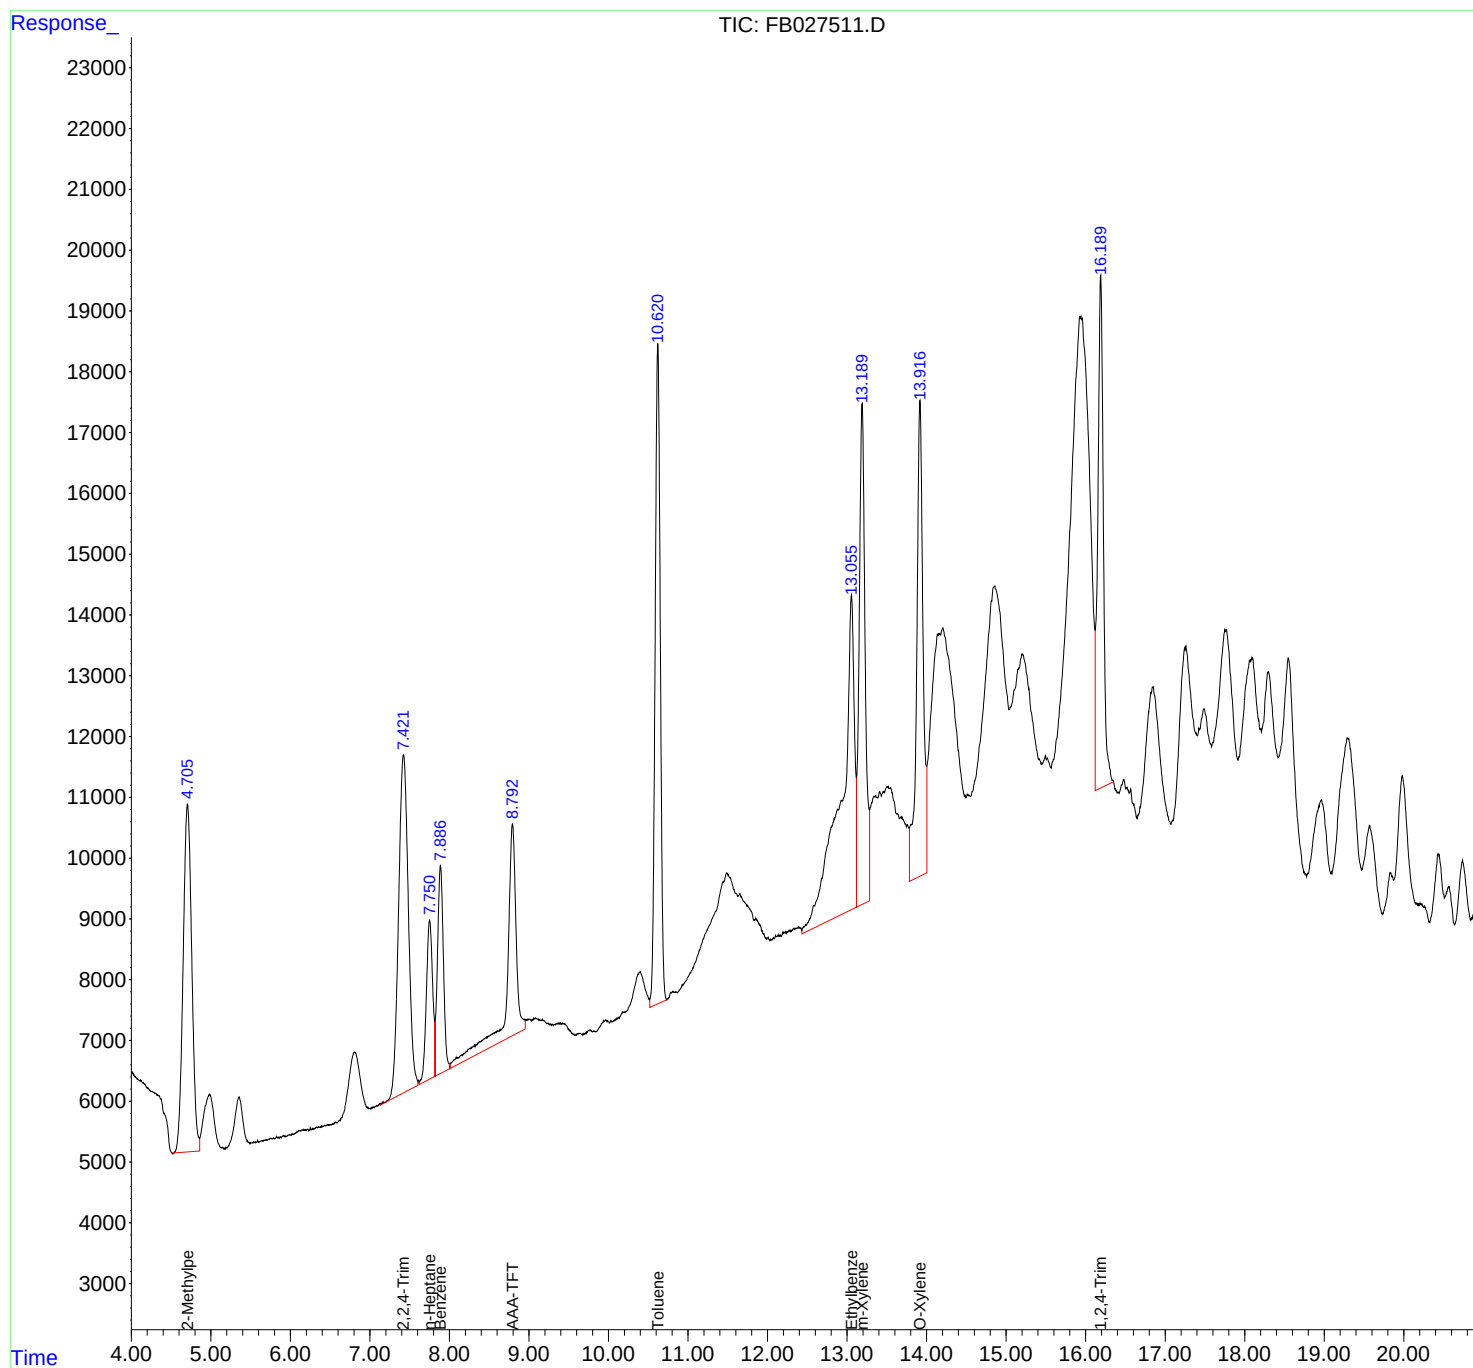


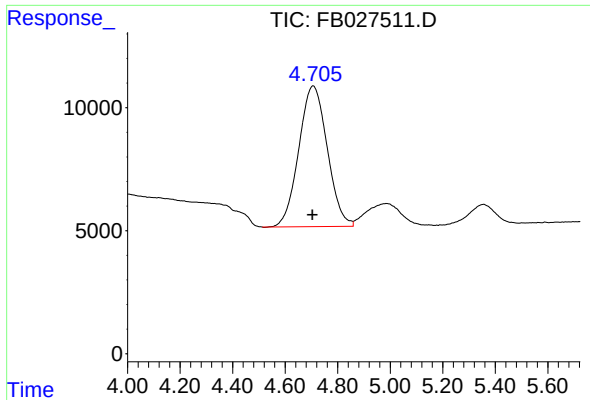

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.003 min
Response: 430421
Conc: 25.55 ng/ml

Instrument :
FID_B
ClientSampleId :

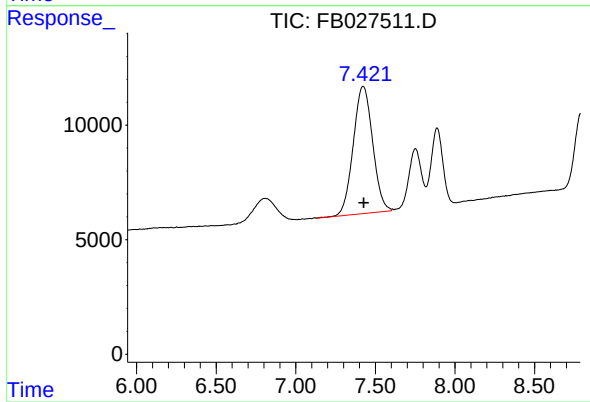


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: -0.004 min
Response: 471502
Conc: 26.85 ng/ml

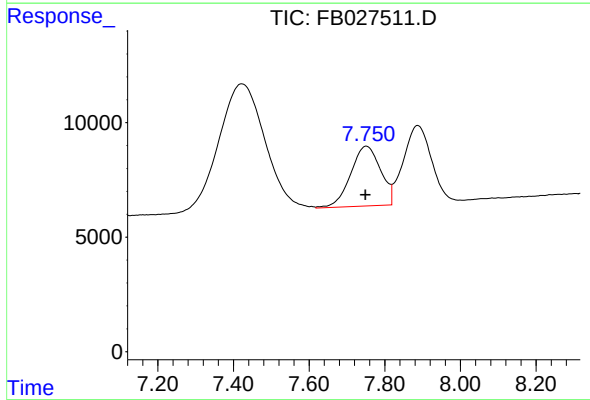


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.002 min
Response: 143438
Conc: 8.19 ng/ml

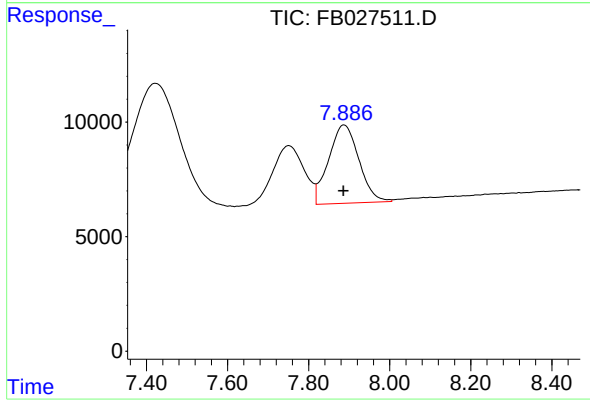

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 177884
Conc: 8.72 ng/ml

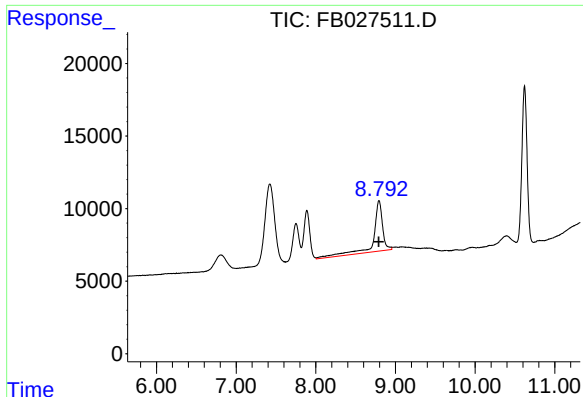

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 276089
Conc: 24.61 ng/ml

Instrument :
FID_B
ClientSampleId :

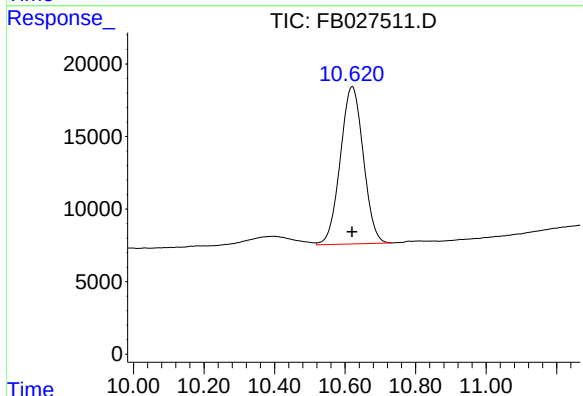


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 489947
Conc: 25.30 ng/ml

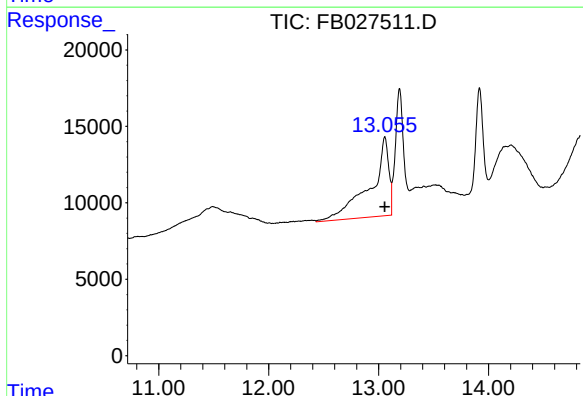


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 605041
Conc: 33.41 ng/ml

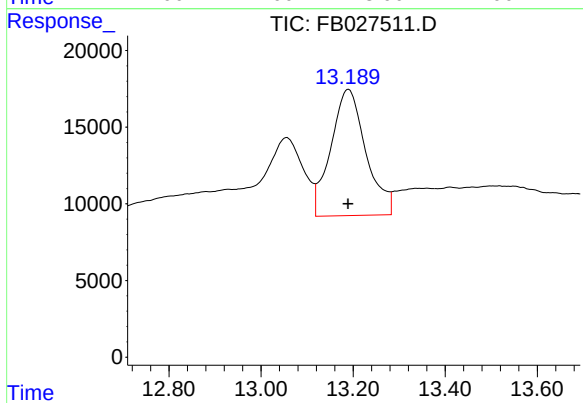

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 436187
Conc: 24.47 ng/ml

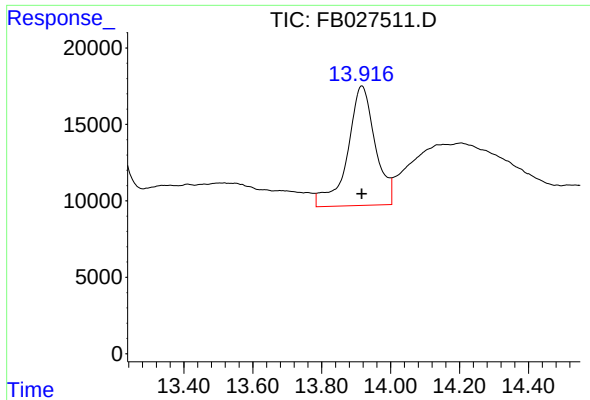

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.001 min
Response: 436475
Conc: 25.12 ng/ml

Instrument :
FID_B
ClientSampleId :

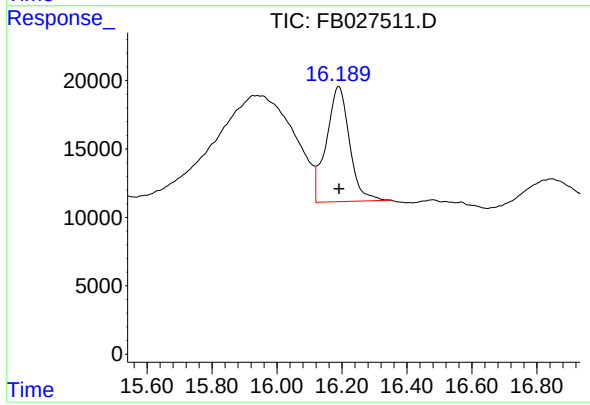

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.001 min
Response: 419861
Conc: 24.44 ng/ml