

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
Data File : FB027491.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2022 14:35
Operator : AJ/MA
Sample : VBF0622S2 50X
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0622S2

Integration File: Calibration.e
Quant Time: Jun 23 07:26:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	185234	16.514 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
Data File : FB027491.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2022 14:35
Operator : AJ/MA
Sample : VBF0622S2 50X
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0622S2

Integration File: Calibration.e
Quant Time: Jun 23 07:26:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

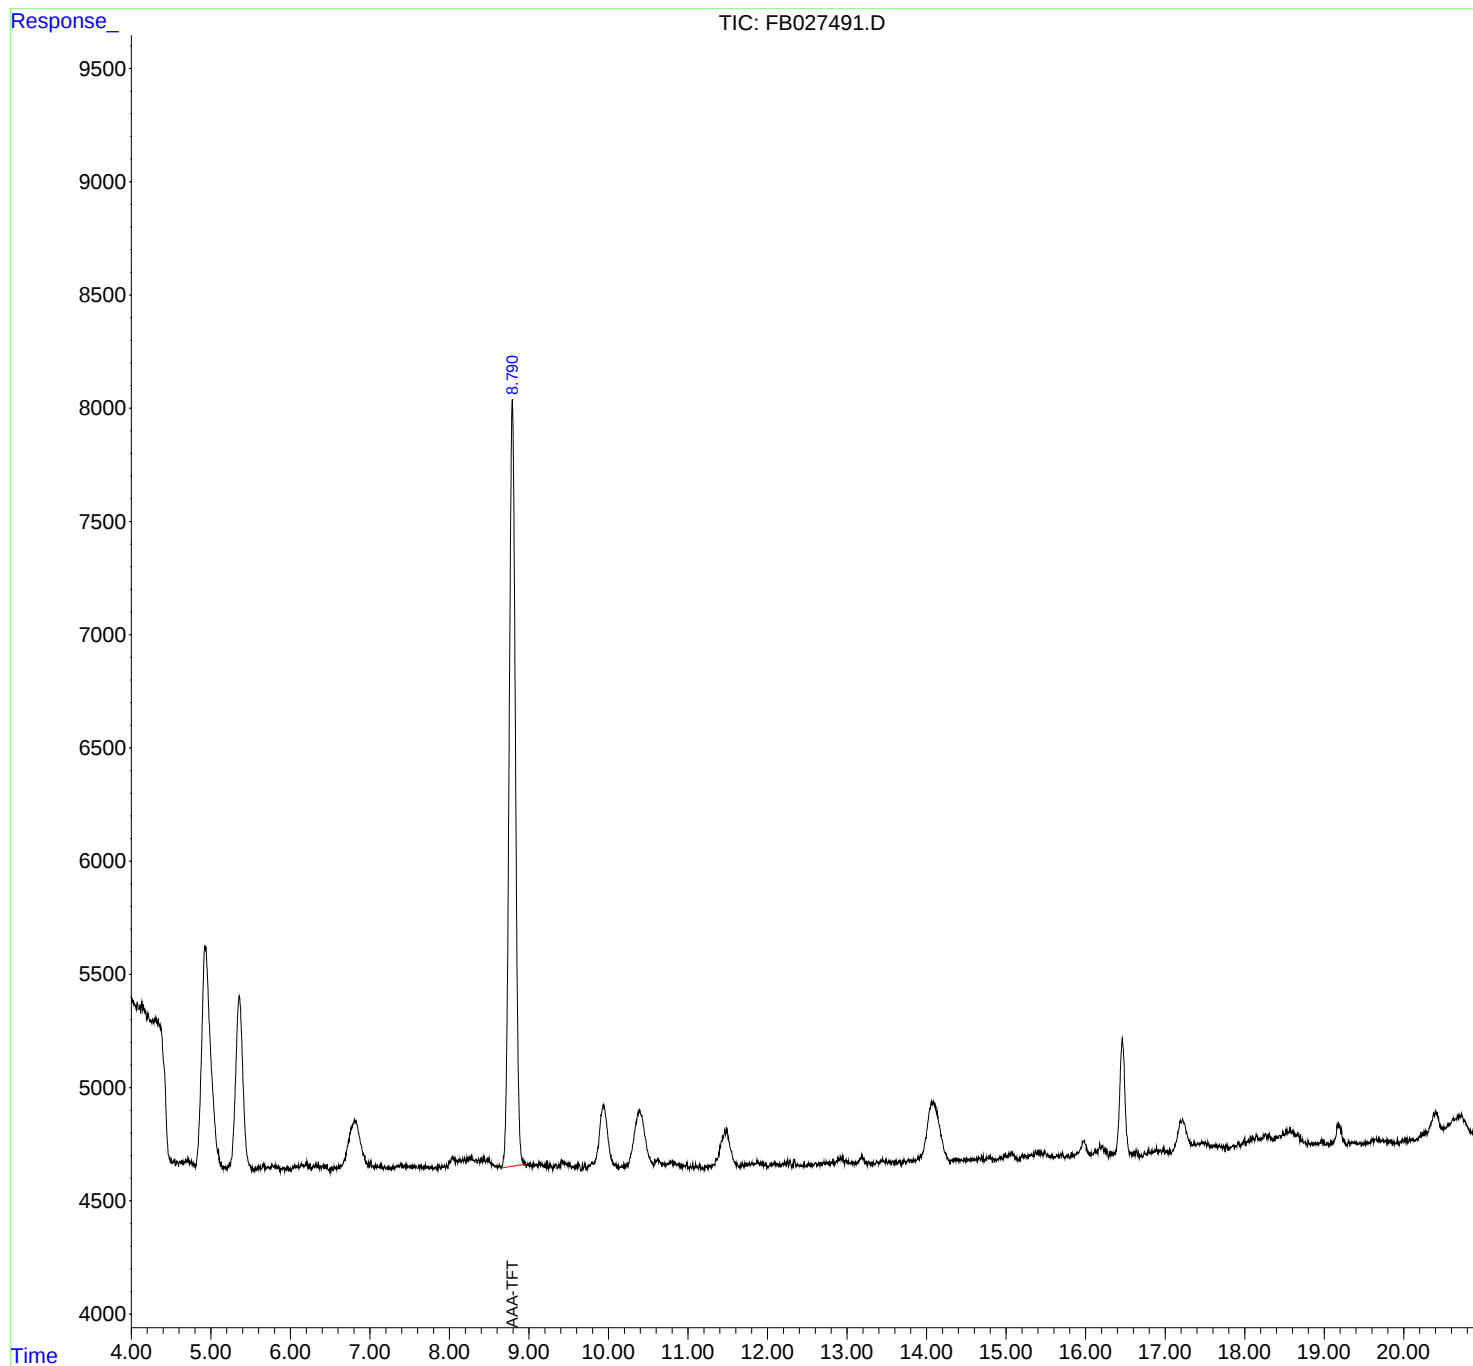

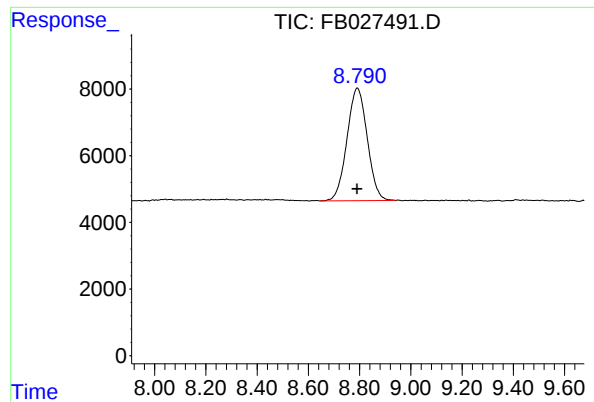

#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 185234
Conc: 16.51 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0622S2