

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
 Data File : FB027492.D
 Signal(s) : FID2B.CH
 Acq On : 22 Jun 2022 15:11
 Operator : AJ/MA
 Sample : BSF0622S1
 Misc : 5.03G/5.00 ML MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0622S1

Integration File: Calibration.e
 Quant Time: Jun 23 07:26:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	219283	19.550 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	424809	25.215 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	463567	26.401 ng/ml
3) t n-Heptane	7.751	144924	8.273 ng/ml
4) t Benzene	7.886	177828	8.720 ng/ml
6) t Toluene	10.620	509977	26.339 ng/ml
7) t Ethylbenzene	13.057	160045	8.838 ng/ml
8) t m-Xylene	13.190	320188	17.962 ng/ml
9) t O-Xylene	13.917	316918	18.239 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	319802	18.617 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062222\
Data File : FB027492.D
Signal(s) : FID2B.CH
Acq On : 22 Jun 2022 15:11
Operator : AJ/MA
Sample : BSF0622S1
Misc : 5.03G/5.00 ML MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0622S1

Integration File: Calibration.e
Quant Time: Jun 23 07:26:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

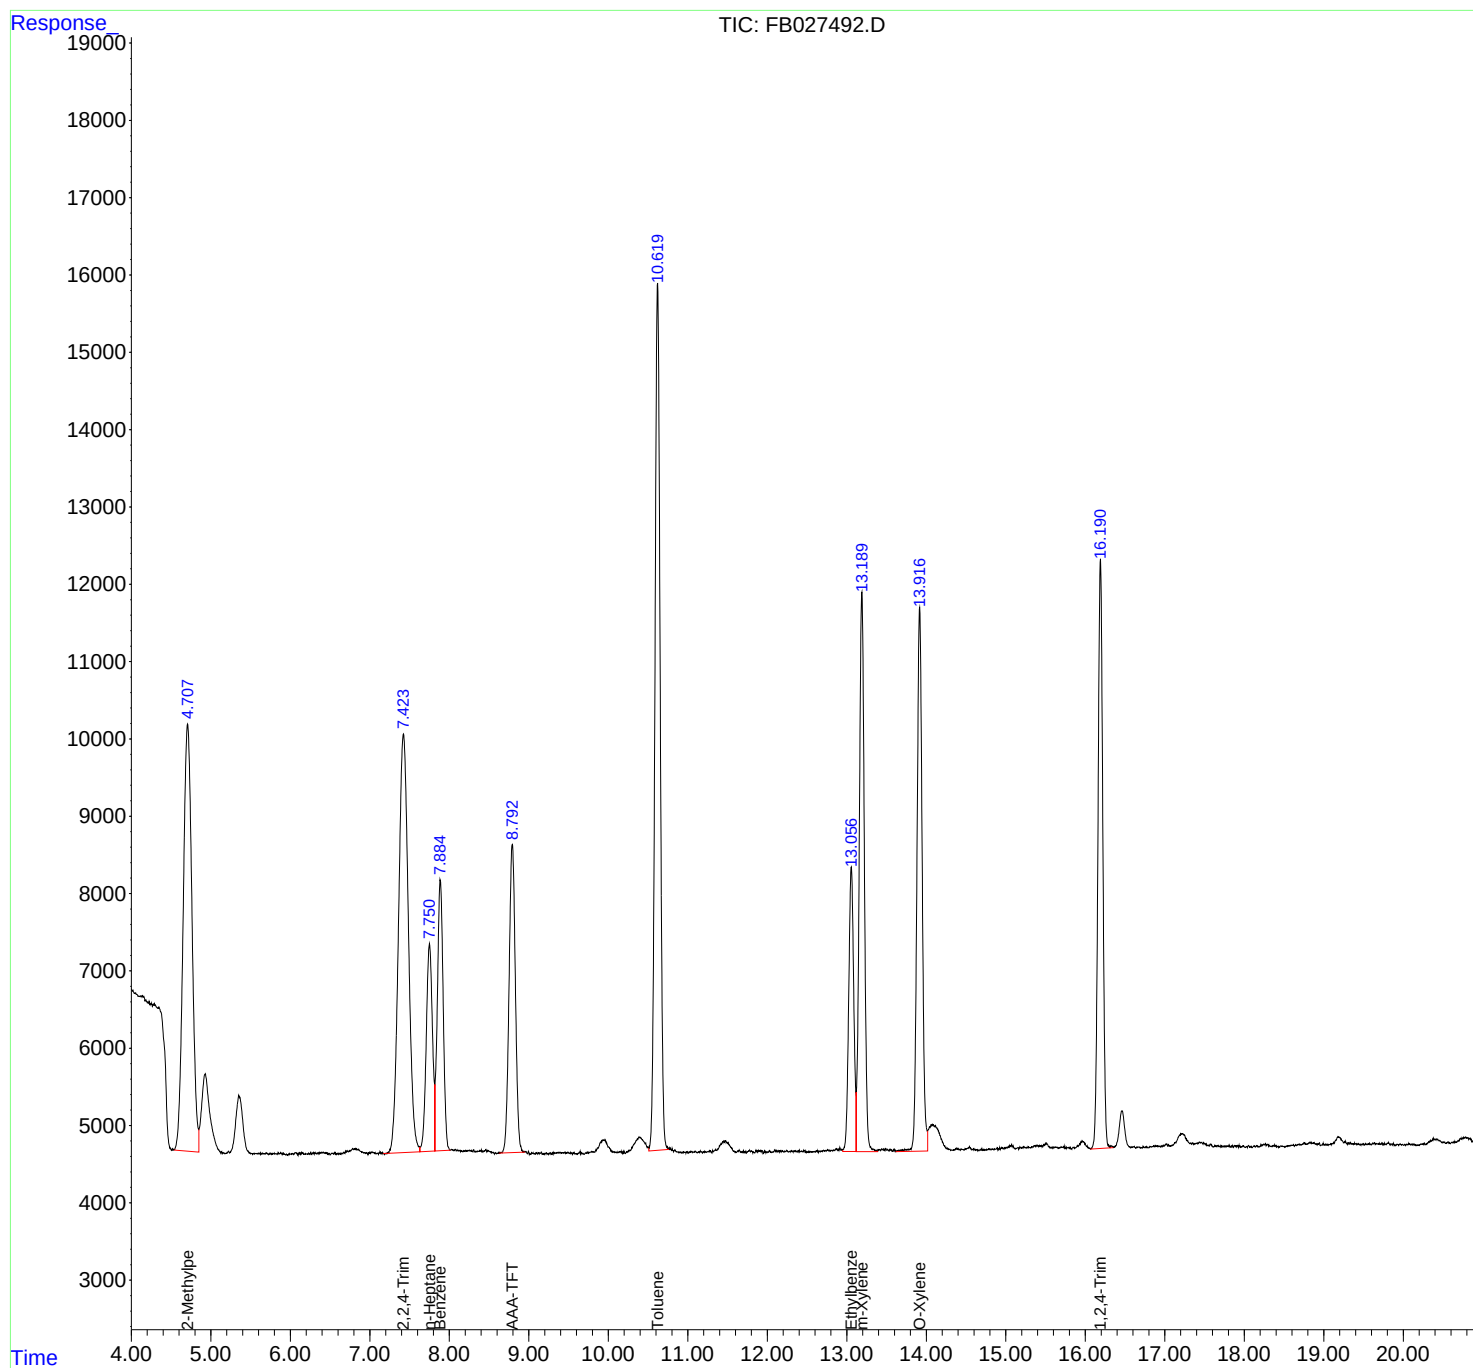


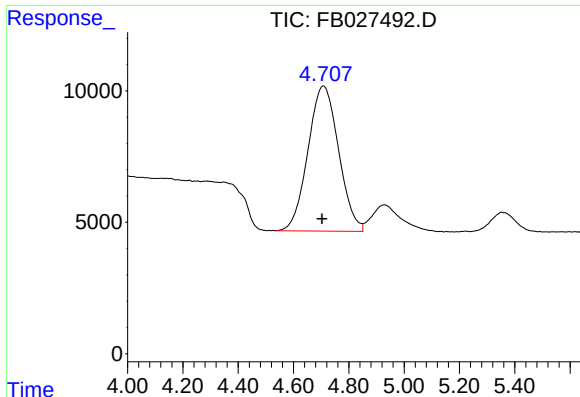

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.005 min
Response: 424809
Conc: 25.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0622S1

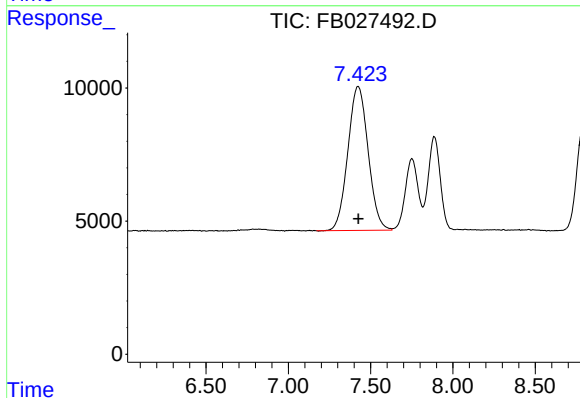


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.002 min
Response: 463567
Conc: 26.40 ng/ml

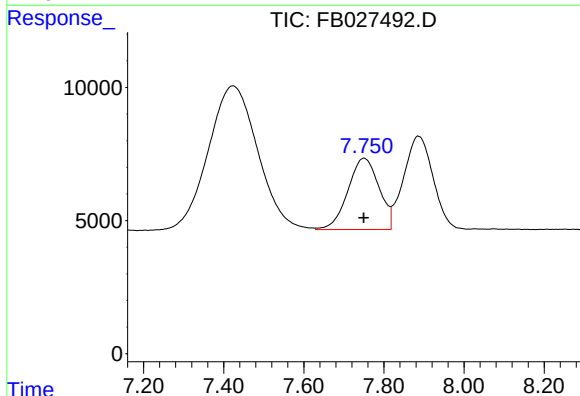


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.002 min
Response: 144924
Conc: 8.27 ng/ml

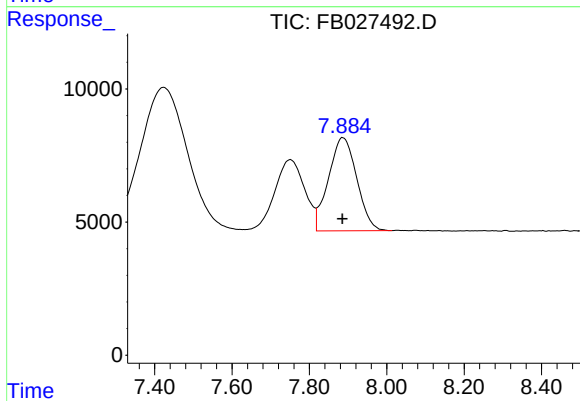

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 177828
Conc: 8.72 ng/ml

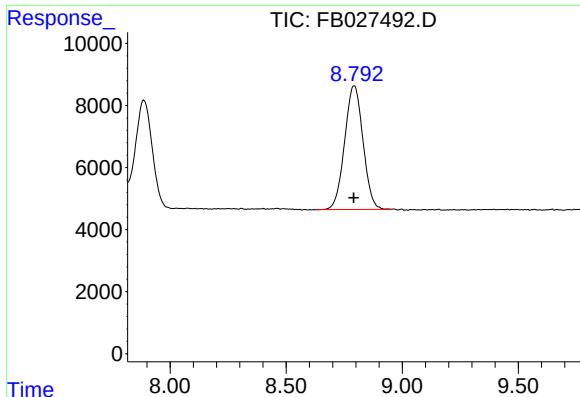

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 219283
Conc: 19.55 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0622S1

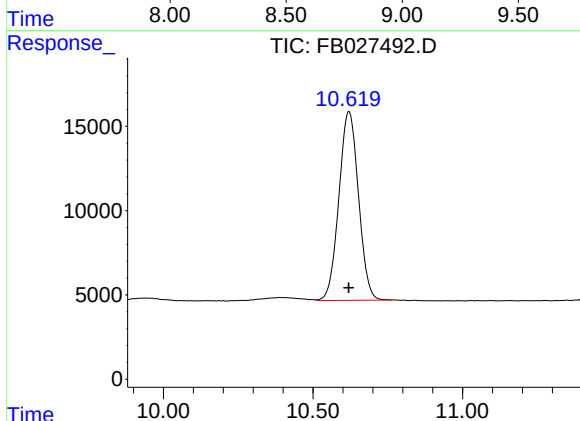


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.001 min
Response: 509977
Conc: 26.34 ng/ml

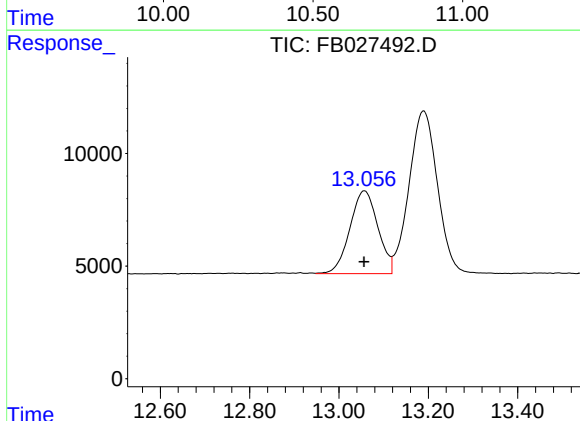


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.001 min
Response: 160045
Conc: 8.84 ng/ml

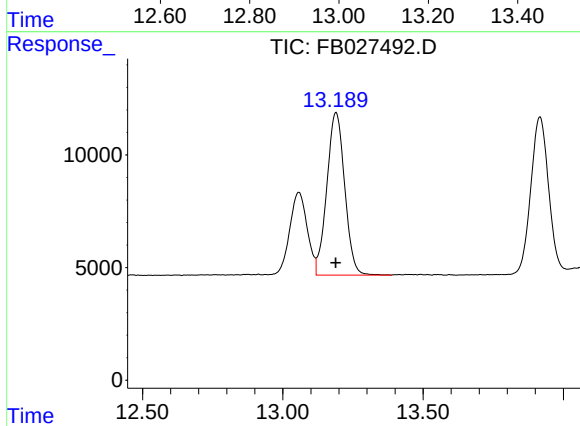

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 320188
Conc: 17.96 ng/ml

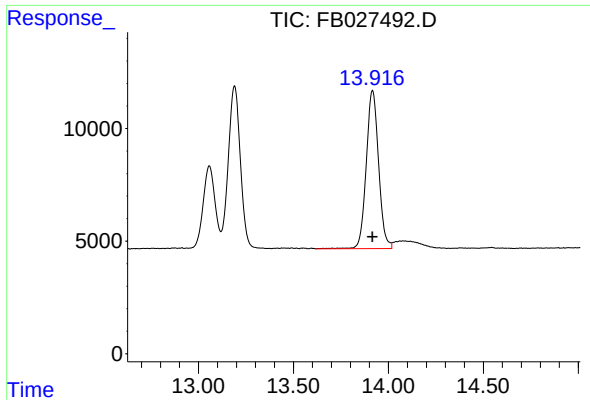

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 316918
Conc: 18.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0622S1

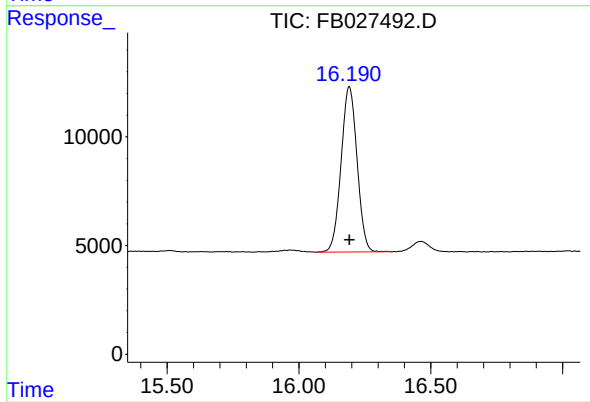

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 319802
Conc: 18.62 ng/ml