

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB062222\  
 Data File : FB027503.D  
 Signal(s) : FID2B.CH  
 Acq On : 22 Jun 2022 22:35  
 Operator : AJ/MA  
 Sample : N3431-17  
 Misc : 5.03G/5.00 ML DI WATER  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :  
 WC-14B-2-4-GR

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 06/23/2022  
 Supervised By :Ankita Jodhani 06/23/2022

Integration File: Calibration.e  
 Quant Time: Jun 23 07:30:51 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB061022.M  
 Quant Title :  
 QLast Update : Mon Jun 13 09:22:45 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units     |
|-----------------------------|-------|----------|----------------|
| -----                       |       |          |                |
| System Monitoring Compounds |       |          |                |
| 5) s AAA-TFT                | 8.871 | 8404153  | 749.255 ng/mlm |
| Target Compounds            |       |          |                |
| -----                       |       |          |                |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB062222\  
Data File : FB027503.D  
Signal(s) : FID2B.CH  
Acq On : 22 Jun 2022 22:35  
Operator : AJ/MA  
Sample : N3431-17  
Misc : 5.03G/5.00 ML DI WATER  
ALS Vial : 16 Sample Multiplier: 1


Instrument :  
FID\_B  
ClientSampleId :  
WC-14B-2-4-GR


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/23/2022  
Supervised By :Ankita Jodhani 06/23/2022

Integration File: Calibration.e  
Quant Time: Jun 23 07:30:51 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB061022.M  
Quant Title :  
QLast Update : Mon Jun 13 09:22:45 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

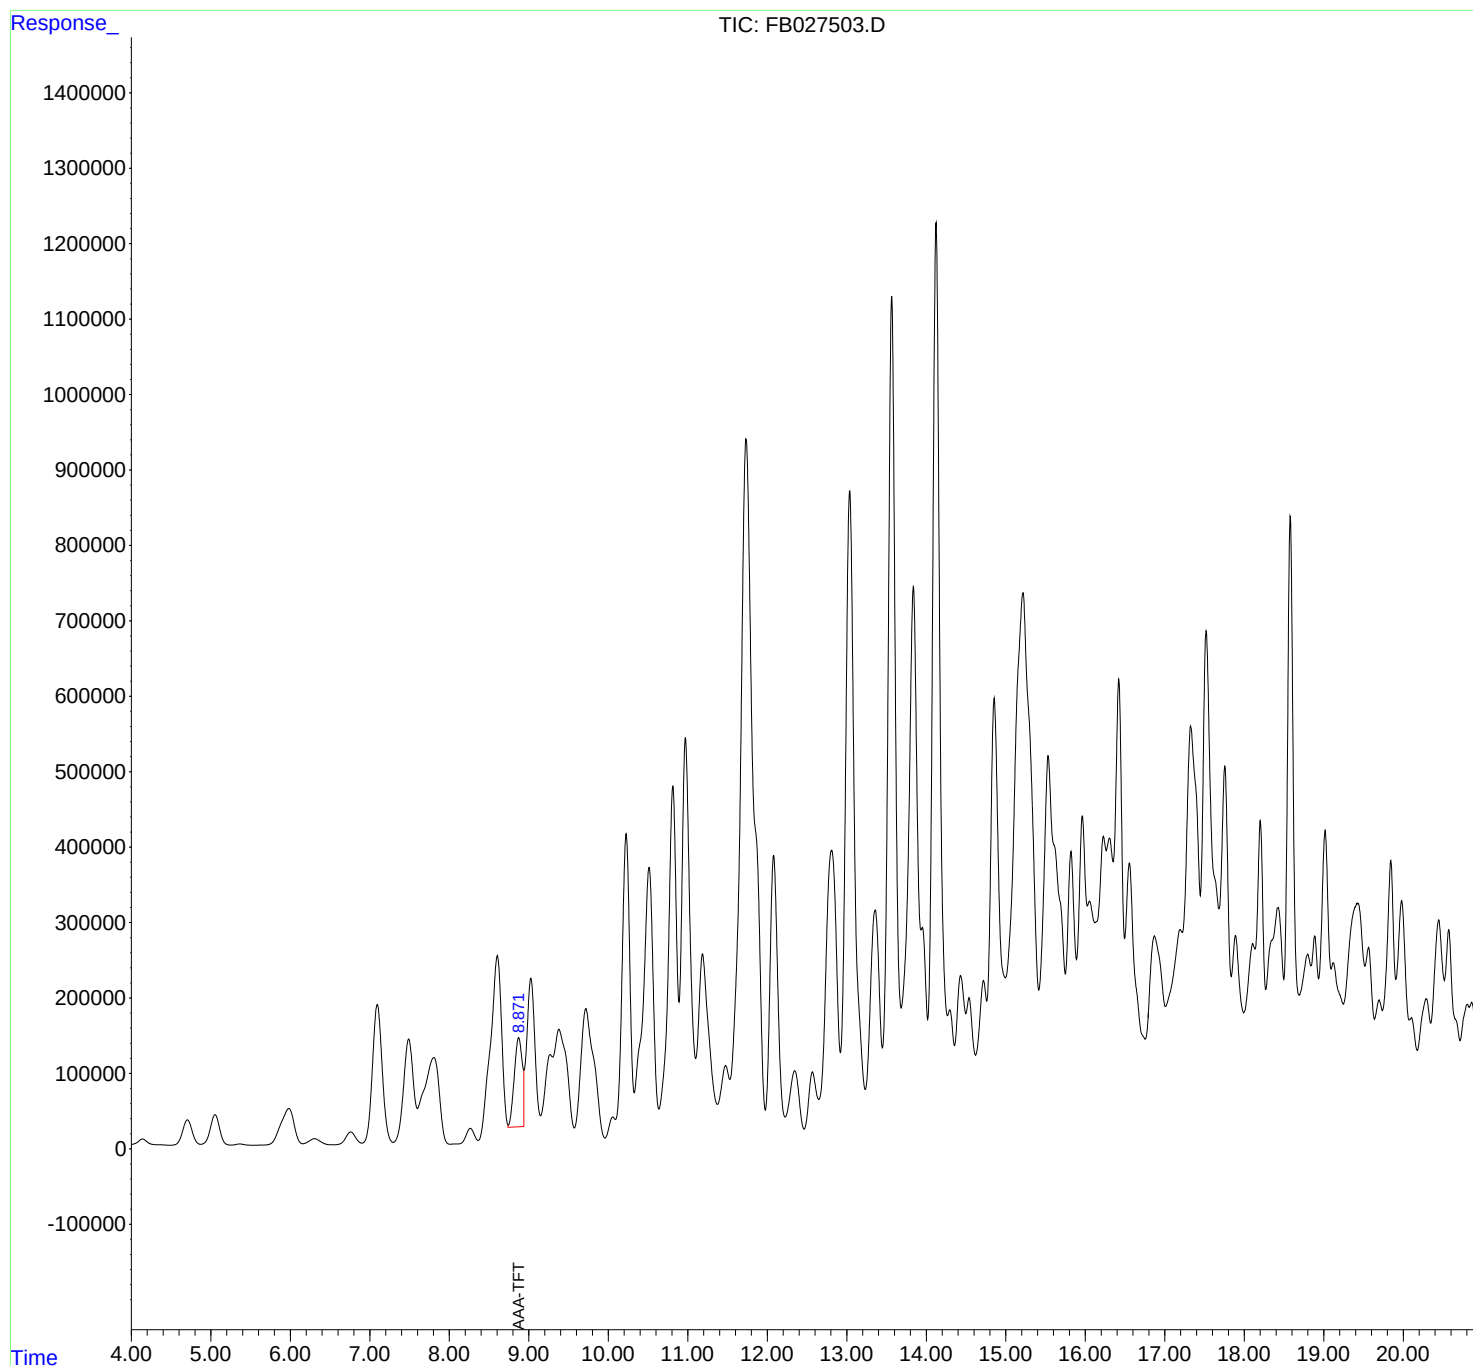

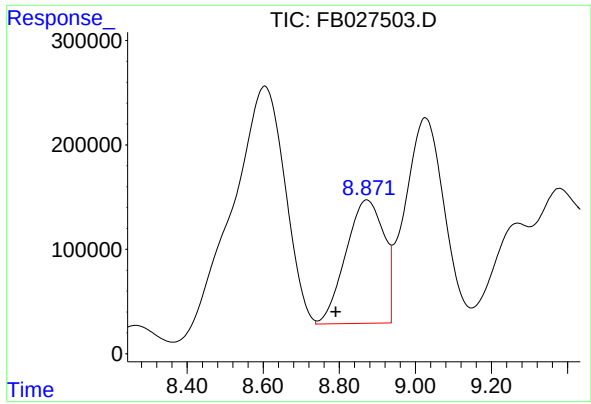

#5 AAA-TFT

R.T.: 8.871 min  
Delta R.T.: 0.080 min  
Response: 8404153  
Conc: 749.26 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
WC-14B-2-4-GR

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/23/2022  
Supervised By :Ankita Jodhani 06/23/2022