

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062322\
 Data File : FB027531.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jun 2022 00:10
 Operator : AJ/MA
 Sample : BSF0623S2
 Misc : 5.04/5.00 ML DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0623S2

Integration File: SAMPLE.e
 Quant Time: Jun 24 02:28:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	232290	20.709 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	473176	28.086 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	507379	28.897 ng/ml
3) t n-Heptane	7.752	159329	9.095 ng/ml
4) t Benzene	7.888	204724	10.039 ng/ml
6) t Toluene	10.621	575827	29.740 ng/ml
7) t Ethylbenzene	13.058	183645	10.141 ng/ml
8) t m-Xylene	13.190	356122	19.978 ng/ml
9) t O-Xylene	13.917	345279	19.871 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	343976	20.024 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062322\
Data File : FB027531.D
Signal(s) : FID2B.CH
Acq On : 24 Jun 2022 00:10
Operator : AJ/MA
Sample : BSF0623S2
Misc : 5.04/5.00 ML DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0623S2

Integration File: SAMPLE.e
Quant Time: Jun 24 02:28:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

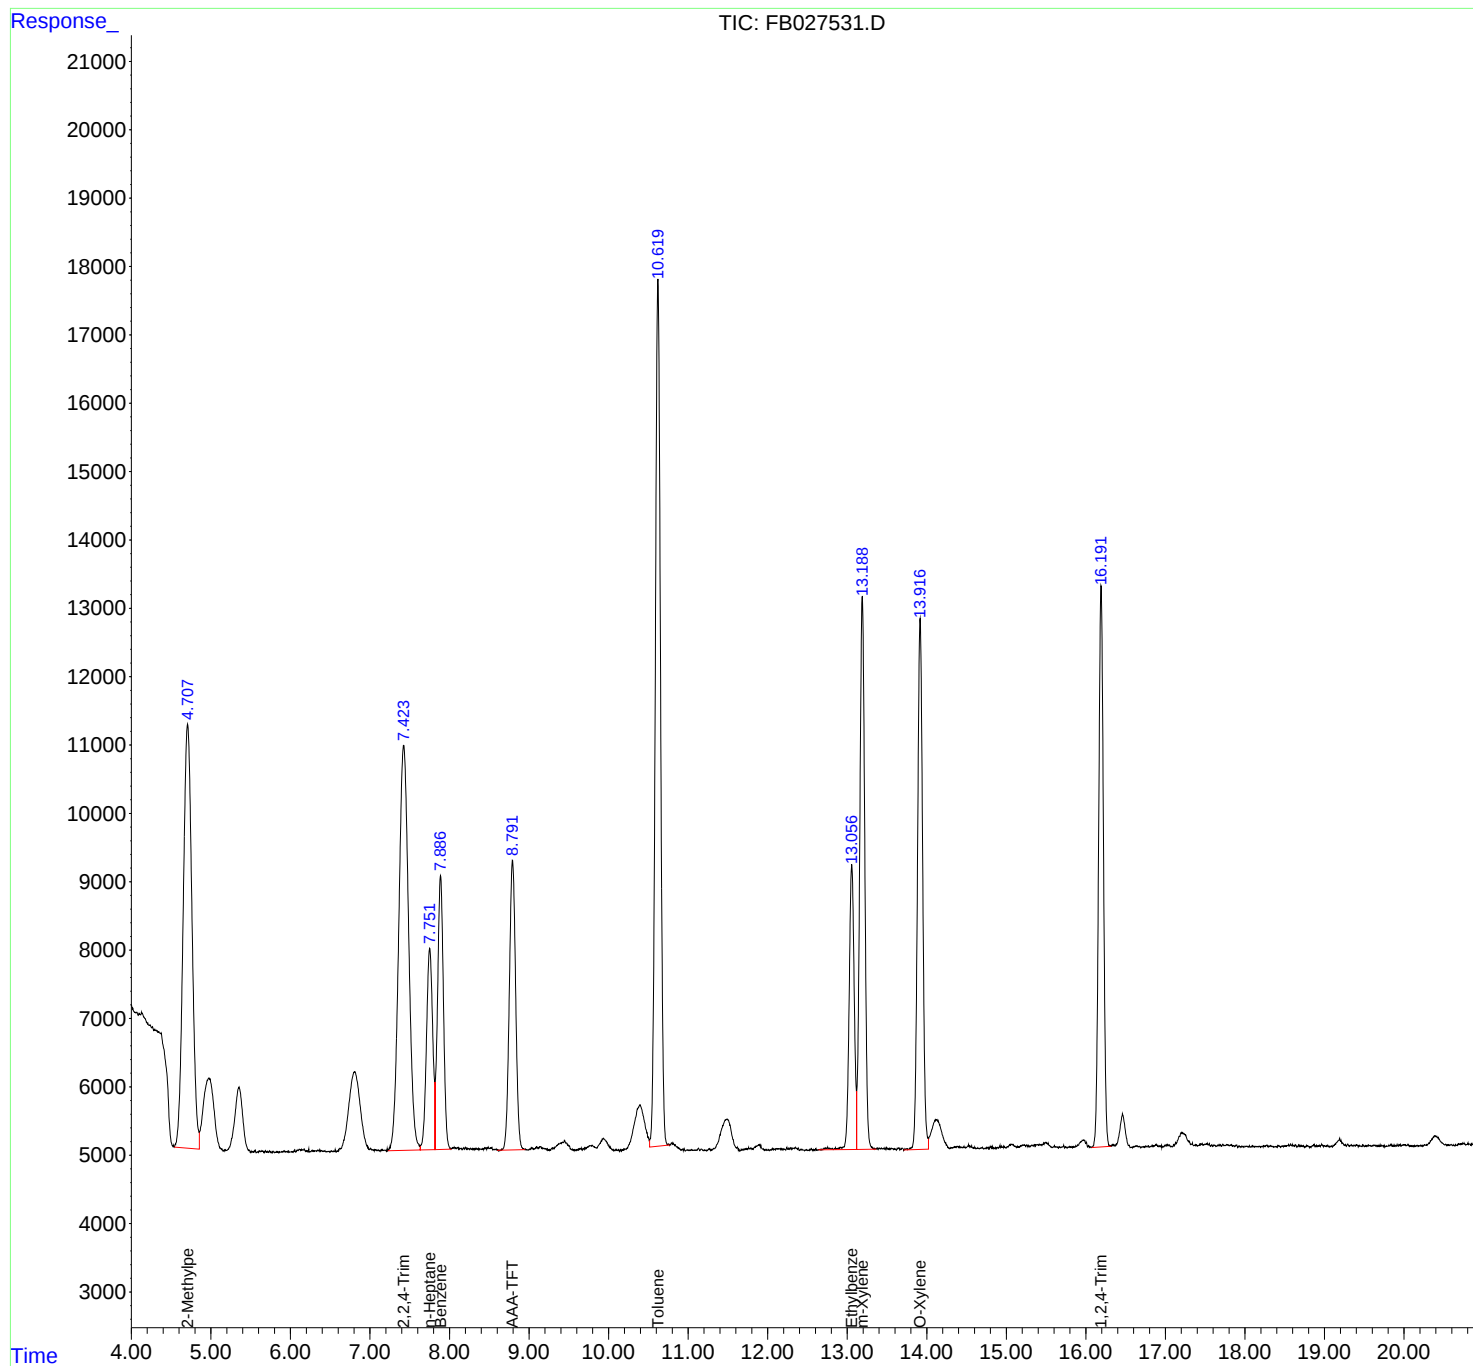


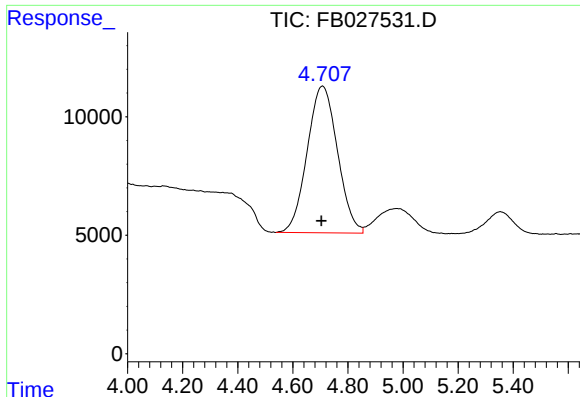

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.004 min
Response: 473176
Conc: 28.09 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0623S2

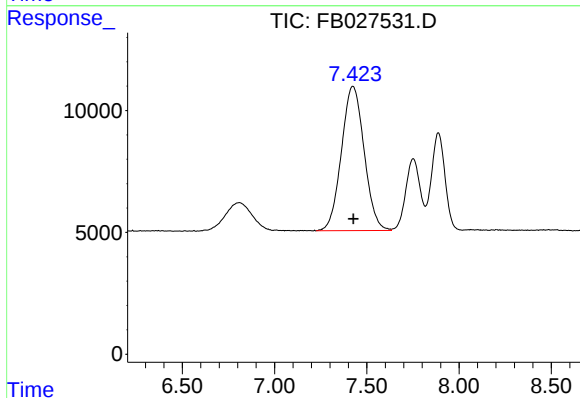


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.002 min
Response: 507379
Conc: 28.90 ng/ml

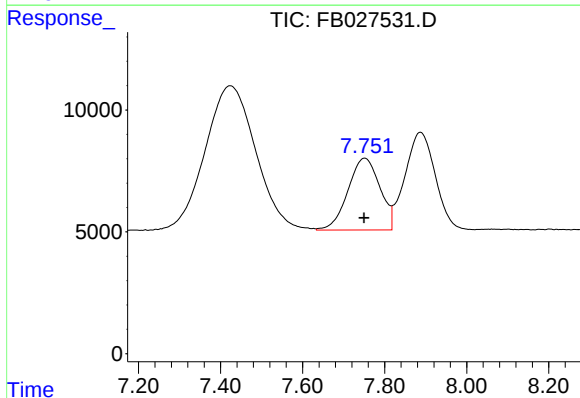


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.002 min
Response: 159329
Conc: 9.09 ng/ml

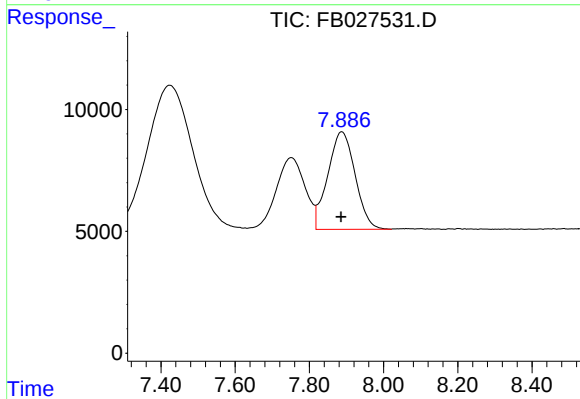

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 204724
Conc: 10.04 ng/ml

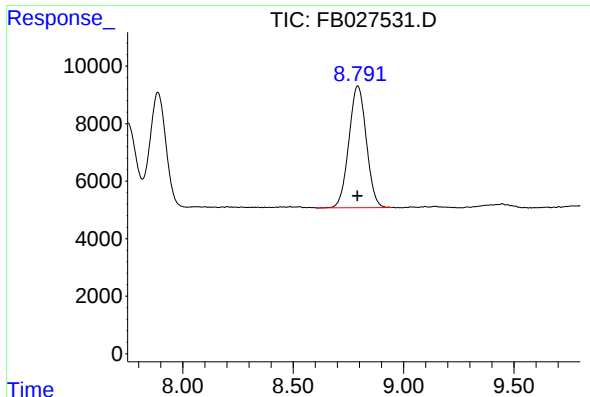

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 232290
Conc: 20.71 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0623S2

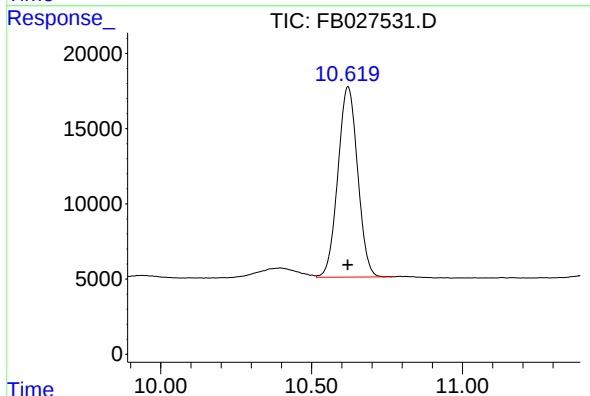


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 575827
Conc: 29.74 ng/ml

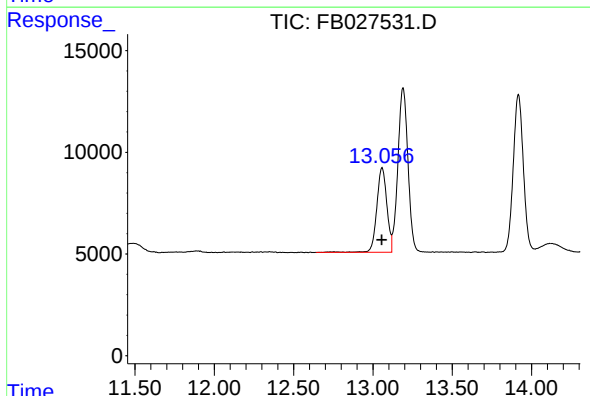


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.001 min
Response: 183645
Conc: 10.14 ng/ml

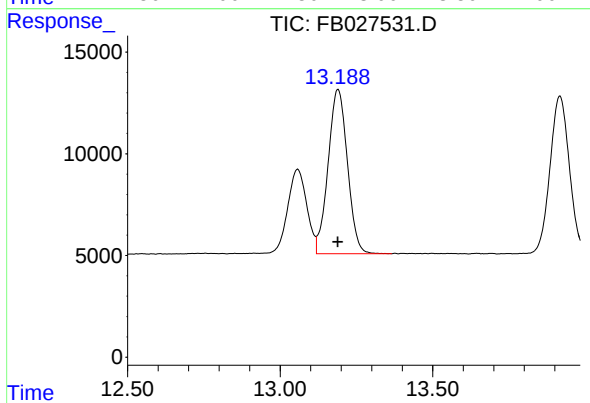

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 356122
Conc: 19.98 ng/ml

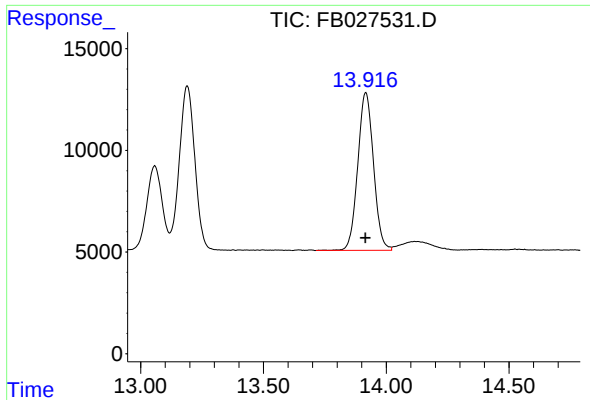

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.001 min
Response: 345279
Conc: 19.87 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0623S2

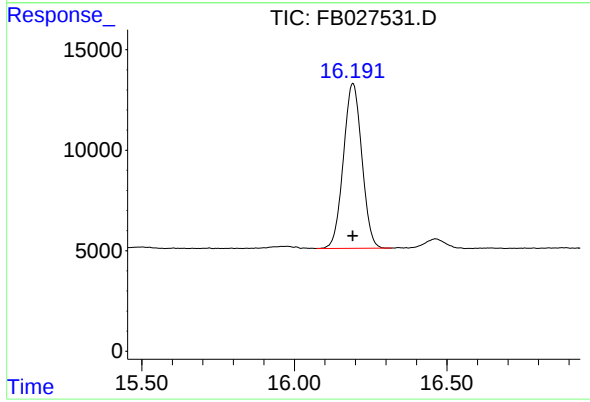

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 343976
Conc: 20.02 ng/ml