

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062419\
 Data File : FB021477.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jun 2019 14:49
 Operator : MJ/SJ
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 24 15:18:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 15:15:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	272172	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	997175	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	912133	30.000 ng/ml
3) t n-Heptane	7.948	288422	10.000 ng/ml
4) t Benzene	8.082	333161	10.000 ng/ml
6) t Toluene	10.830	678829	30.000 ng/ml
7) t Ethylbenzene	13.275	231488	10.000 ng/ml
8) t m-Xylene	13.408	494156	20.000 ng/ml
9) t O-Xylene	14.138	512435	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	514999	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062419\
Data File : FB021477.D
Signal(s) : FID2B.CH
Acq On : 24 Jun 2019 14:49
Operator : MJ/SJ
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 24 15:18:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 15:15:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

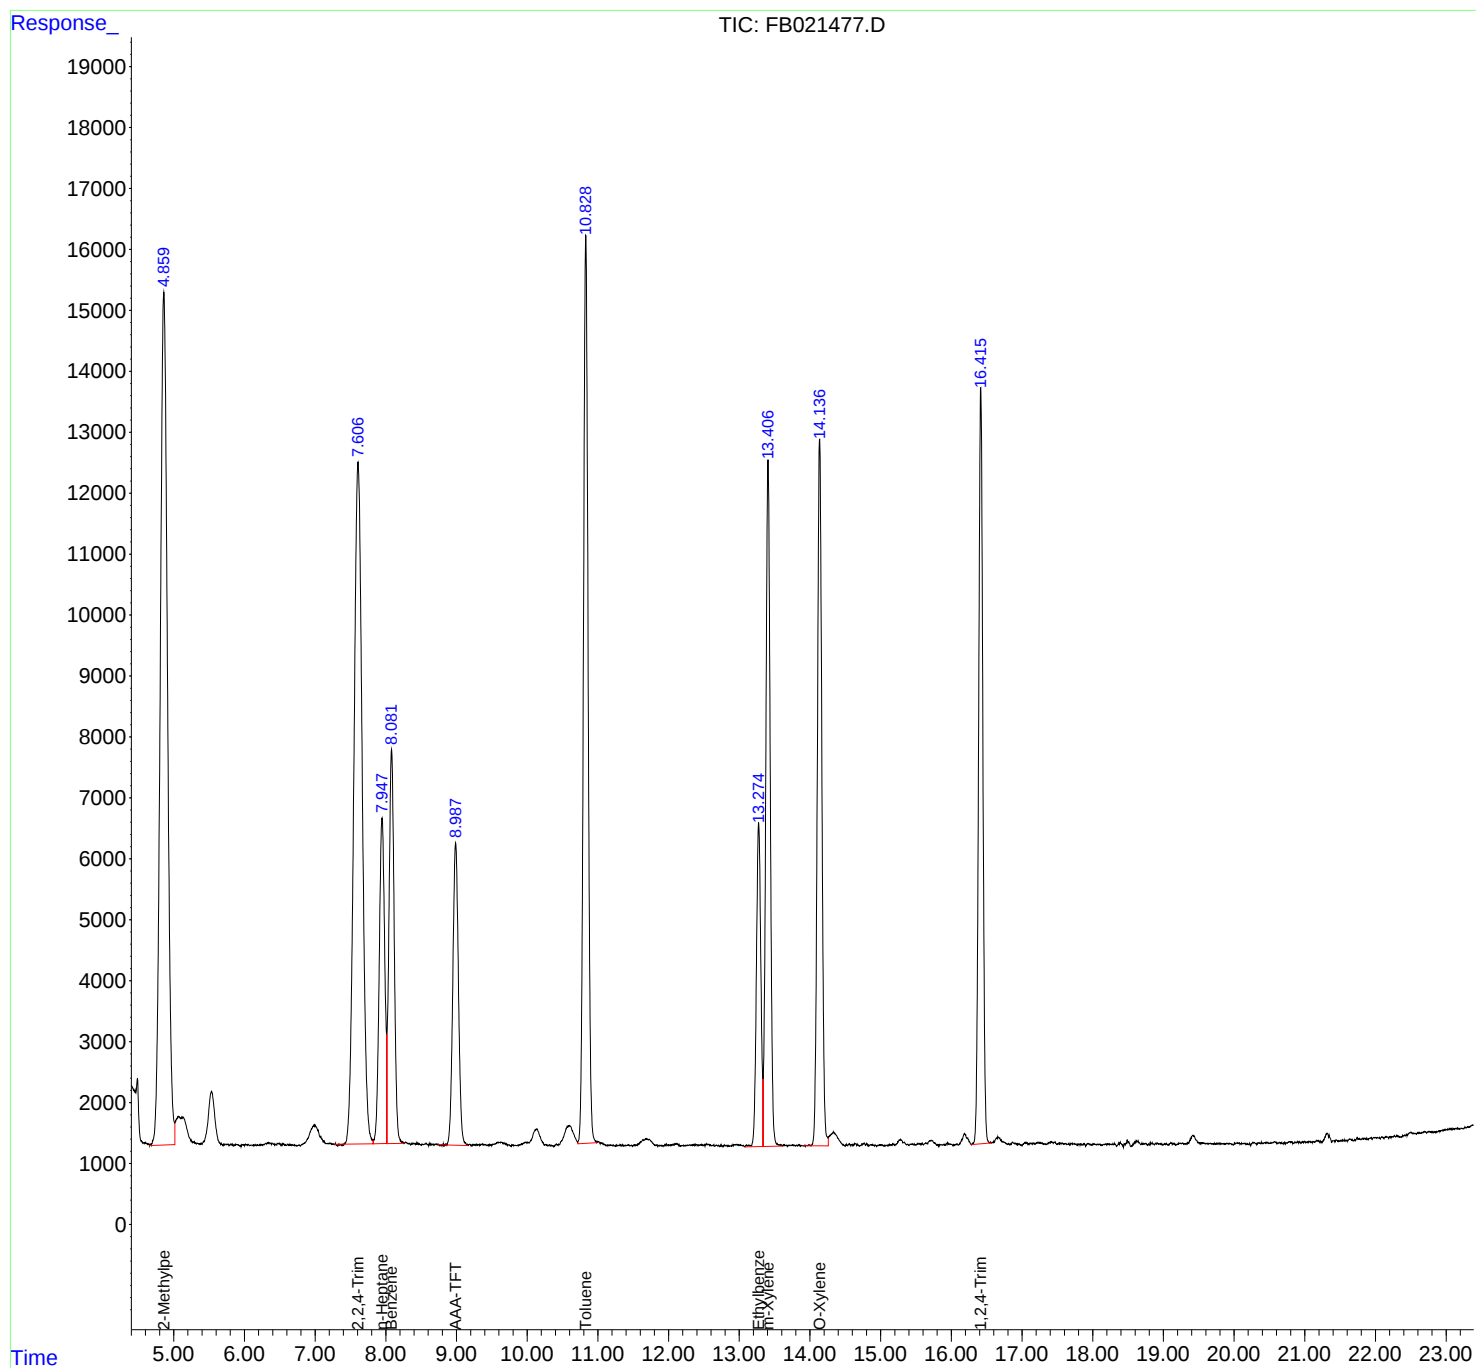


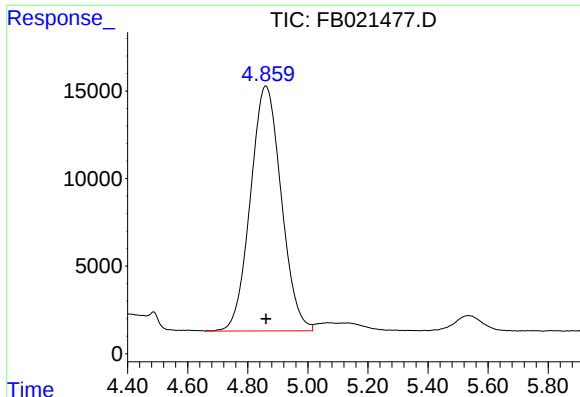

#1 2-Methylpentane


R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 997175
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :

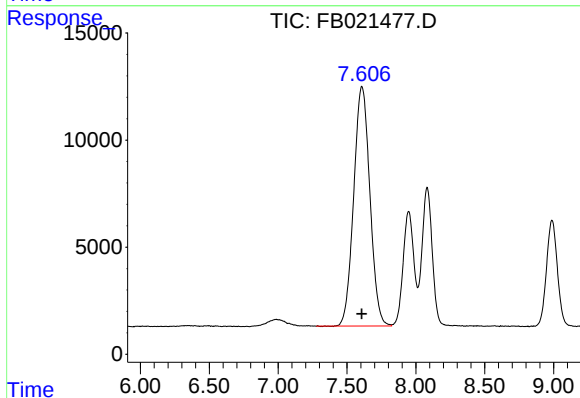


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 912133
Conc: 30.00 ng/ml

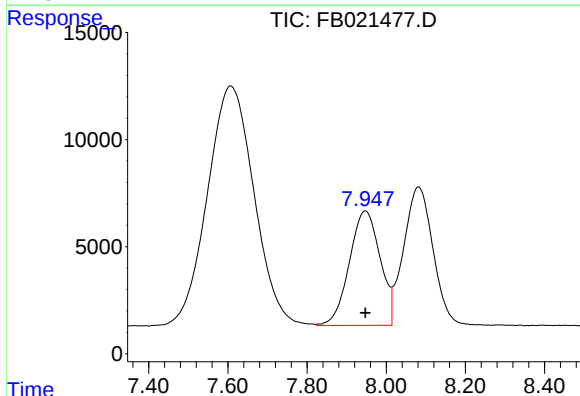


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 288422
Conc: 10.00 ng/ml

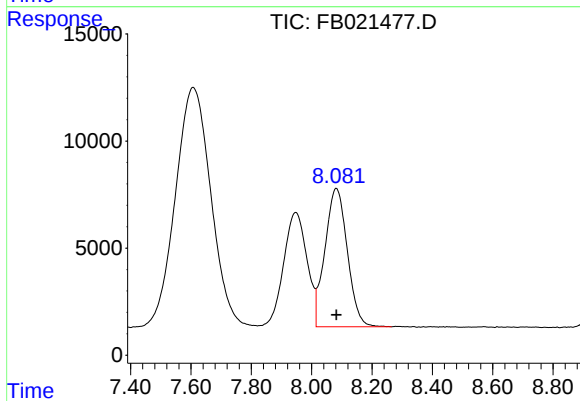

#4 Benzene


R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 333161
Conc: 10.00 ng/ml

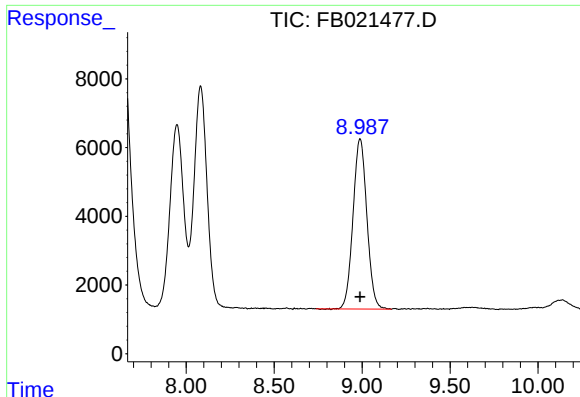

#5 AAA-TFT


R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 272172
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

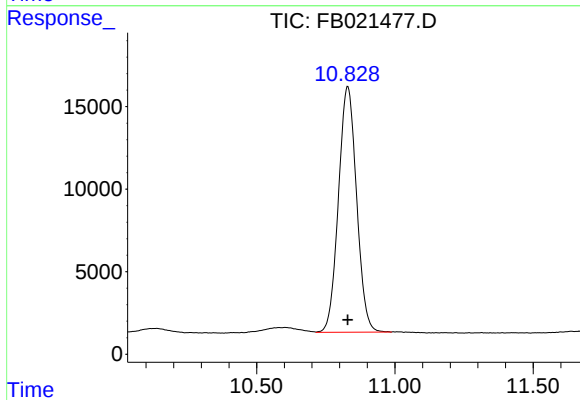


#6 Toluene

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 678829
Conc: 30.00 ng/ml

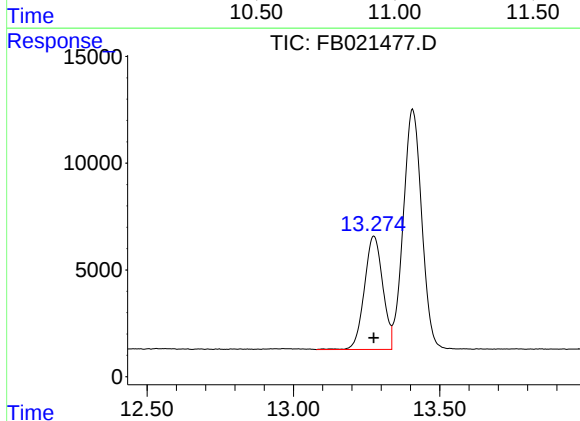


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: 0.000 min
Response: 231488
Conc: 10.00 ng/ml

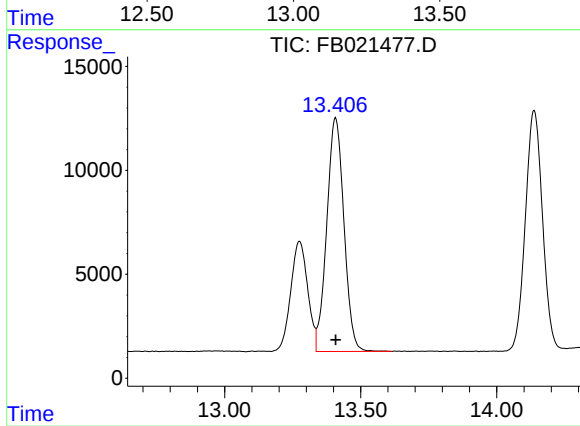

#8 m-Xylene


R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 494156
Conc: 20.00 ng/ml

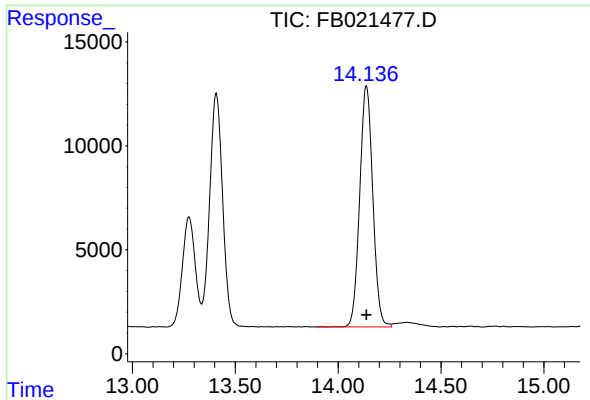

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: 0.000 min
Response: 512435
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

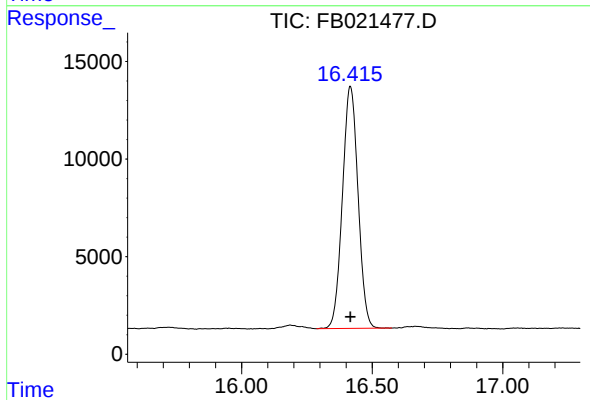

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: 0.000 min
Response: 514999
Conc: 20.00 ng/ml