

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062420\
 Data File : FB024489.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jun 2020 16:00
 Operator : DD/AJ
 Sample : BSF0624S1
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 25 00:56:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	487175	20.136 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	938455	29.360 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	979430	29.216 ng/ml
3) t n-Heptane	7.757	325917	9.638 ng/ml
4) t Benzene	7.893	393074	9.723 ng/ml
6) t Toluene	10.631	1128327	28.712 ng/ml
7) t Ethylbenzene	13.072	348081	9.919 ng/ml
8) t m-Xylene	13.204	674399	19.693 ng/ml
9) t O-Xylene	13.932	661009	19.716 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	564444	20.329 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062420\
Data File : FB024489.D
Signal(s) : FID2B.CH
Acq On : 24 Jun 2020 16:00
Operator : DD/AJ
Sample : BSF0624S1
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 25 00:56:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

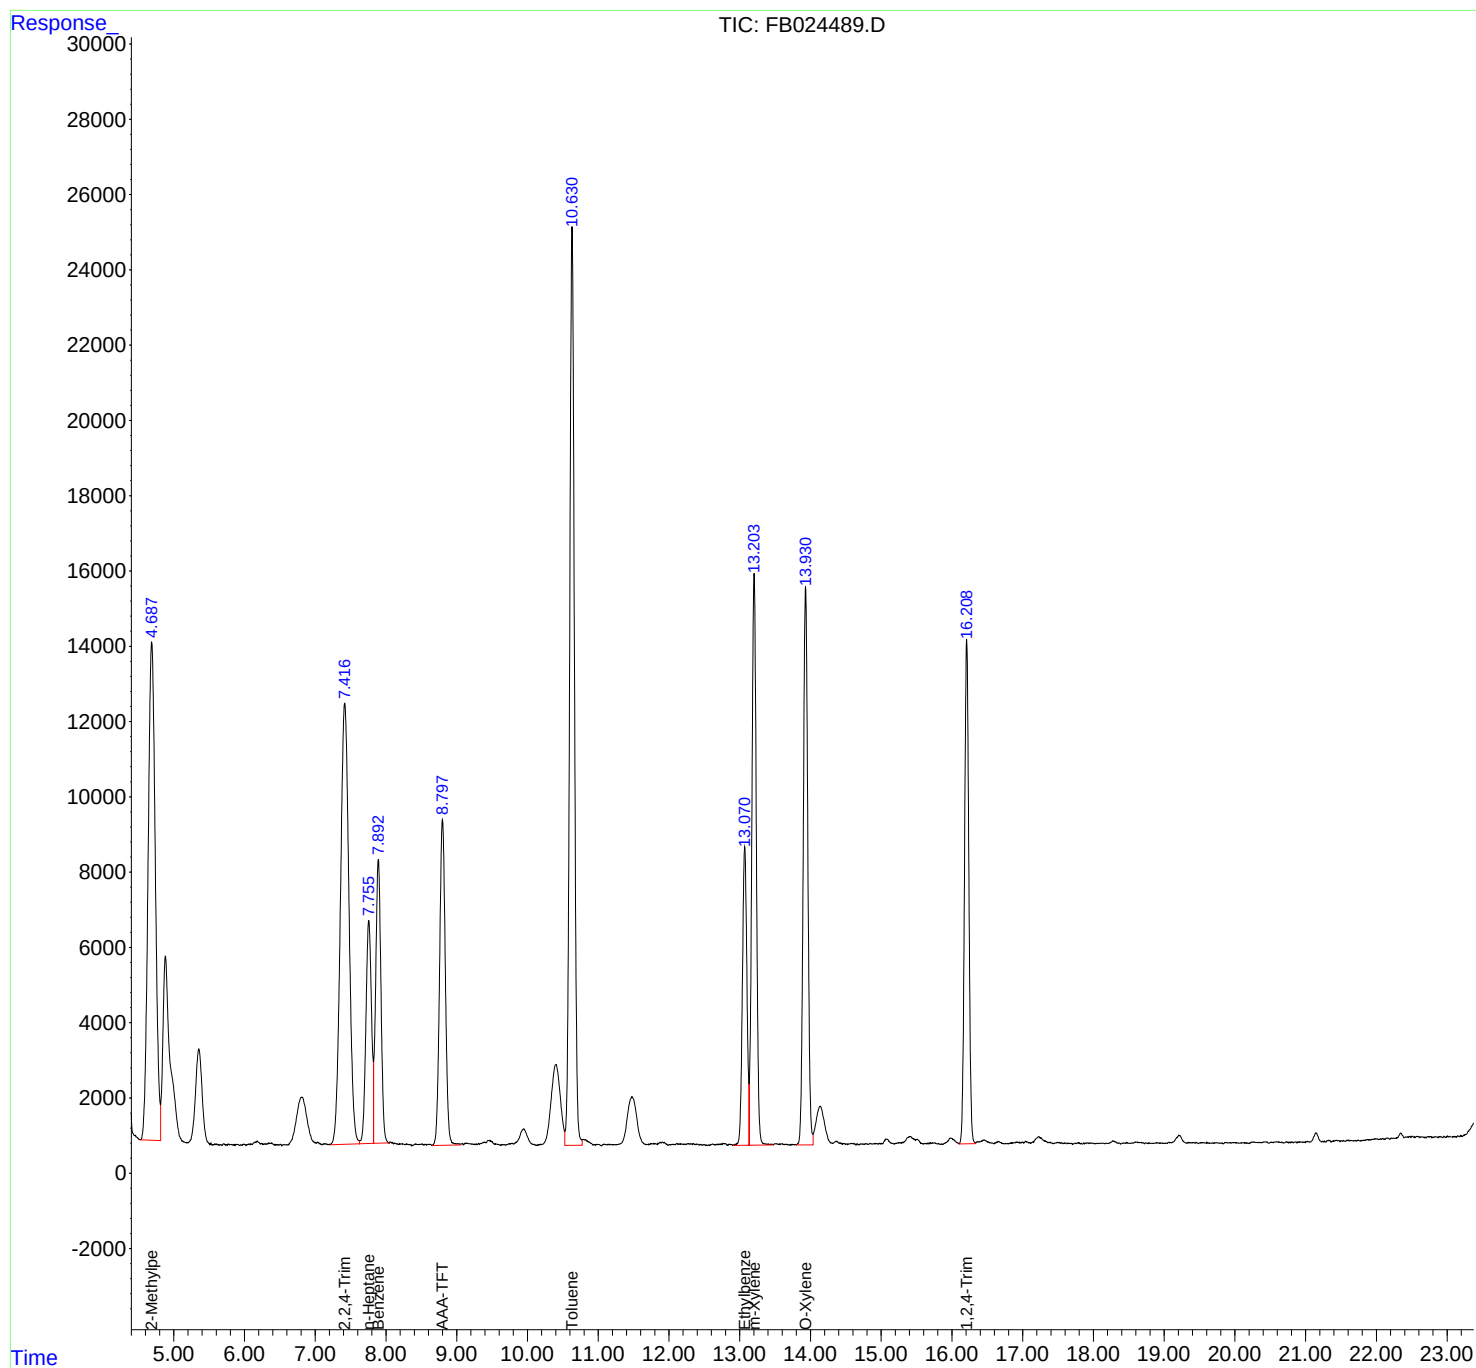

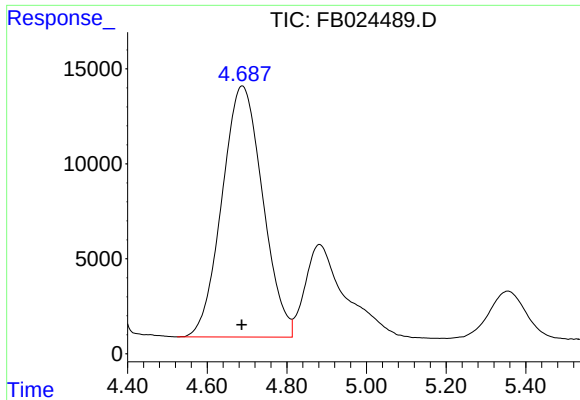


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.002 min
Response: 938455
Conc: 29.36 ng/ml

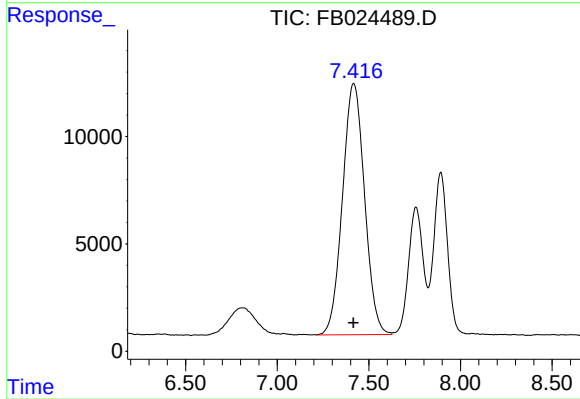


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.001 min
Response: 979430
Conc: 29.22 ng/ml

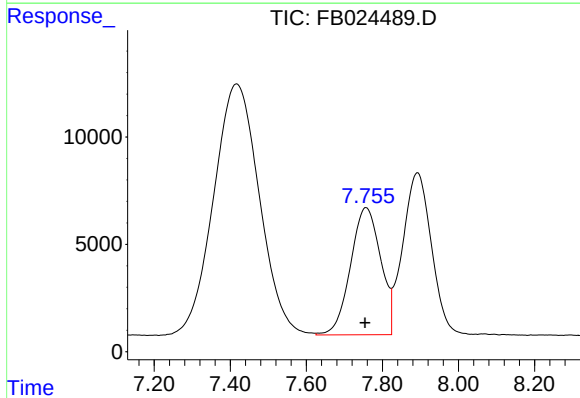


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.002 min
Response: 325917
Conc: 9.64 ng/ml

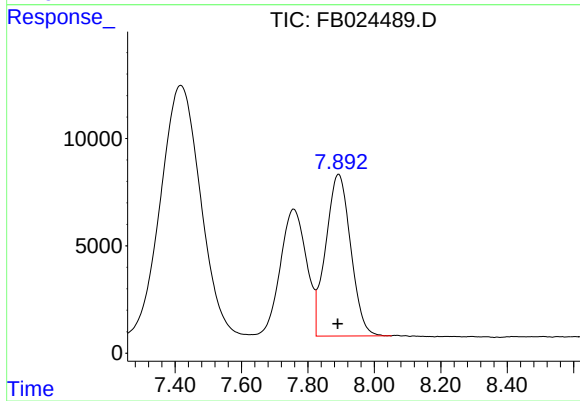


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.003 min
Response: 393074
Conc: 9.72 ng/ml

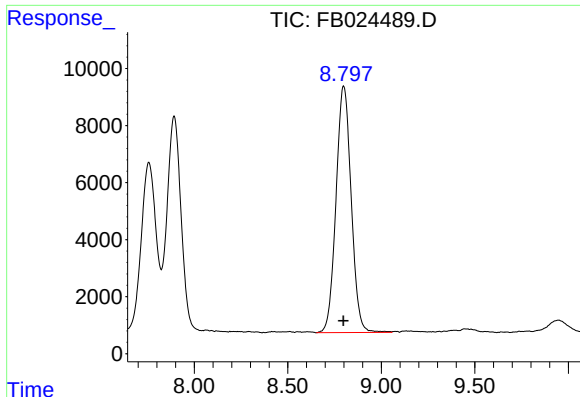


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.002 min
Response: 487175
Conc: 20.14 ng/ml

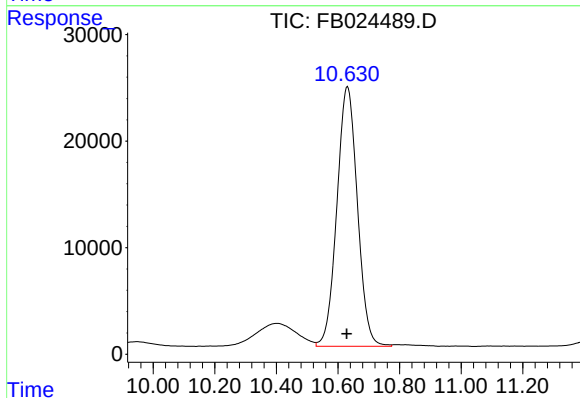


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.003 min
Response: 1128327
Conc: 28.71 ng/ml

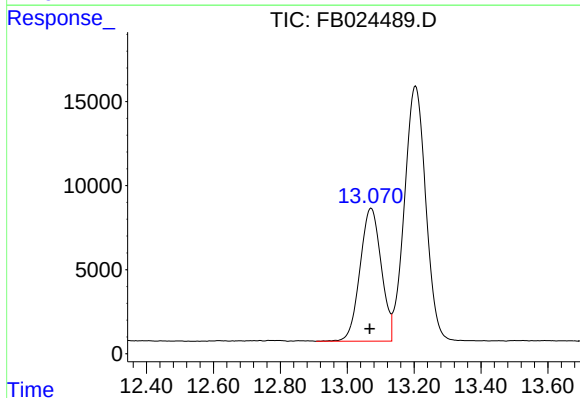


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.004 min
Response: 348081
Conc: 9.92 ng/ml

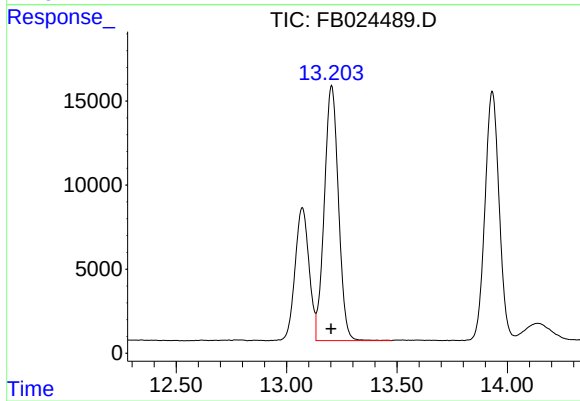

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 674399
Conc: 19.69 ng/ml

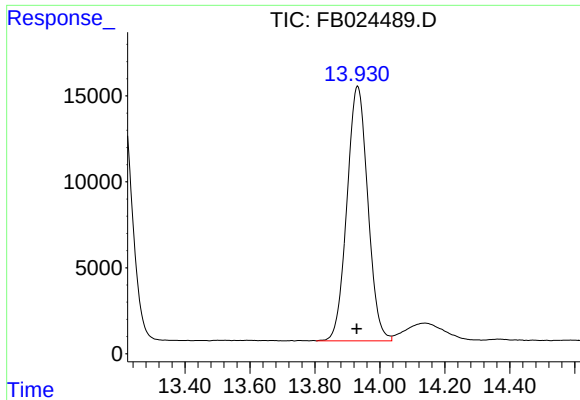


#9 O-Xylene

R.T.: 13.932 min

Delta R.T.: 0.003 min

Response: 661009

Conc: 19.72 ng/ml

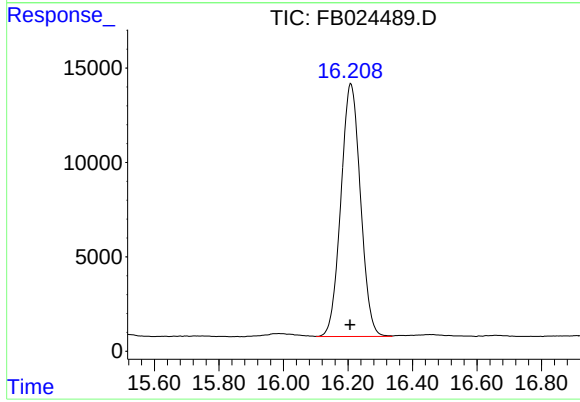

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min

Delta R.T.: 0.003 min

Response: 564444

Conc: 20.33 ng/ml