

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062421\
 Data File : FB025890.D
 Signal(s) : FID2B.CH
 Acq On : 24 Jun 2021 9:45
 Operator : DD/AJ
 Sample : BSF0624w1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 24 13:23:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.210	464153	19.206 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.164	748950	28.459 ng/ml
2) t 2,2,4-Trimethylpentane	7.862	632767	31.411 ng/ml
3) t n-Heptane	8.184	319919	8.900 ng/ml
4) t Benzene	8.335	383732	9.192 ng/ml
6) t Toluene	11.030	1091465	26.524 ng/ml
7) t Ethylbenzene	13.438	335972	8.815 ng/ml
8) t m-Xylene	13.568	661316	16.822 ng/ml
9) t o-Xylene	14.291	589976	18.503 ng/ml
10) t 1,2,4-Trimethylbenzene	16.544	392748	19.954 ng/ml


(f)=RT Delta > 1/2 window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062421\
Data File : FB025890.D
Signal(s) : FID2B.CH
Acq On : 24 Jun 2021 9:45
Operator : DD/AJ
Sample : BSF0624W1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 24 13:23:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

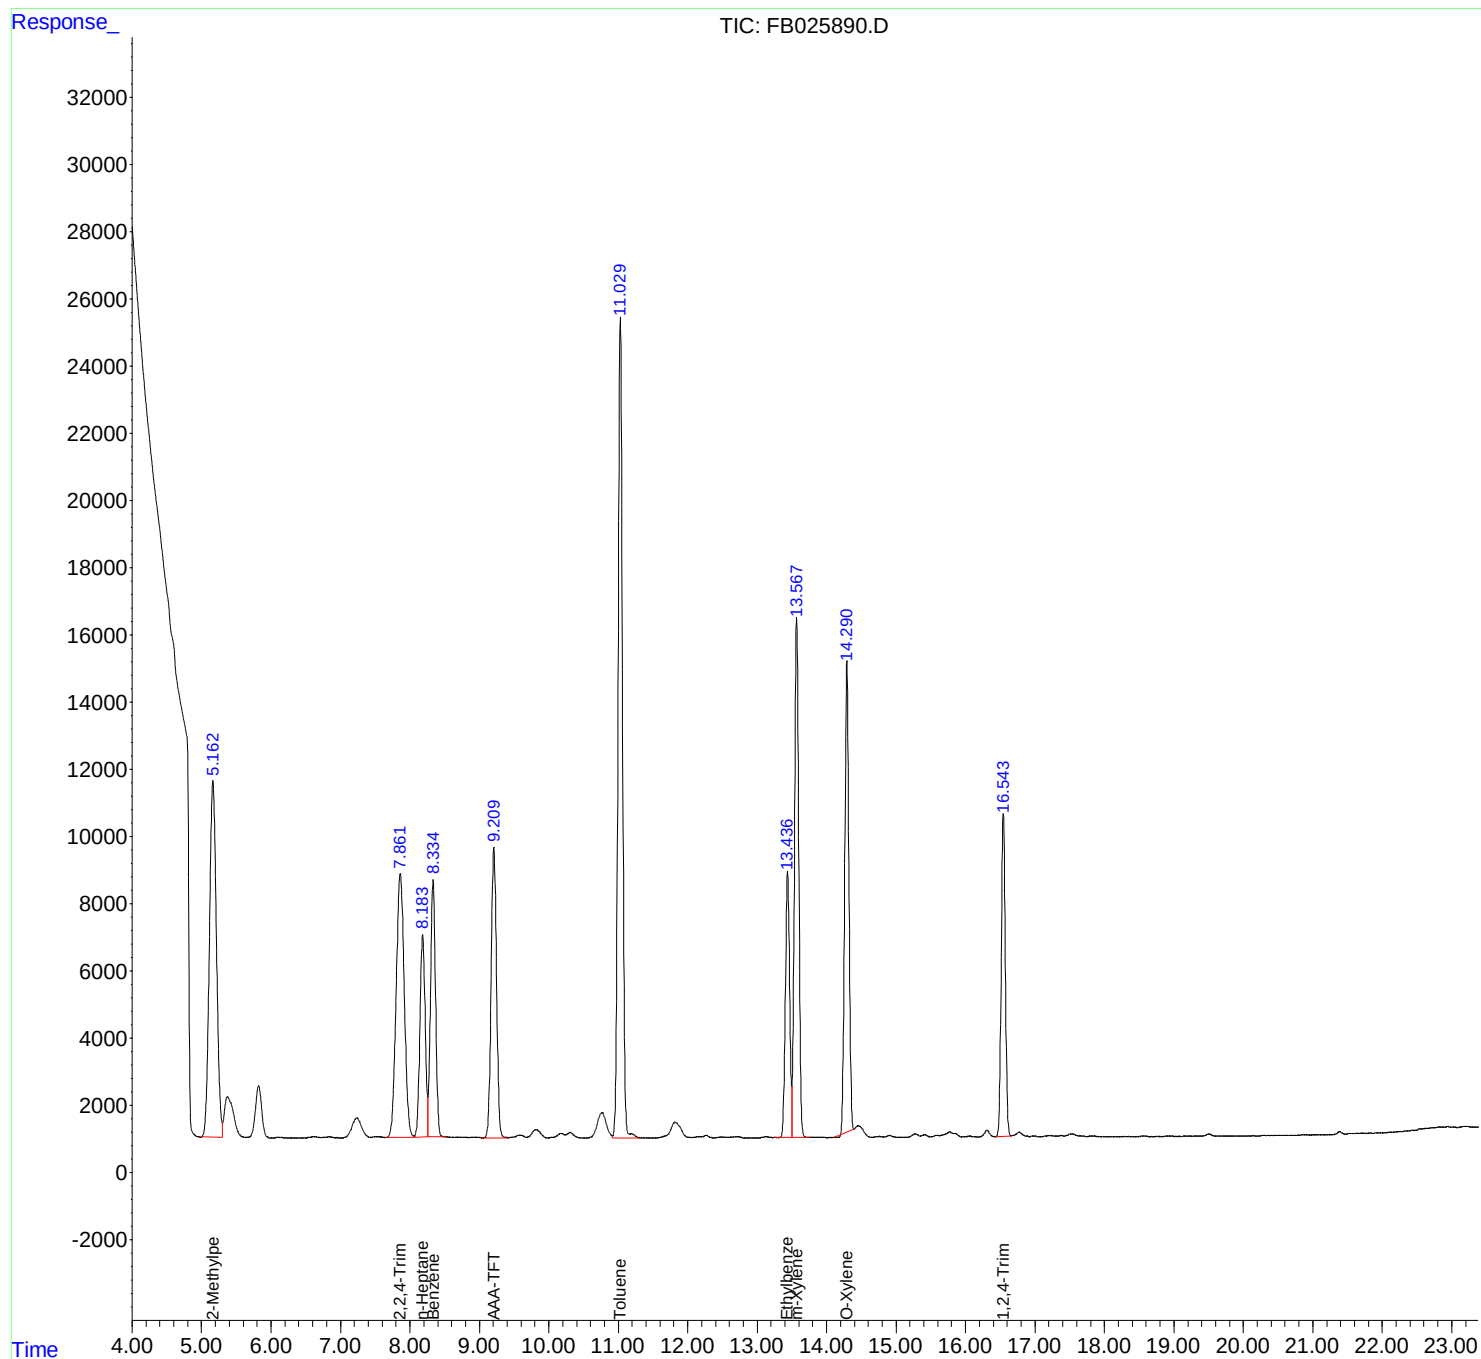

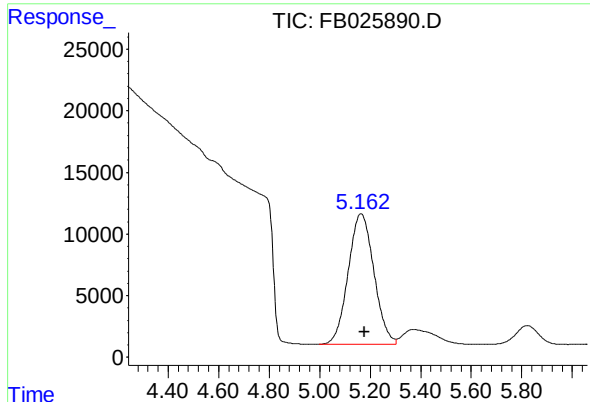


#1 2-Methylpentane

R.T.: 5.164 min
Delta R.T.: -0.013 min
Response: 748950
Conc: 28.46 ng/ml

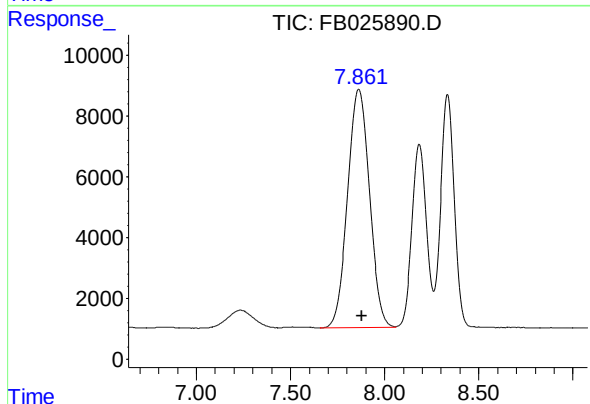


#2 2,2,4-Trimethylpentane

R.T.: 7.862 min
Delta R.T.: -0.016 min
Response: 632767
Conc: 31.41 ng/ml

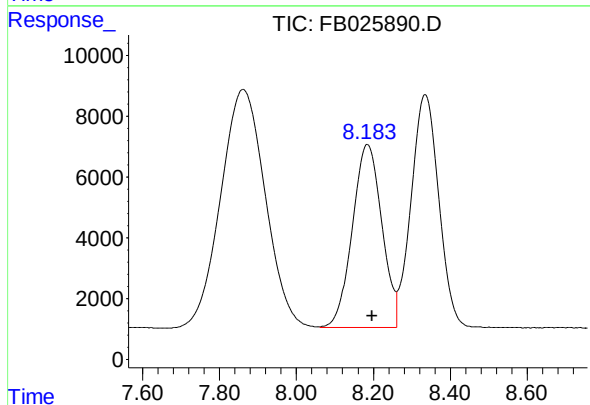


#3 n-Heptane

R.T.: 8.184 min
Delta R.T.: -0.012 min
Response: 319919
Conc: 8.90 ng/ml

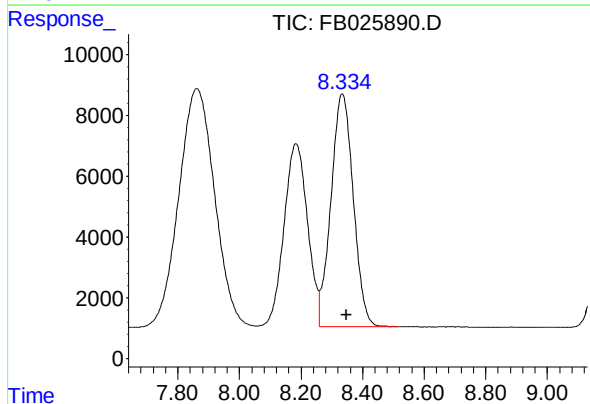


#4 Benzene

R.T.: 8.335 min
Delta R.T.: -0.012 min
Response: 383732
Conc: 9.19 ng/ml

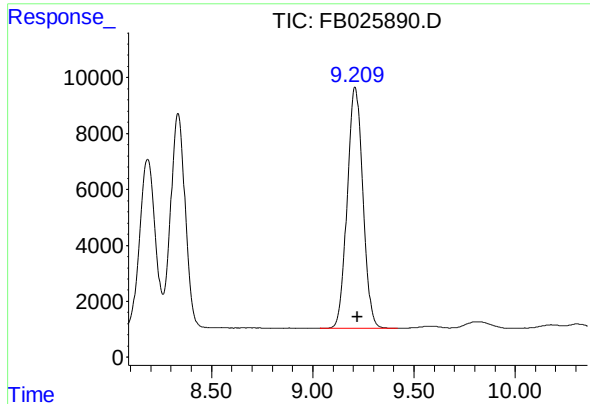


#5 AAA-TFT

R.T.: 9.210 min
Delta R.T.: -0.011 min
Response: 464153
Conc: 19.21 ng/ml

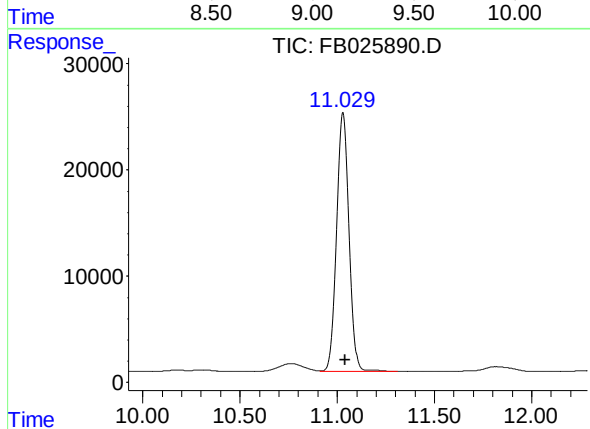


#6 Toluene

R.T.: 11.030 min
Delta R.T.: -0.011 min
Response: 1091465
Conc: 26.52 ng/ml

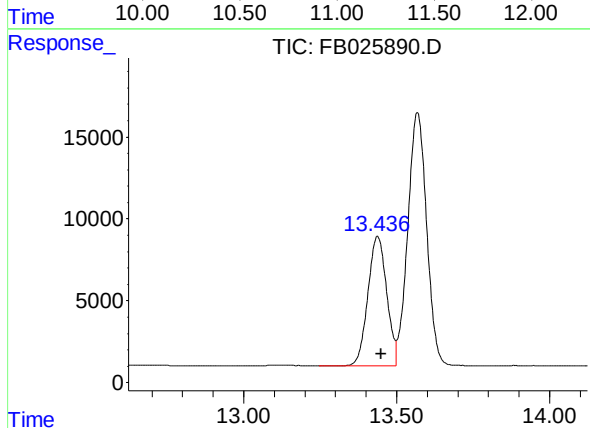


#7 Ethylbenzene

R.T.: 13.438 min
Delta R.T.: -0.010 min
Response: 335972
Conc: 8.82 ng/ml

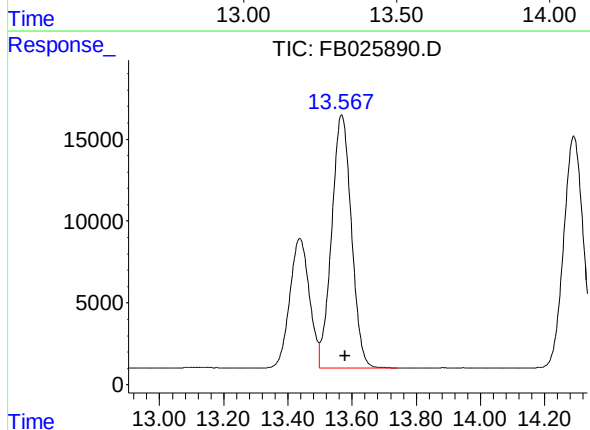


#8 m-Xylene

R.T.: 13.568 min
Delta R.T.: -0.010 min
Response: 661316
Conc: 16.82 ng/ml

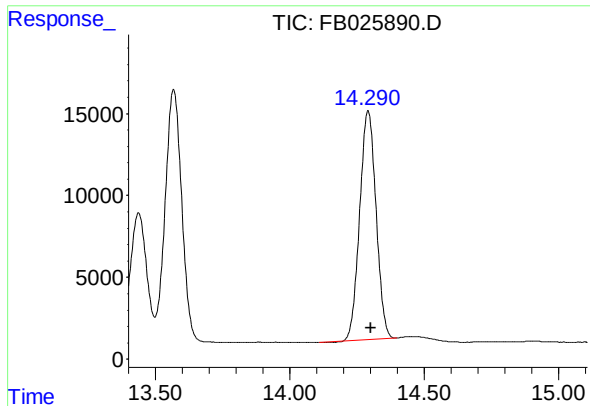

#9 O-Xylene

R.T.: 14.291 min
Delta R.T.: -0.010 min
Response: 589976
Conc: 18.50 ng/ml

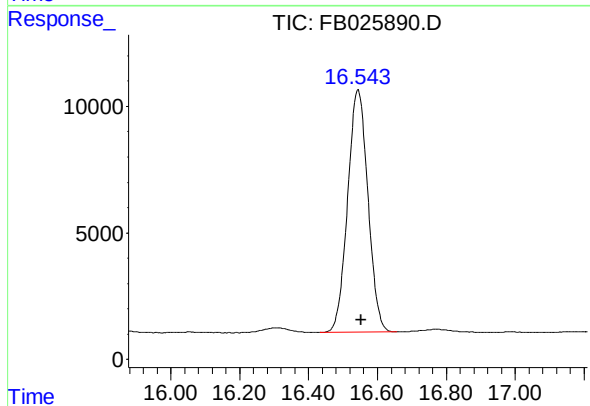

#10 1,2,4-Trimethylbenzene

R.T.: 16.544 min
Delta R.T.: -0.010 min
Response: 392748
Conc: 19.95 ng/ml