

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062519\
 Data File : FB021485.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jun 2019 15:22
 Operator : MJ/SJ
 Sample : K3510-01MS
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 26 02:12:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	298149	20.222 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.864	970490	25.815 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	848467	24.845 ng/ml
3) t n-Heptane	7.950	263675	8.088 ng/ml
4) t Benzene	8.084	341792	9.902 ng/ml
6) t Toluene	10.831	696552	29.388 ng/ml
7) t Ethylbenzene	13.276	231132	9.891 ng/ml
8) t m-Xylene	13.409	496459	19.890 ng/ml
9) t O-Xylene	14.138	521043	19.973 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	510780	19.019 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062519\
Data File : FB021485.D
Signal(s) : FID2B.CH
Acq On : 25 Jun 2019 15:22
Operator : MJ/SJ
Sample : K3510-01MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 26 02:12:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

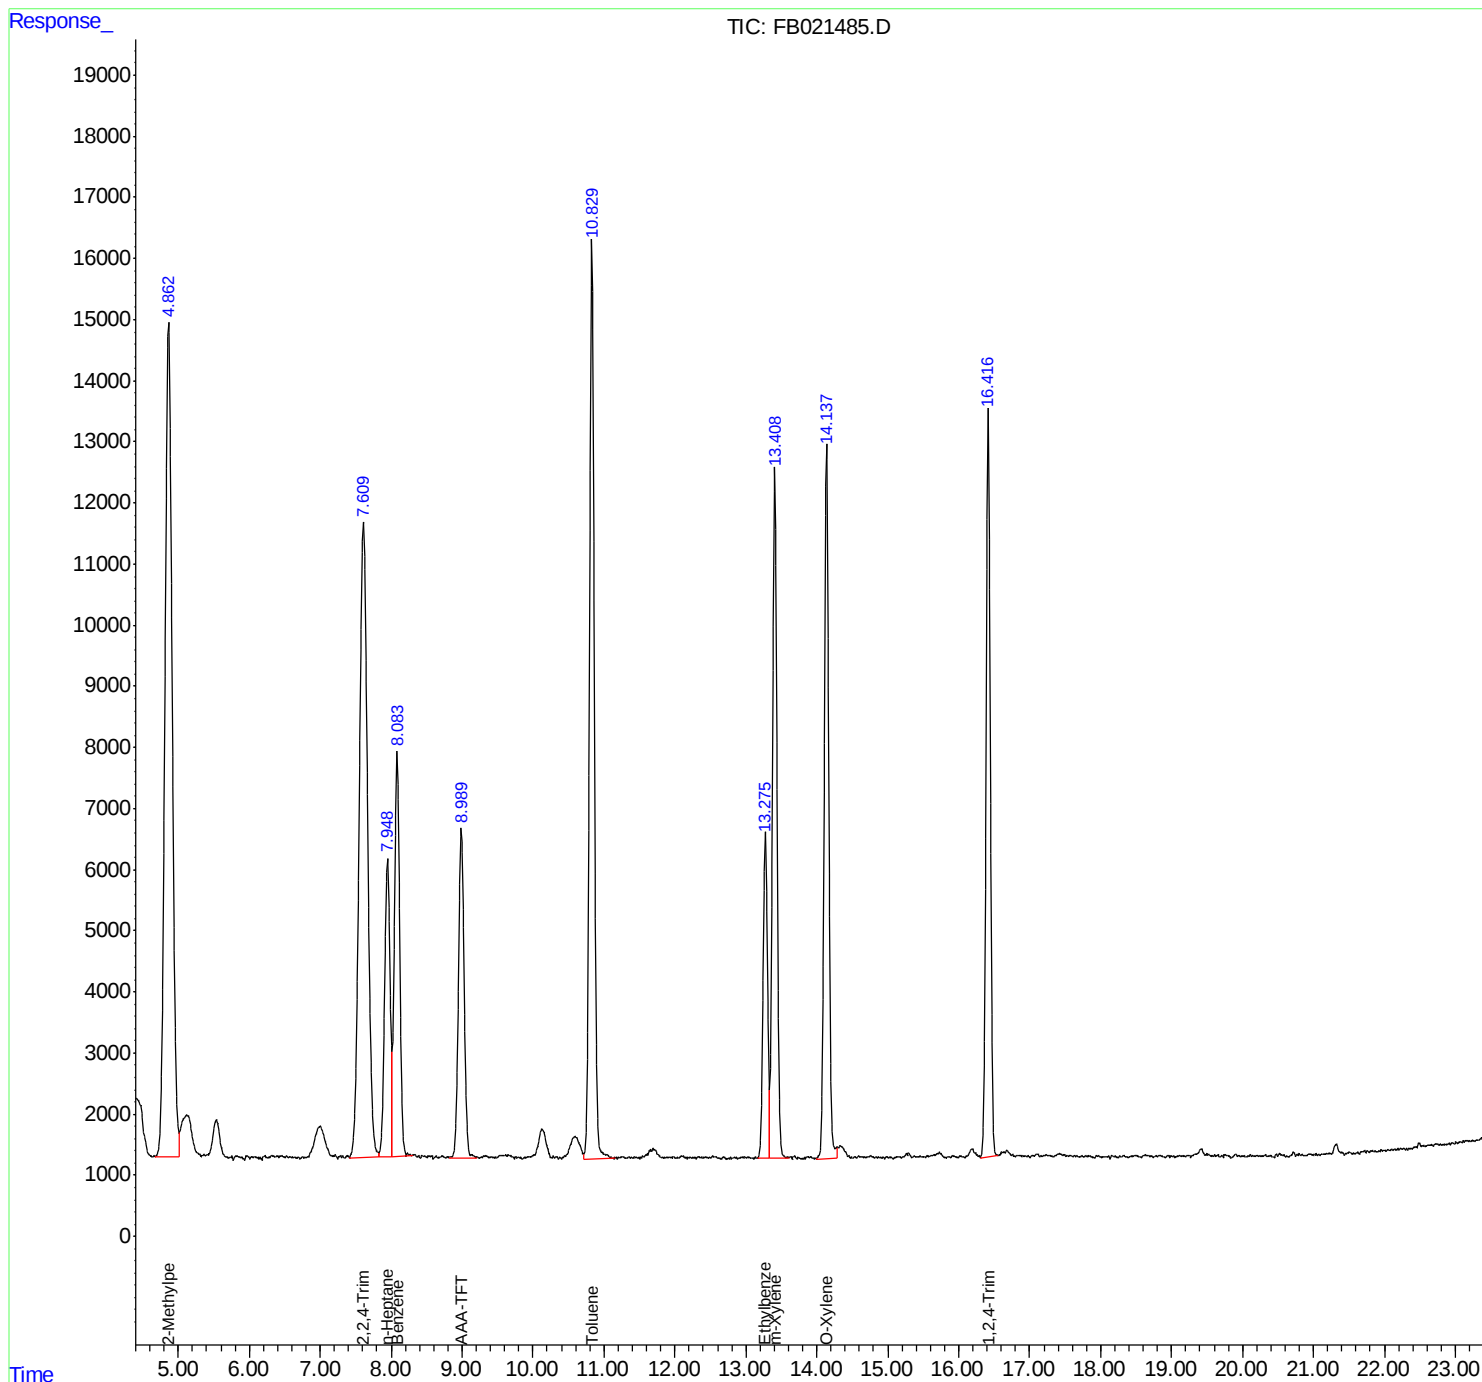

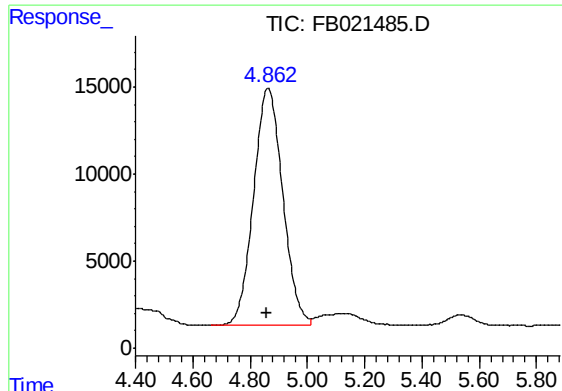


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: 0.006 min
Response: 970490
Conc: 25.82 ng/ml

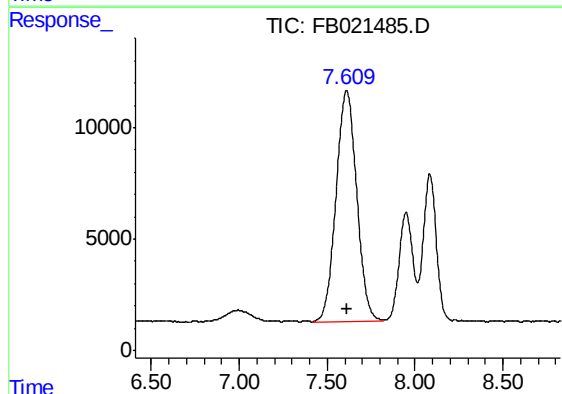


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: -0.003 min
Response: 848467
Conc: 24.84 ng/ml

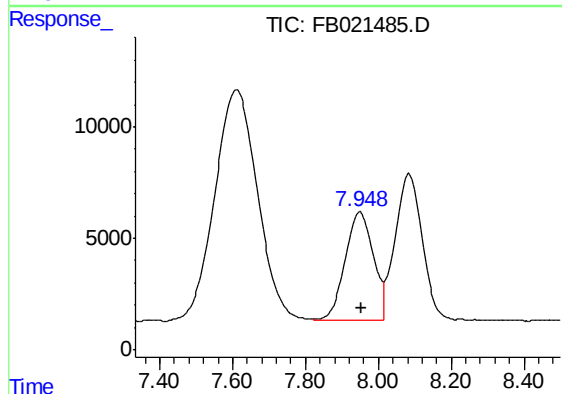


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.005 min
Response: 263675
Conc: 8.09 ng/ml

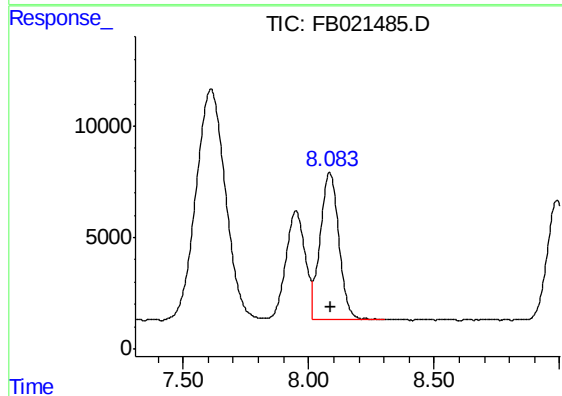


#4 Benzene

R.T.: 8.084 min
Delta R.T.: -0.006 min
Response: 341792
Conc: 9.90 ng/ml

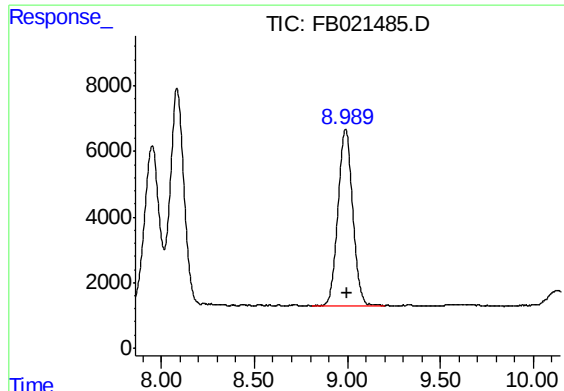


#5 AAA-TFT

R.T.: 8.990 min
Delta R.T.: -0.008 min
Response: 298149
Conc: 20.22 ng/ml

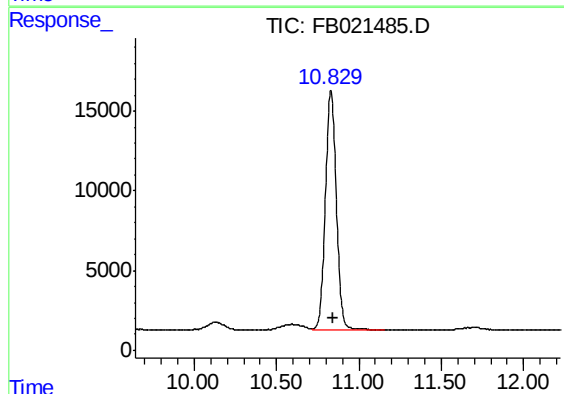


#6 Toluene

R.T.: 10.831 min
Delta R.T.: -0.012 min
Response: 696552
Conc: 29.39 ng/ml

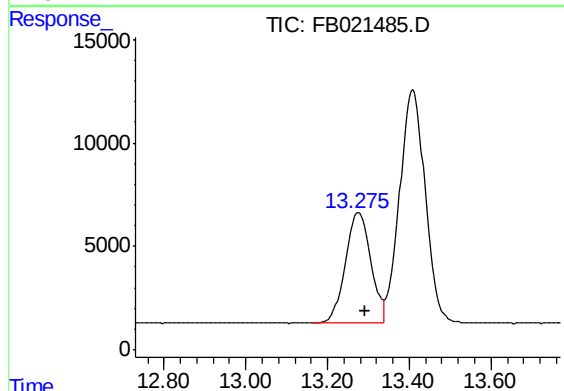


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: -0.017 min
Response: 231132
Conc: 9.89 ng/ml

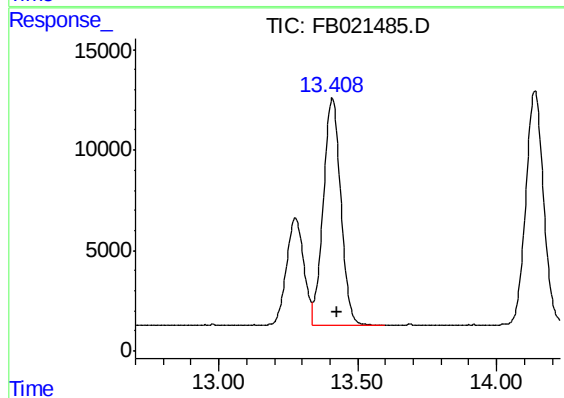


#8 m-Xylene

R.T.: 13.409 min
Delta R.T.: -0.017 min
Response: 496459
Conc: 19.89 ng/ml

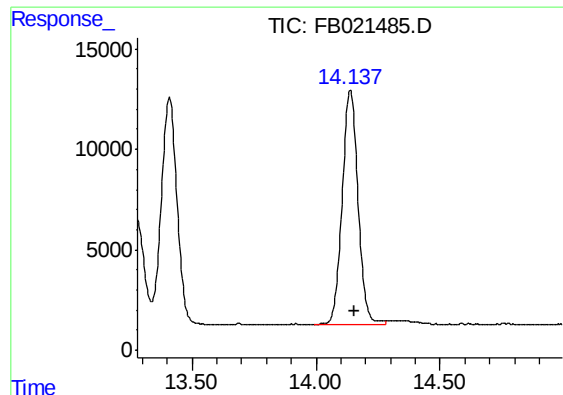

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: -0.018 min
Response: 521043
Conc: 19.97 ng/ml

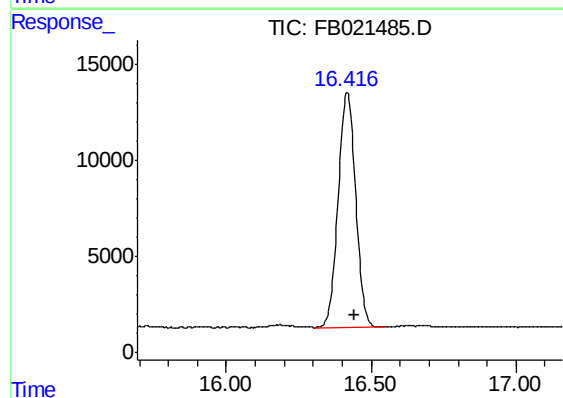

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: -0.023 min
Response: 510780
Conc: 19.02 ng/ml