

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062520\
 Data File : FB024499.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jun 2020 9:37
 Operator : DD/AJ
 Sample : BSF0625S1
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 26 00:58:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.796	499756	20.656 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	937419	29.328 ng/ml
2) t	2,2,4-Trimethylpentane	7.415	1011071	30.160 ng/ml
3) t	n-Heptane	7.755	333565	9.864 ng/ml
4) t	Benzene	7.889	395965	9.795 ng/ml
6) t	Toluene	10.627	1125774	28.647 ng/ml
7) t	Ethylbenzene	13.067	345033	9.833 ng/ml
8) t	m-Xylene	13.200	676068	19.742 ng/ml
9) t	O-Xylene	13.927	661594	19.733 ng/ml
10) t	1,2,4-Trimethylbenzene	16.205	551420	19.860 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062520\
Data File : FB024499.D
Signal(s) : FID2B.CH
Acq On : 25 Jun 2020 9:37
Operator : DD/AJ
Sample : BSF0625S1
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 26 00:58:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

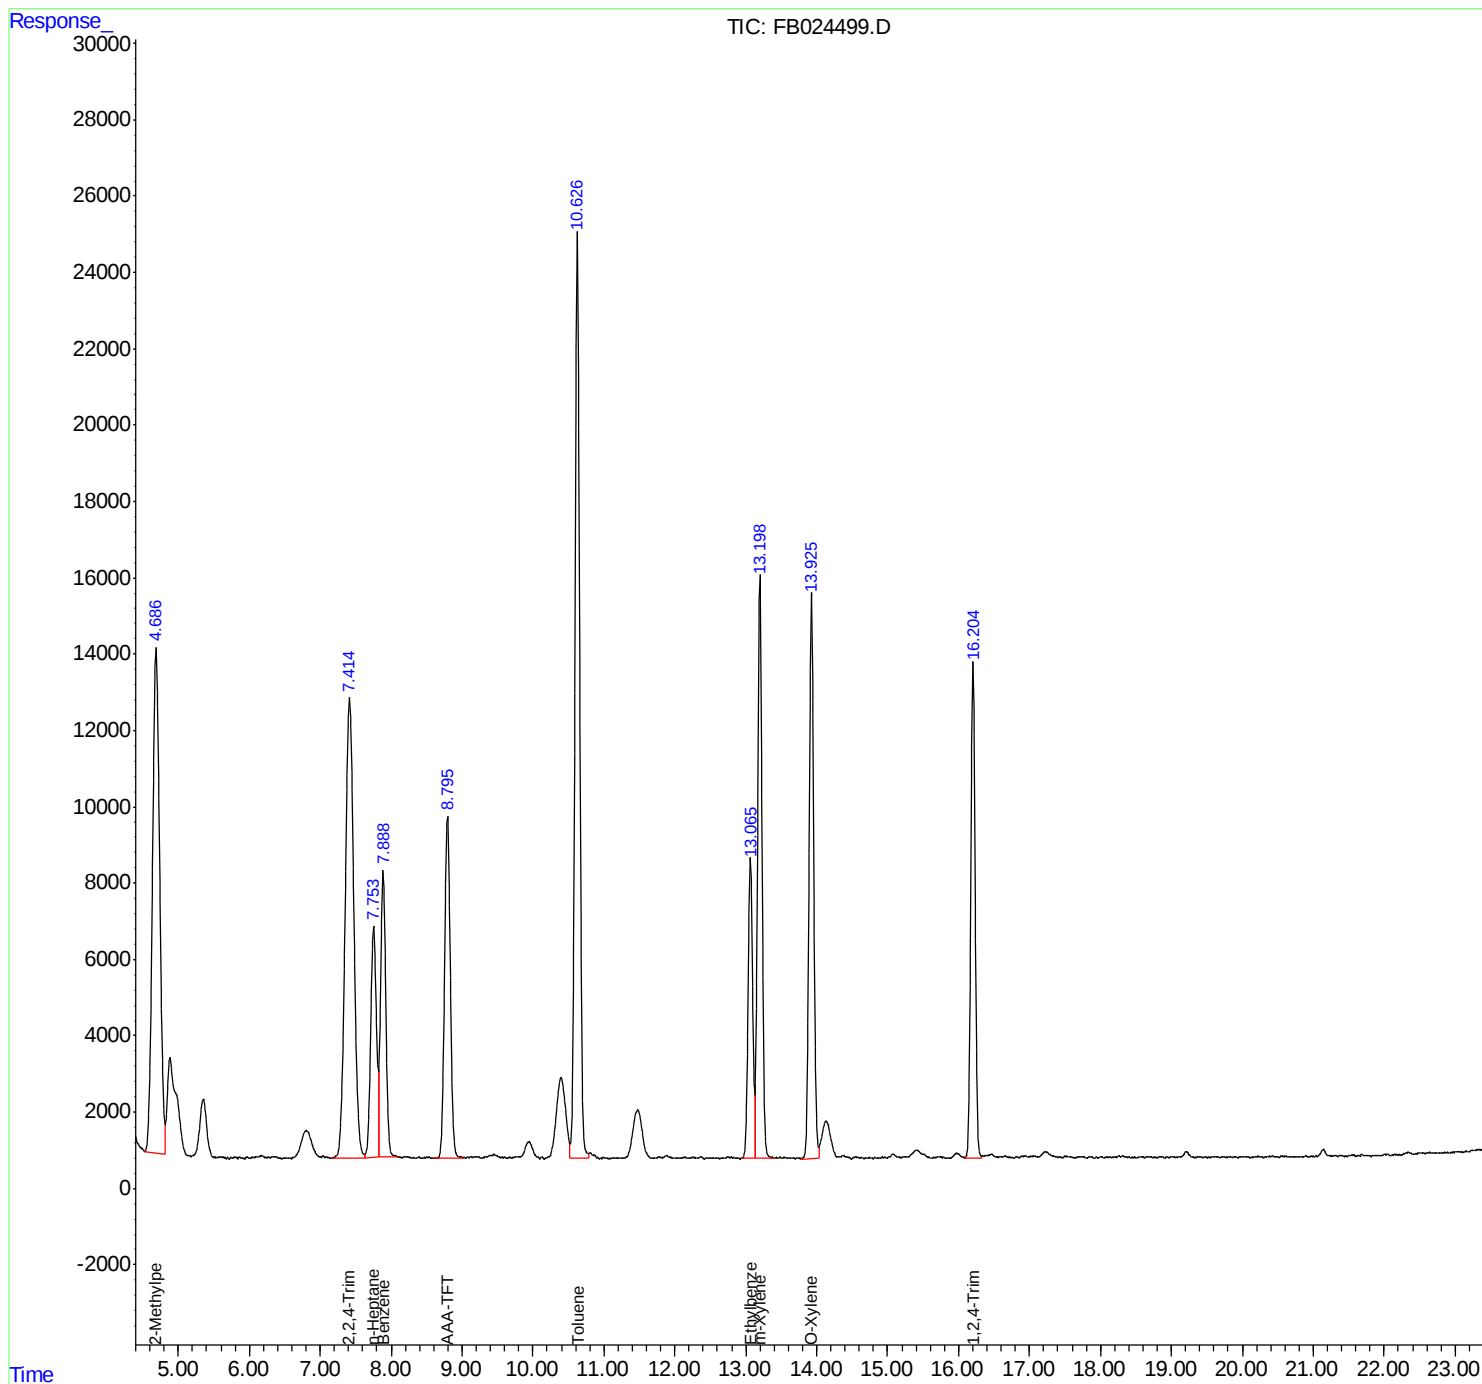

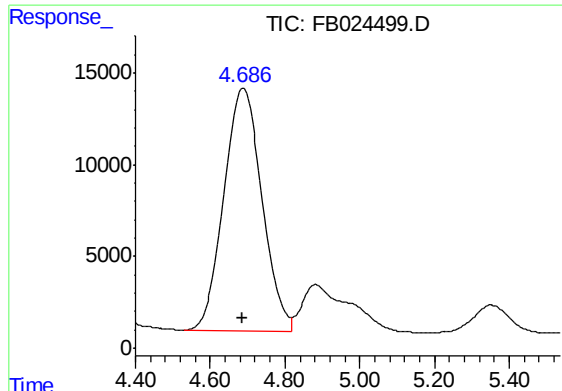


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 937419
Conc: 29.33 ng/ml

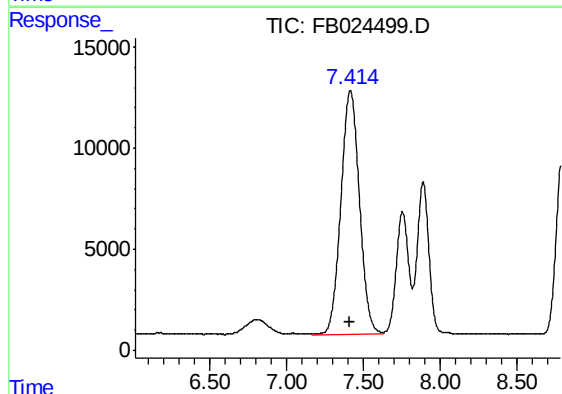


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 1011071
Conc: 30.16 ng/ml

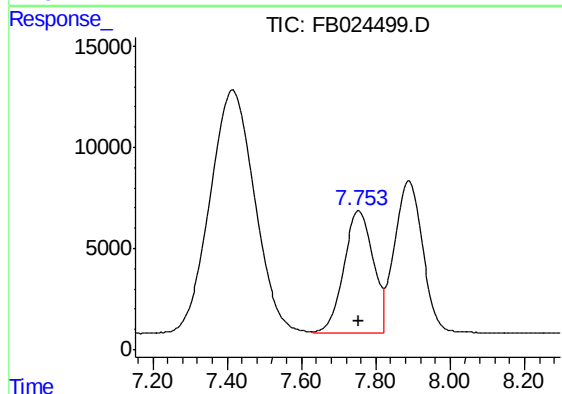


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 333565
Conc: 9.86 ng/ml

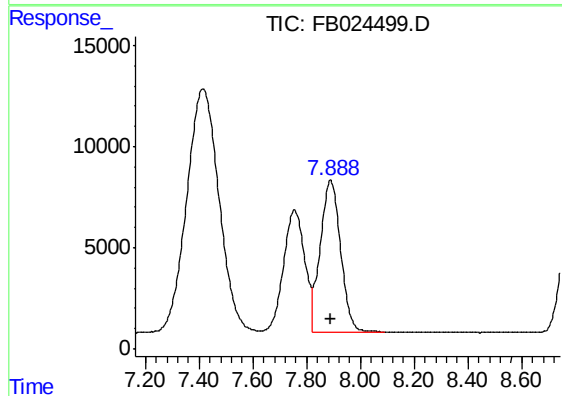


#4 Benzene

R.T.: 7.889 min
Delta R.T.: 0.000 min
Response: 395965
Conc: 9.79 ng/ml

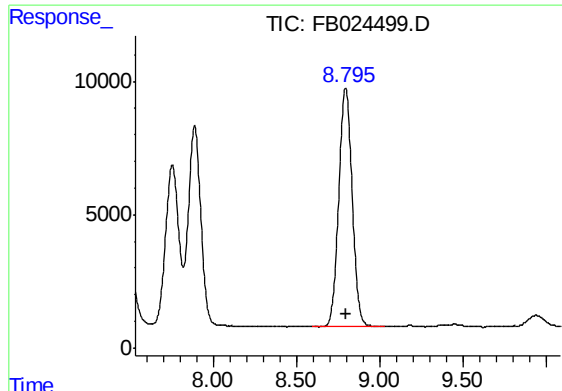


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 499756
Conc: 20.66 ng/ml

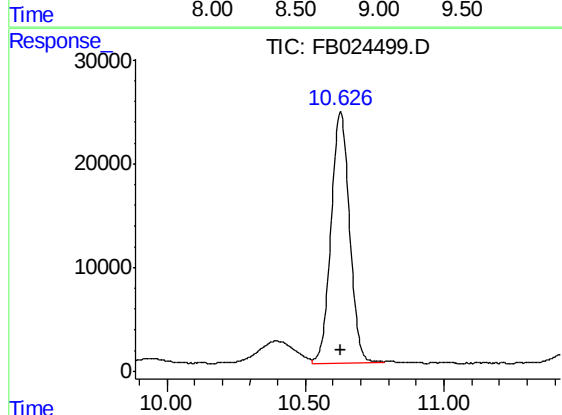


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.001 min
Response: 1125774
Conc: 28.65 ng/ml

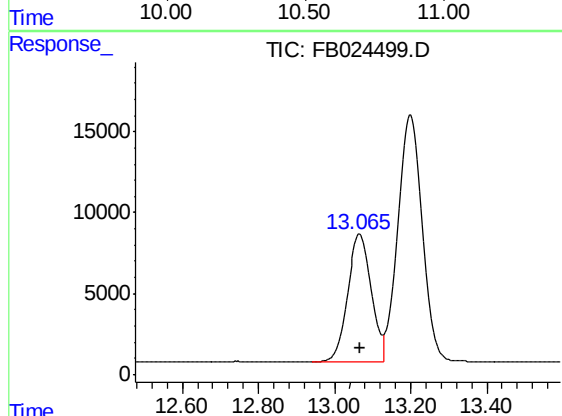


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.001 min
Response: 345033
Conc: 9.83 ng/ml

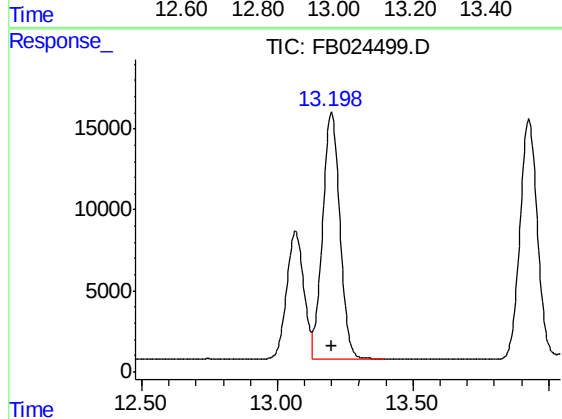


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.001 min
Response: 676068
Conc: 19.74 ng/ml

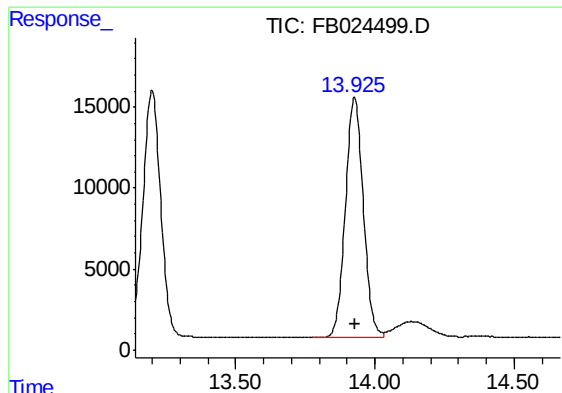

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.002 min
Response: 661594
Conc: 19.73 ng/ml

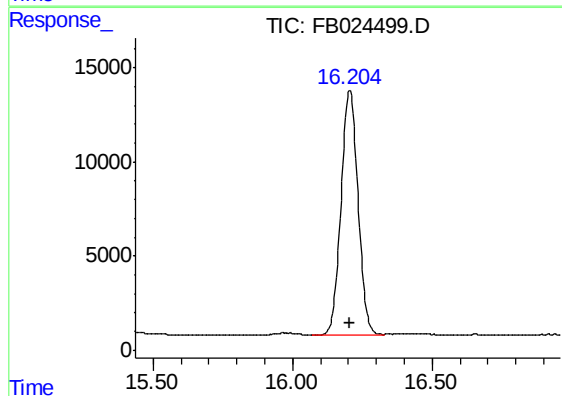

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.002 min
Response: 551420
Conc: 19.86 ng/ml