

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062520\
 Data File : FB024504.D
 Signal(s) : FID2B.CH
 Acq On : 25 Jun 2020 13:10
 Operator : DD/AJ
 Sample : L2815-12MSD
 Misc : 5.03gm/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 26 00:59:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	480638	19.866 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	763282	23.880 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	728764	21.739 ng/ml
3) t n-Heptane	7.757	237775	7.031 ng/ml
4) t Benzene	7.890	385563	9.538 ng/ml
6) t Toluene	10.629	1043122	26.544 ng/ml
7) t Ethylbenzene	13.069	302074	8.608 ng/ml
8) t m-Xylene	13.202	590657	17.247 ng/ml
9) t O-Xylene	13.929	579603	17.288 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	450308	16.218 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062520\
Data File : FB024504.D
Signal(s) : FID2B.CH
Acq On : 25 Jun 2020 13:10
Operator : DD/AJ
Sample : L2815-12MSD
Misc : 5.03gm/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 26 00:59:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

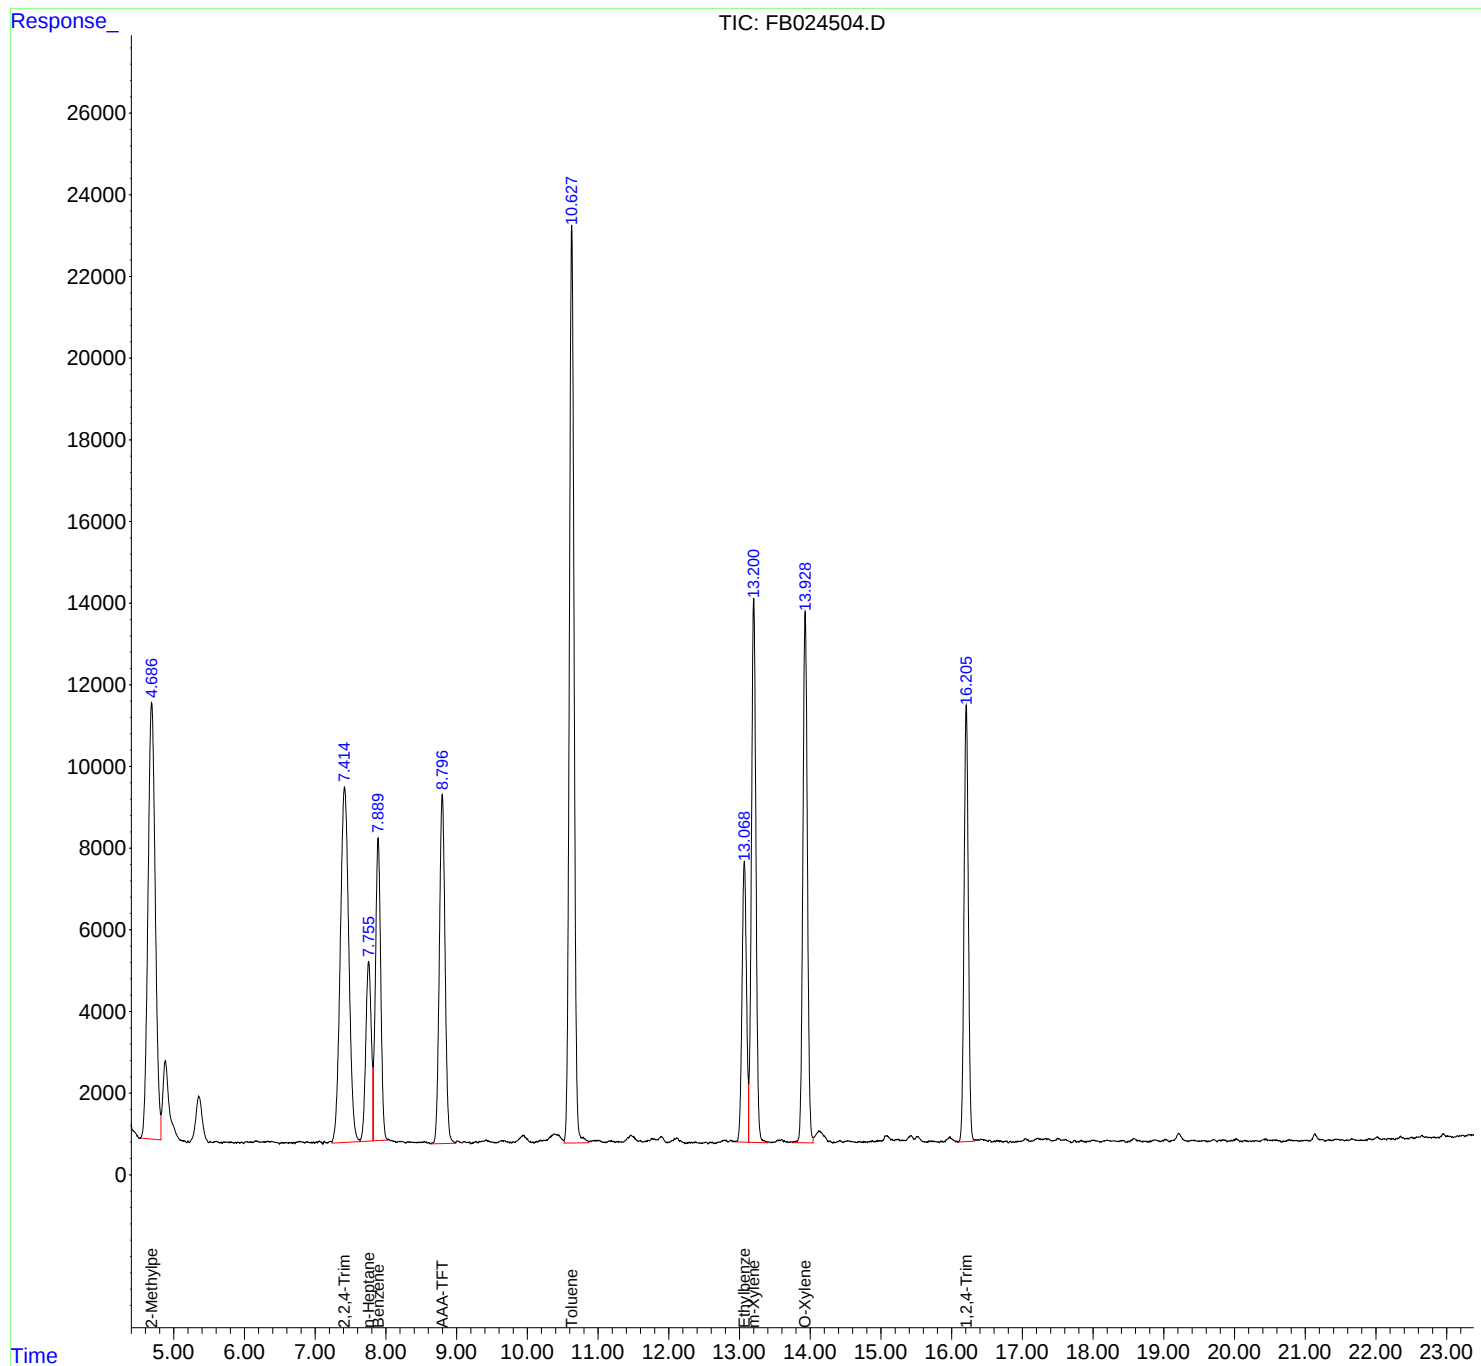

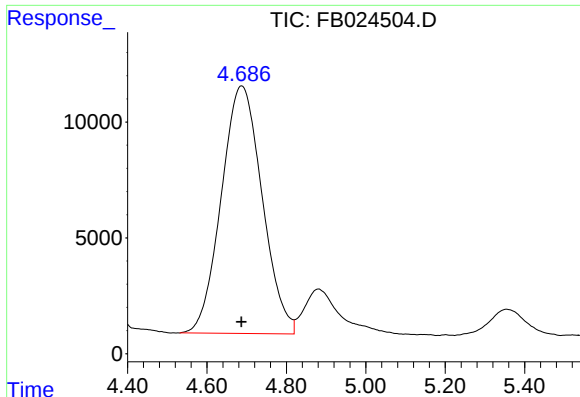


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 763282
Conc: 23.88 ng/ml

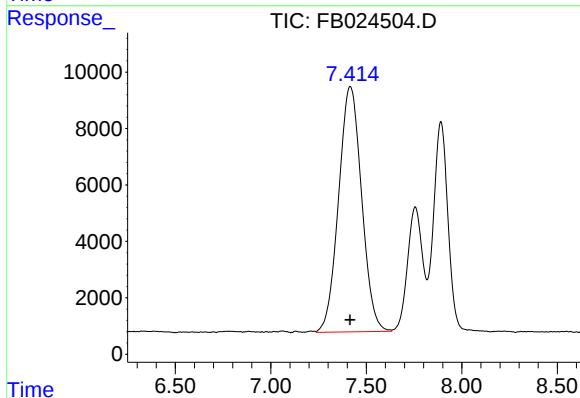


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 728764
Conc: 21.74 ng/ml

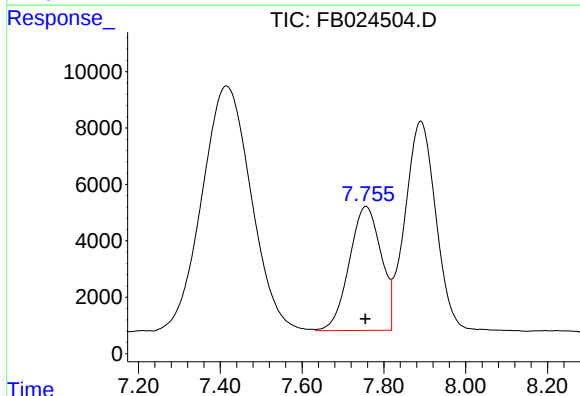


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.002 min
Response: 237775
Conc: 7.03 ng/ml

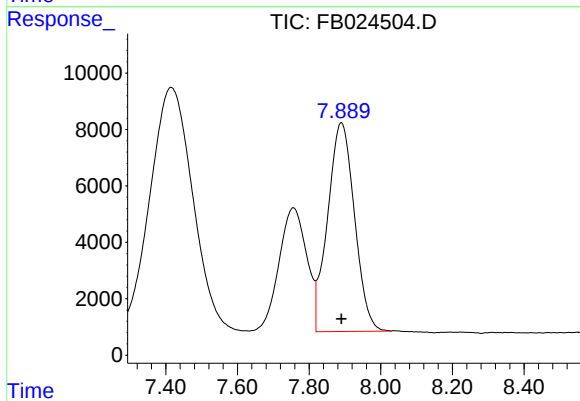


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.000 min
Response: 385563
Conc: 9.54 ng/ml

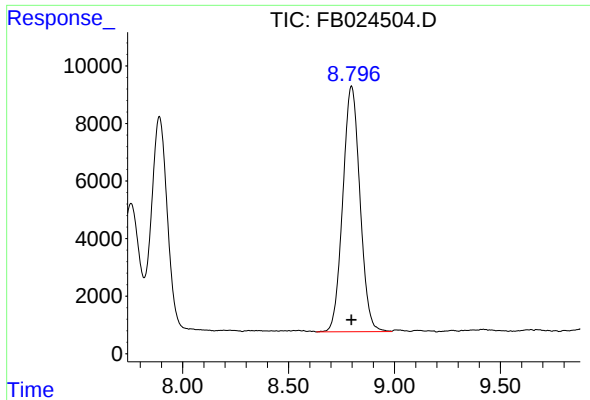


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 480638
Conc: 19.87 ng/ml

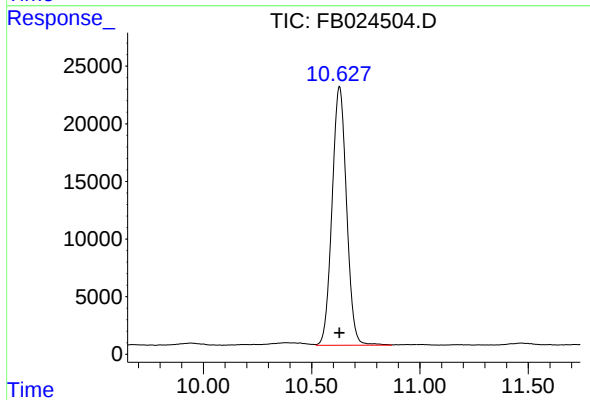


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 1043122
Conc: 26.54 ng/ml

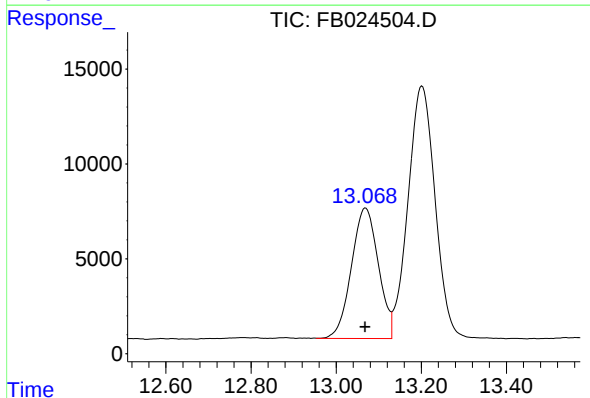


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.001 min
Response: 302074
Conc: 8.61 ng/ml

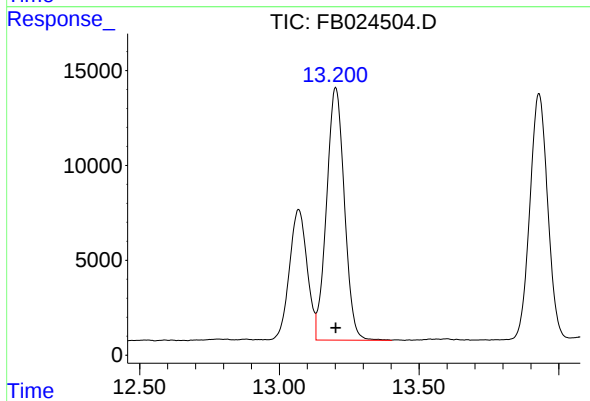


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.000 min
Response: 590657
Conc: 17.25 ng/ml

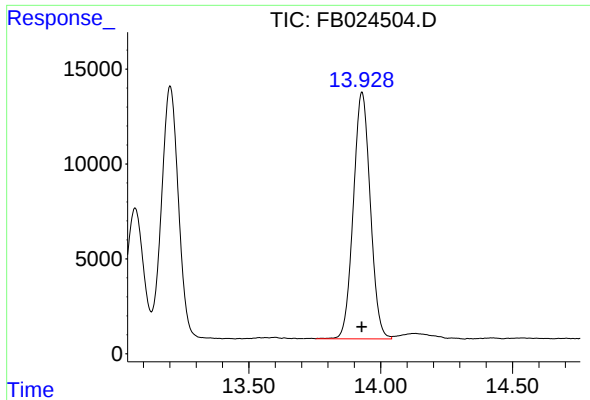

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.000 min
Response: 579603
Conc: 17.29 ng/ml

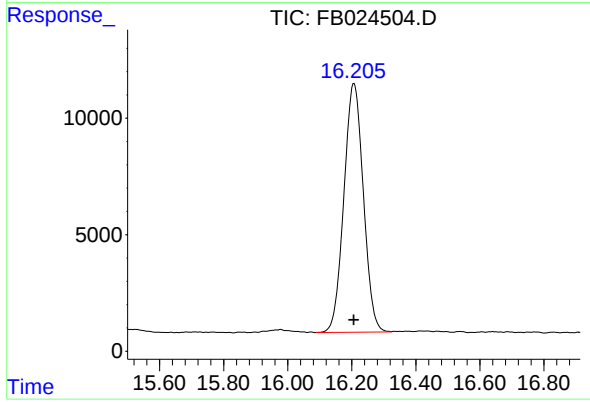

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 450308
Conc: 16.22 ng/ml