

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062619\
 Data File : FB021497.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jun 2019 9:36
 Operator : MJ/SJ
 Sample : BSF0626S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 27 07:26:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 15:15:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.988	271910	19.666 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.860	1005668	29.460 ng/ml
2) t	2,2,4-Trimethylpentane	7.608	924355	29.912 ng/ml
3) t	n-Heptane	7.947	289958	9.907 ng/ml
4) t	Benzene	8.082	330263	9.840 ng/ml
6) t	Toluene	10.829	681093	29.817 ng/ml
7) t	Ethylbenzene	13.274	243747	10.296 ng/ml
8) t	m-Xylene	13.407	519354	20.491 ng/ml
9) t	O-Xylene	14.136	538996	20.551 ng/ml
10) t	1,2,4-Trimethylbenzene	16.415	539559	20.536 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062619\
Data File : FB021497.D
Signal(s) : FID2B.CH
Acq On : 26 Jun 2019 9:36
Operator : MJ/SJ
Sample : BSF0626S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 27 07:26:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 15:15:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

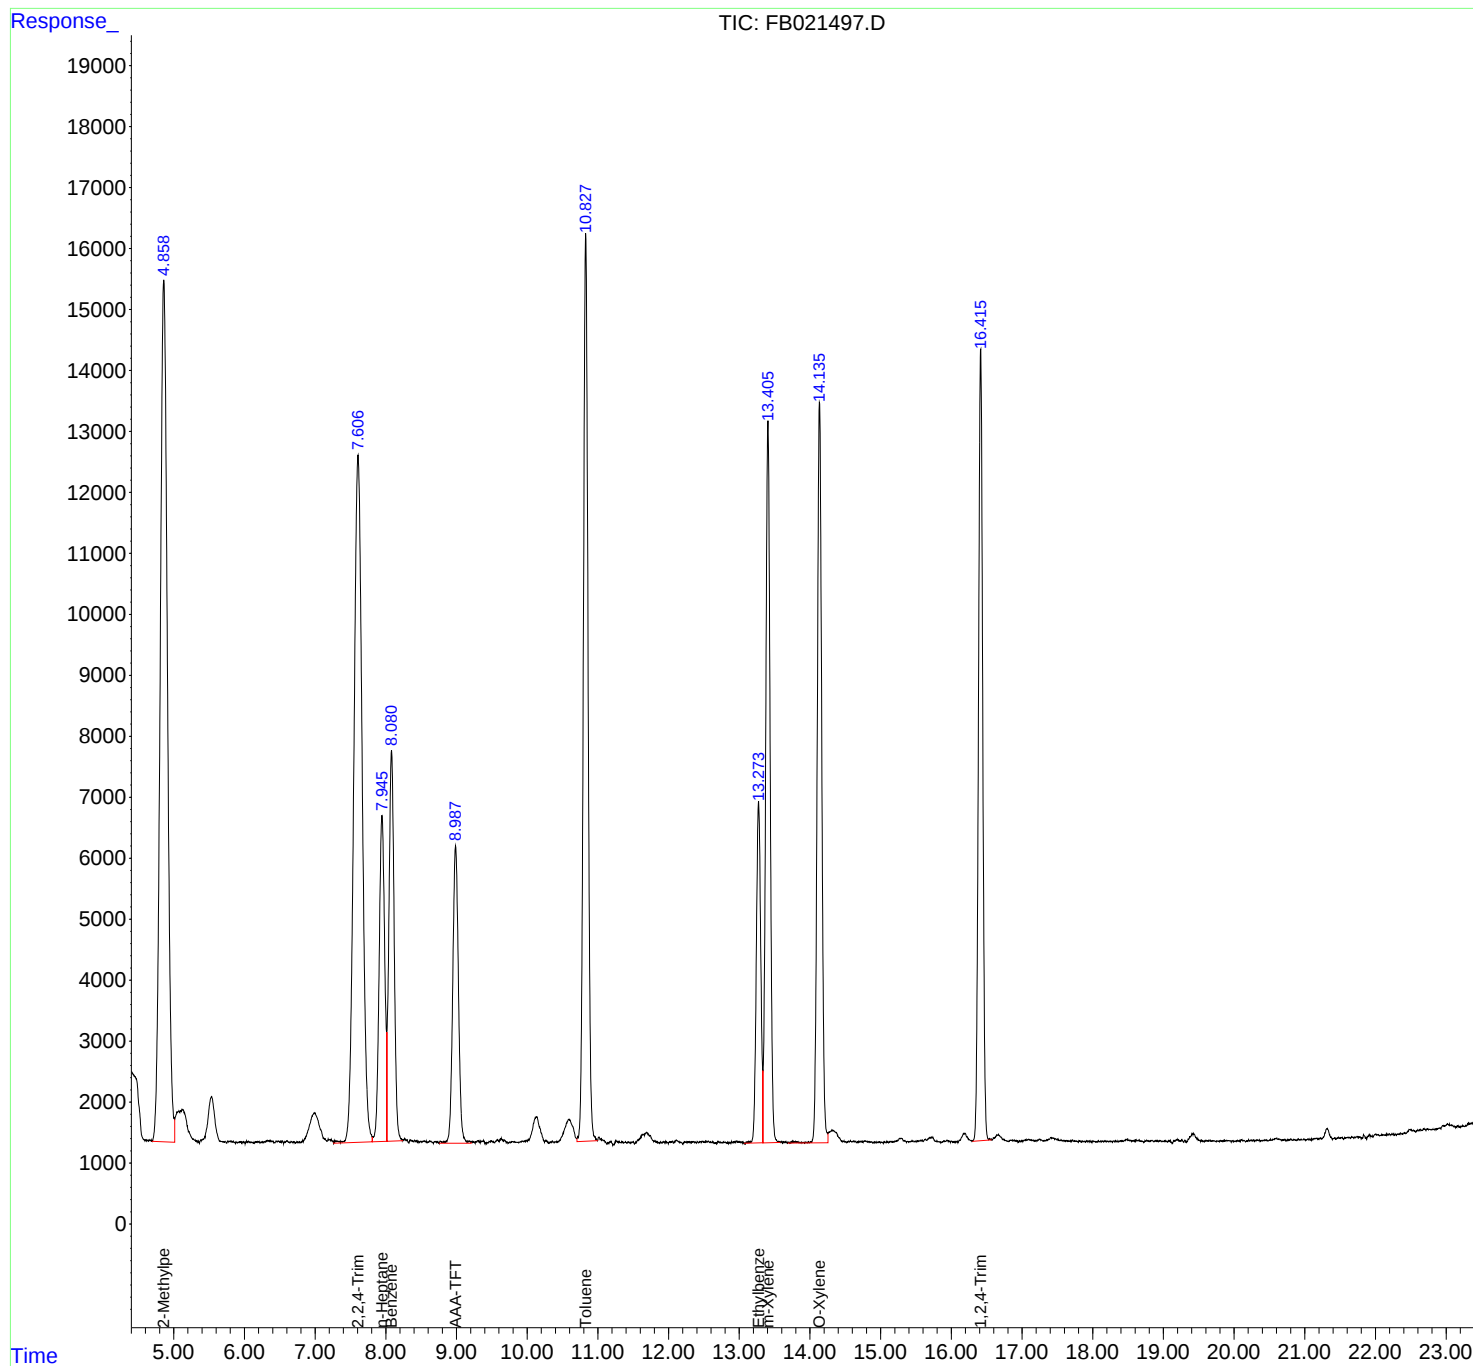

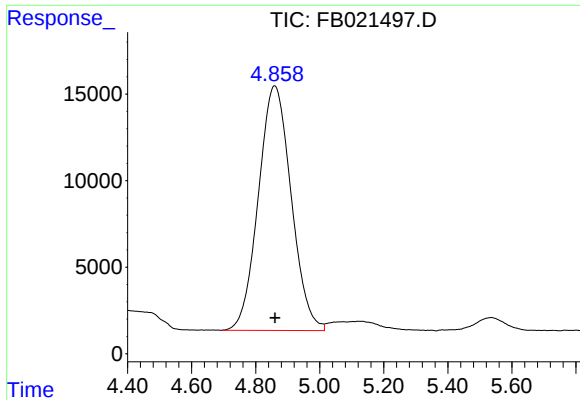


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: -0.001 min
Response: 1005668
Conc: 29.46 ng/ml

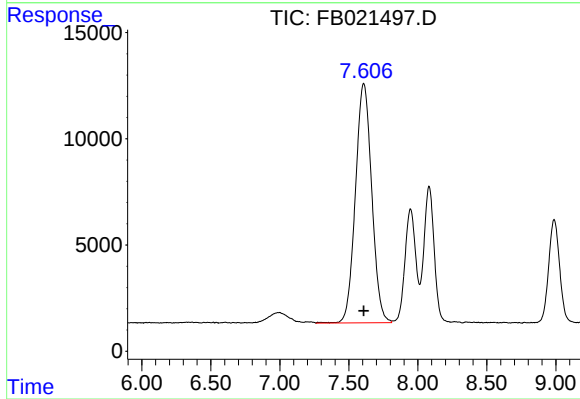


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 924355
Conc: 29.91 ng/ml

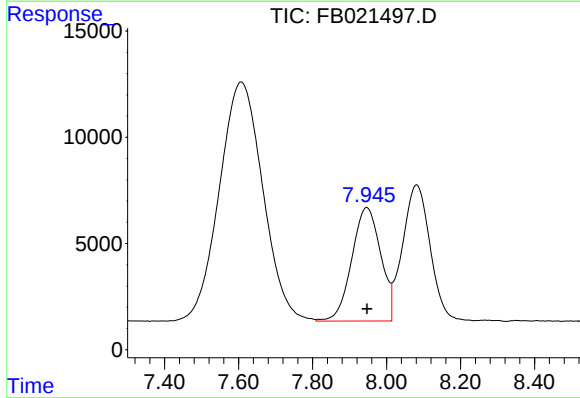


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 289958
Conc: 9.91 ng/ml

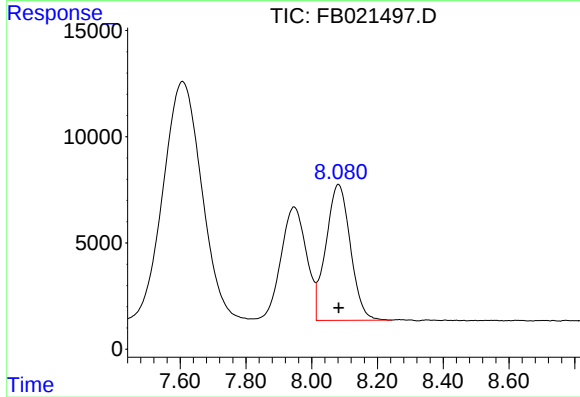


#4 Benzene

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 330263
Conc: 9.84 ng/ml

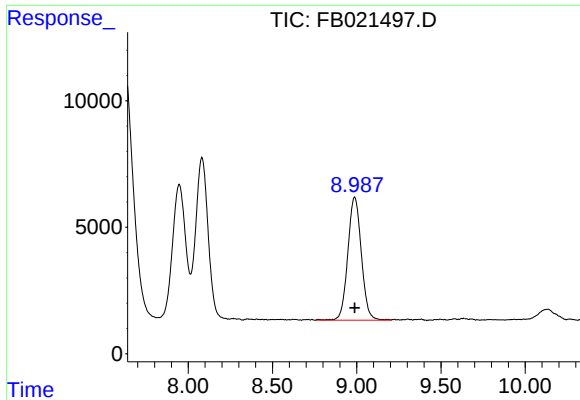


#5 AAA-TFT

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 271910
Conc: 19.67 ng/ml

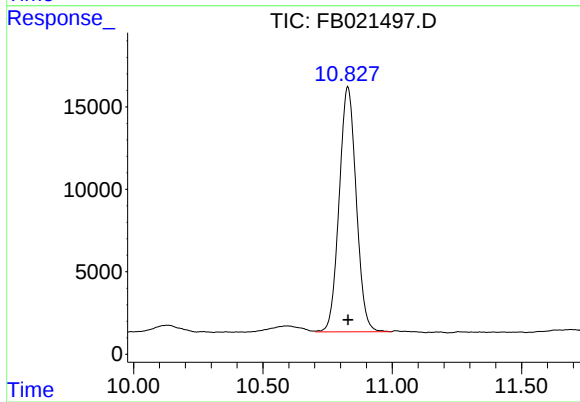


#6 Toluene

R.T.: 10.829 min
Delta R.T.: -0.001 min
Response: 681093
Conc: 29.82 ng/ml

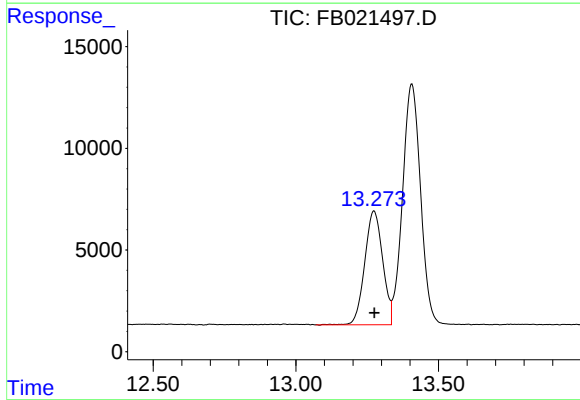


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: -0.001 min
Response: 243747
Conc: 10.30 ng/ml

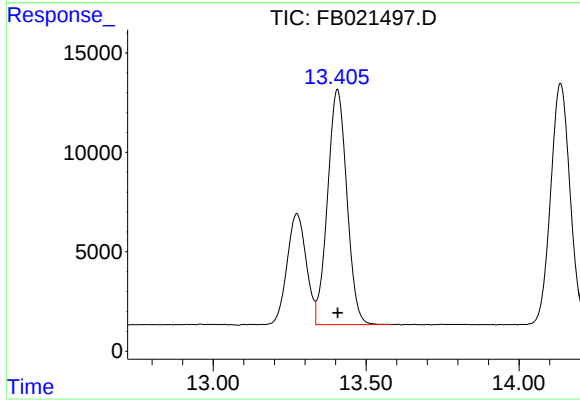


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: -0.001 min
Response: 519354
Conc: 20.49 ng/ml

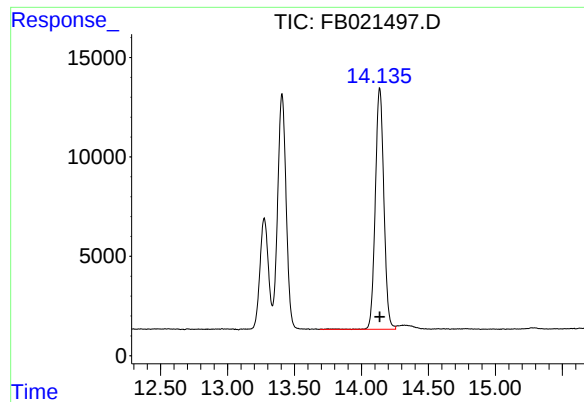

#9 O-Xylene

R.T.: 14.136 min
Delta R.T.: -0.001 min
Response: 538996
Conc: 20.55 ng/ml

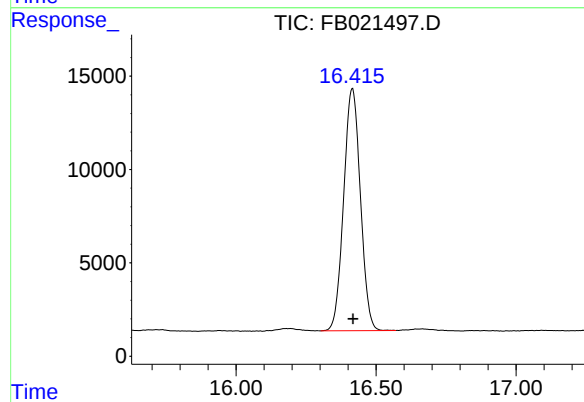

#10 1,2,4-Trimethylbenzene

R.T.: 16.415 min
Delta R.T.: -0.002 min
Response: 539559
Conc: 20.54 ng/ml