

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062619\
 Data File : FB021500.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jun 2019 11:23
 Operator : MJ/SJ
 Sample : K3526-04MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 27 07:26:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 15:15:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	271871	19.663 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	995296	29.156 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	906065	29.320 ng/ml
3) t n-Heptane	7.947	284964	9.736 ng/ml
4) t Benzene	8.082	333622	9.940 ng/ml
6) t Toluene	10.829	693828	30.374 ng/ml
7) t Ethylbenzene	13.274	251515	10.624 ng/ml
8) t m-Xylene	13.406	535363	21.122 ng/ml
9) t O-Xylene	14.136	547978	20.894 ng/ml
10) t 1,2,4-Trimethylbenzene	16.416	544778	20.735 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062619\
Data File : FB021500.D
Signal(s) : FID2B.CH
Acq On : 26 Jun 2019 11:23
Operator : MJ/SJ
Sample : K3526-04MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 27 07:26:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 15:15:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

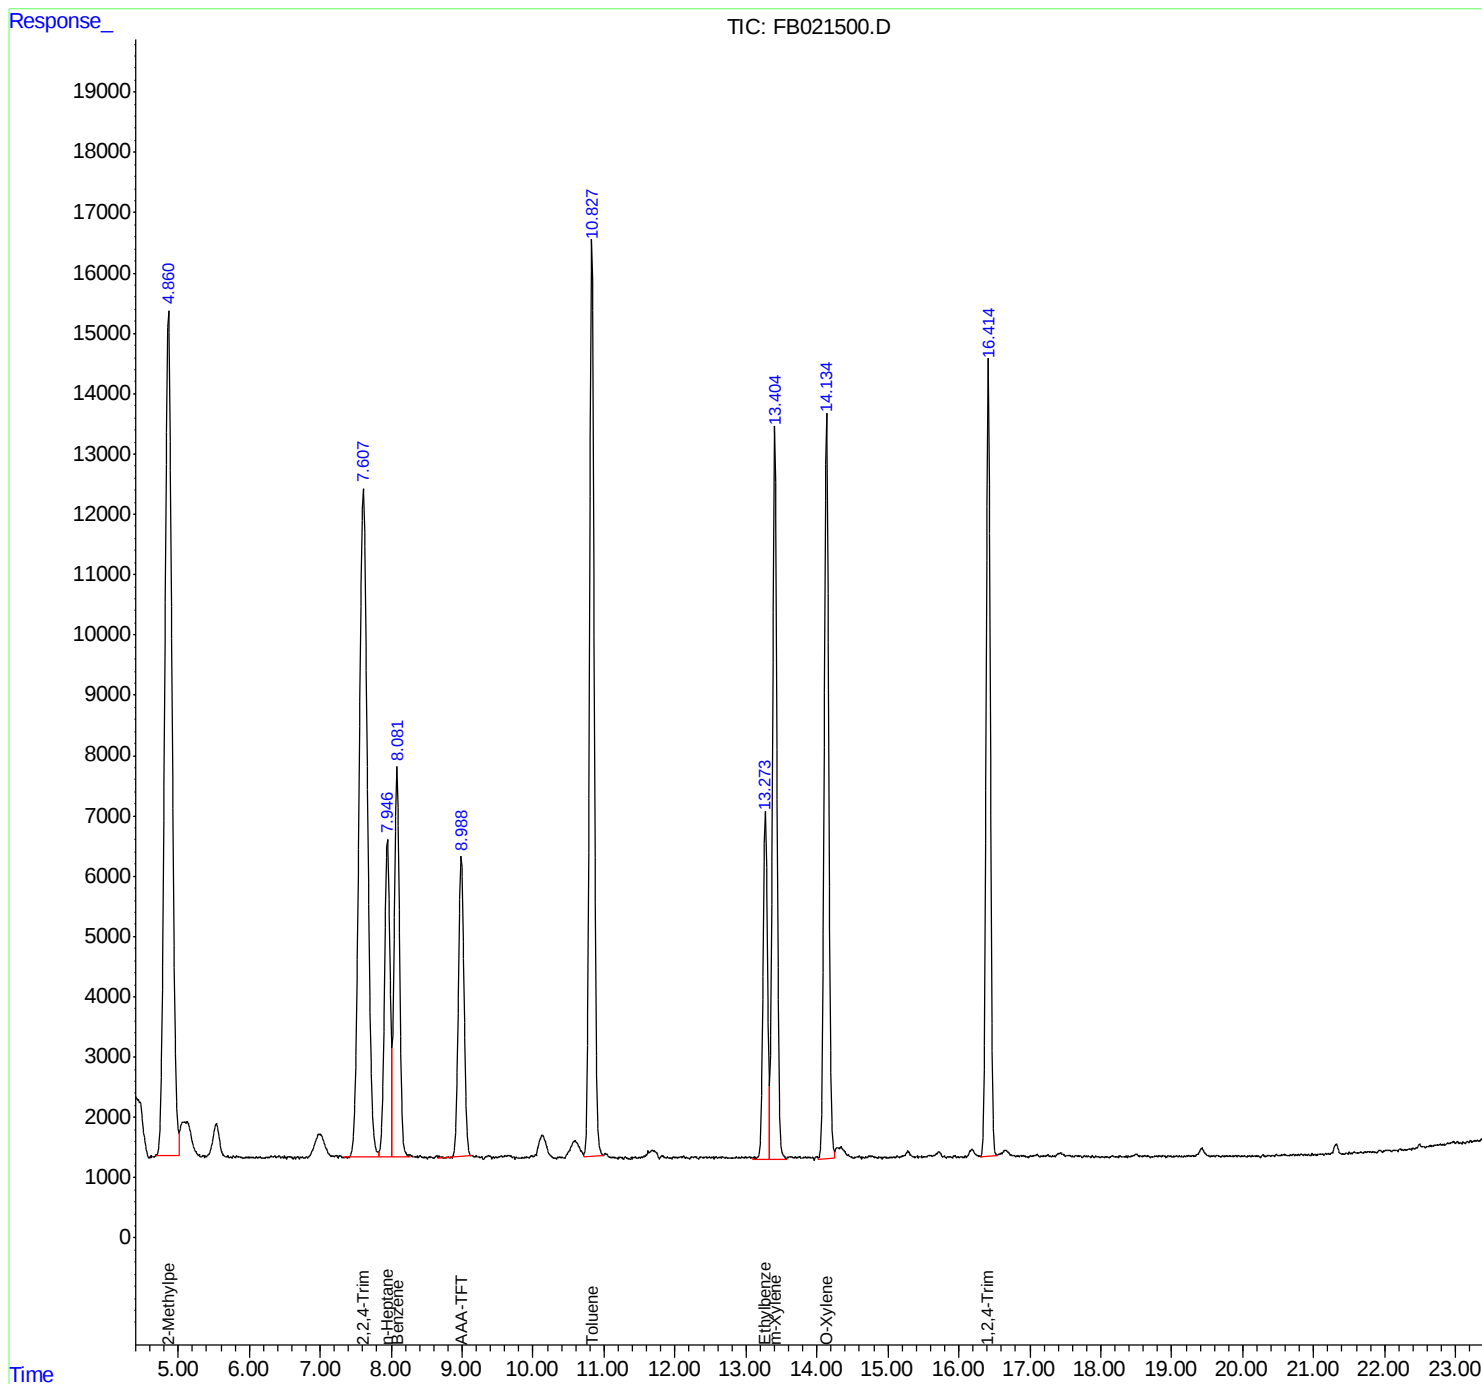

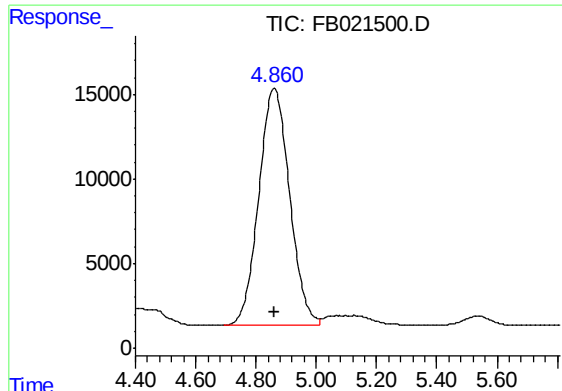


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 995296
Conc: 29.16 ng/ml

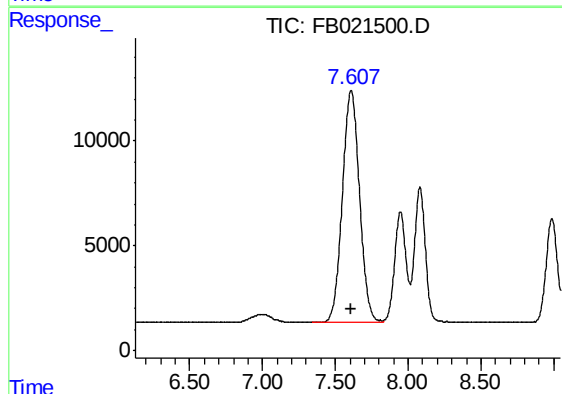


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 906065
Conc: 29.32 ng/ml

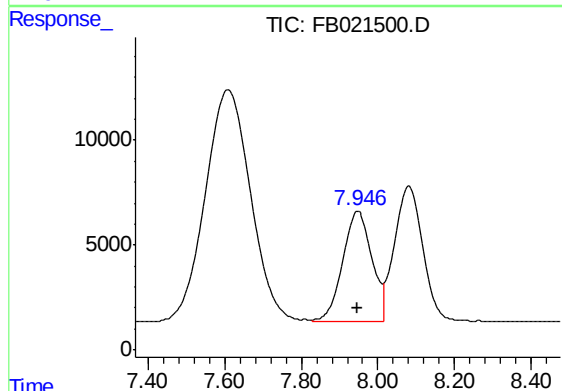


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 284964
Conc: 9.74 ng/ml

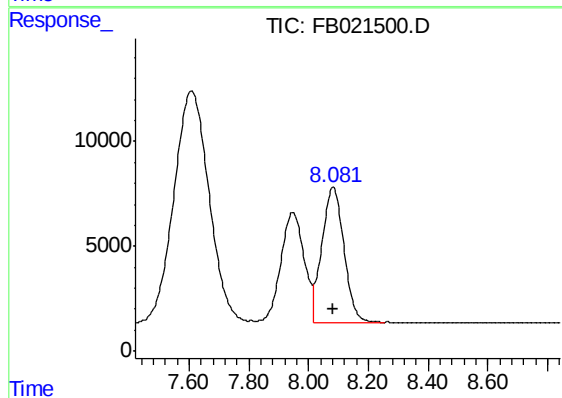


#4 Benzene

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 333622
Conc: 9.94 ng/ml

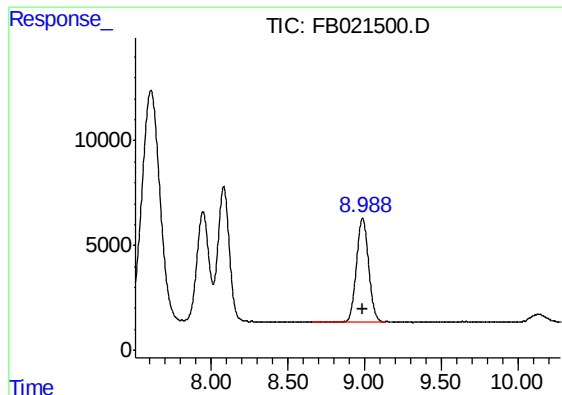


#5 AAA-TFT

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 271871
Conc: 19.66 ng/ml

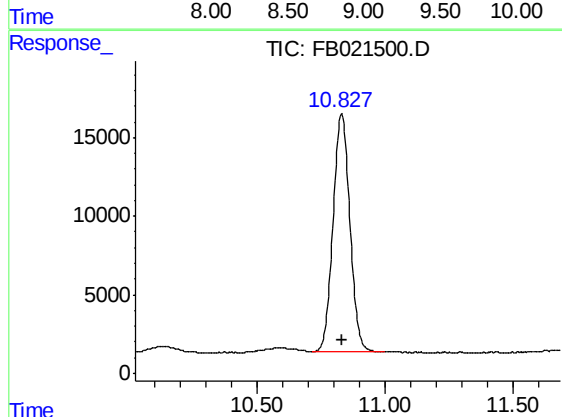


#6 Toluene

R.T.: 10.829 min
Delta R.T.: 0.000 min
Response: 693828
Conc: 30.37 ng/ml

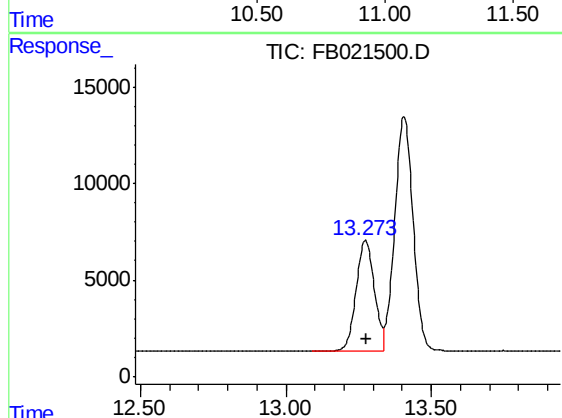


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: 0.000 min
Response: 251515
Conc: 10.62 ng/ml

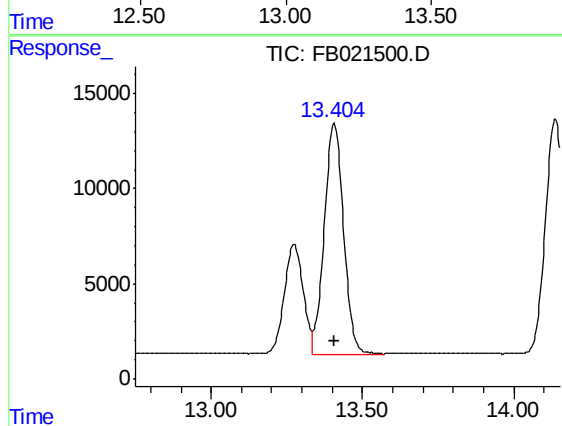


#8 m-Xylene

R.T.: 13.406 min
Delta R.T.: -0.001 min
Response: 535363
Conc: 21.12 ng/ml

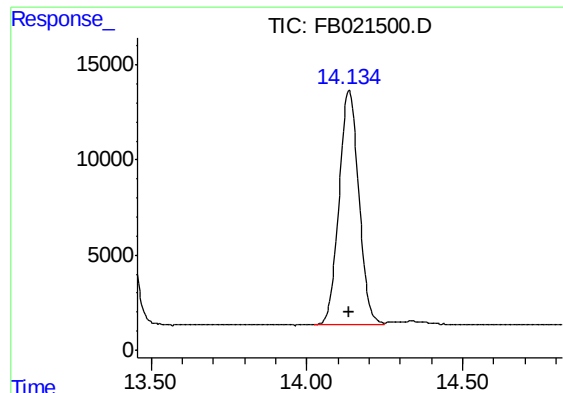

#9 O-Xylene

R.T.: 14.136 min
Delta R.T.: -0.001 min
Response: 547978
Conc: 20.89 ng/ml

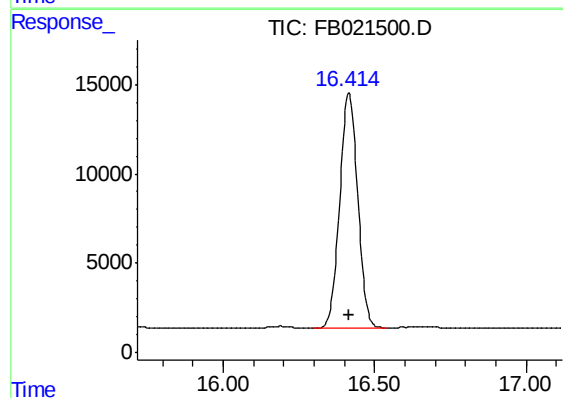

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: -0.002 min
Response: 544778
Conc: 20.73 ng/ml