

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062623\
 Data File : FB030116.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jun 2023 12:00
 Operator : YP/AJ
 Sample : 10 GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 26 12:48:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 12:48:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	127339	9.349 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	286841	15.595 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	314468	14.912 ng/ml
3) t n-Heptane	7.750	99500	5.052 ng/ml
4) t Benzene	7.885	118879	5.064 ng/ml
6) t Toluene	10.618	346750	15.000 ng/ml
7) t Ethylbenzene	13.055	109742	4.883 ng/ml
8) t m-Xylene	13.187	224667	9.792 ng/ml
9) t O-Xylene	13.914	223614	9.539 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	231154	9.417 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062623\
Data File : FB030116.D
Signal(s) : FID2B.CH
Acq On : 26 Jun 2023 12:00
Operator : YP/AJ
Sample : 10 GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 26 12:48:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 12:48:05 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

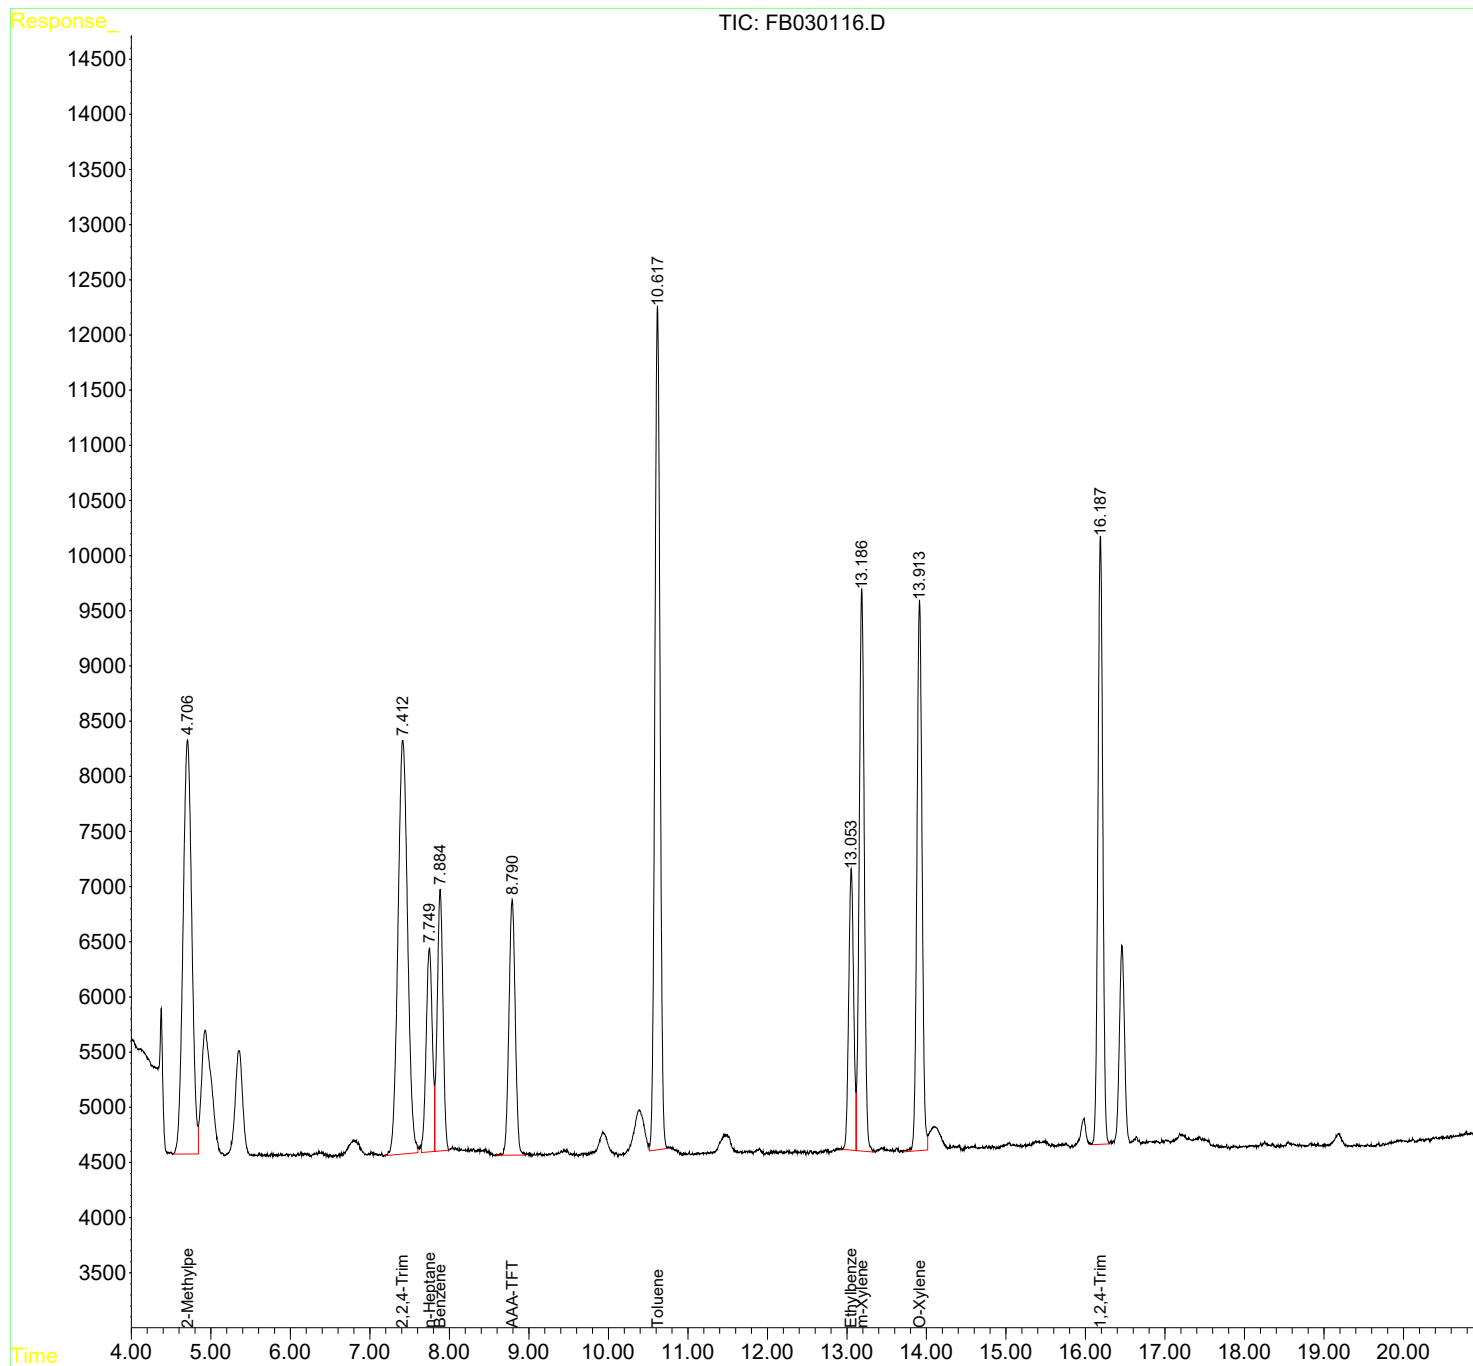

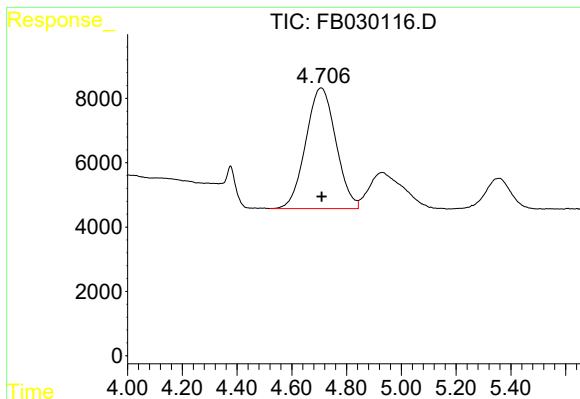


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: -0.001 min
Response: 286841
Conc: 15.59 ng/ml

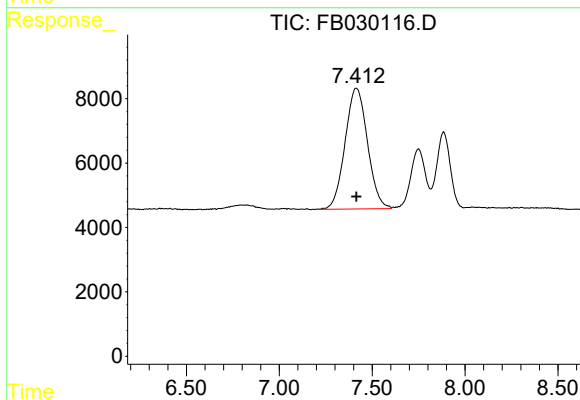


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.002 min
Response: 314468
Conc: 14.91 ng/ml

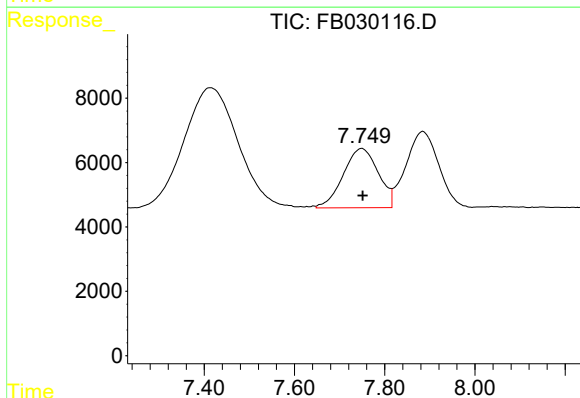


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.001 min
Response: 99500
Conc: 5.05 ng/ml

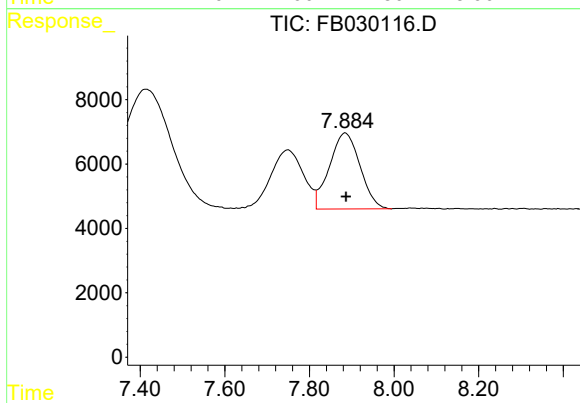


#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 118879
Conc: 5.06 ng/ml

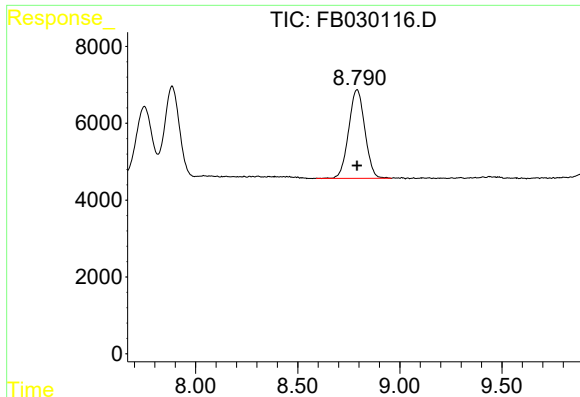


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 127339
Conc: 9.35 ng/ml

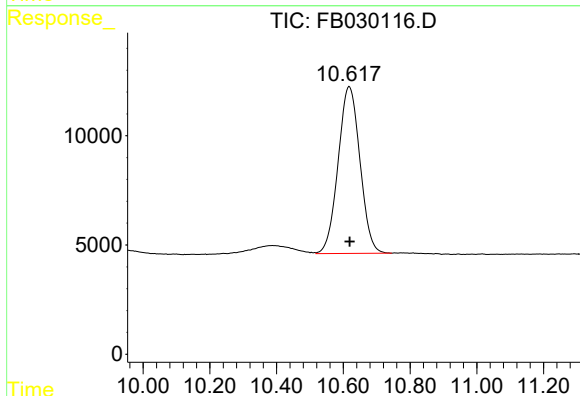


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.001 min
Response: 346750
Conc: 15.00 ng/ml

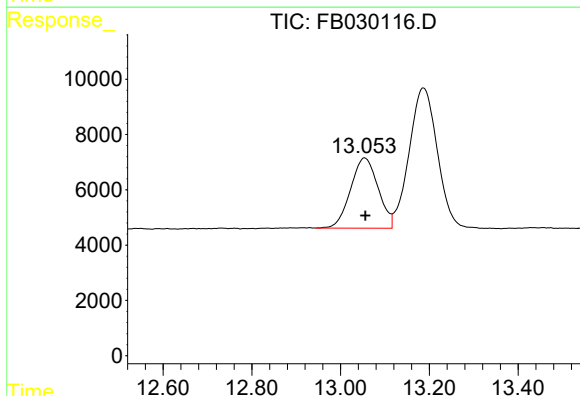


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.002 min
Response: 109742
Conc: 4.88 ng/ml

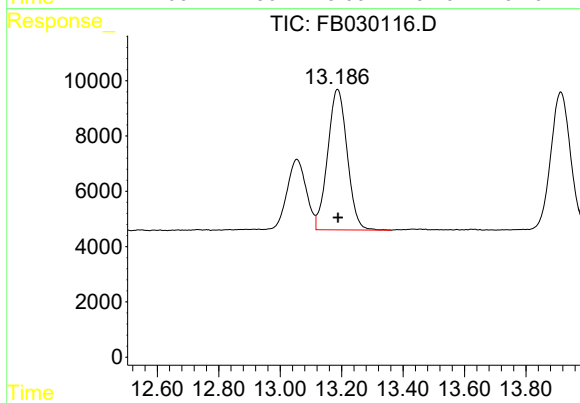


#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.002 min
Response: 224667
Conc: 9.79 ng/ml

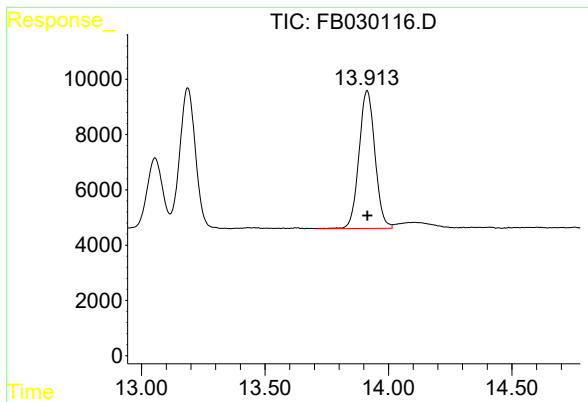

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.001 min
Response: 223614
Conc: 9.54 ng/ml

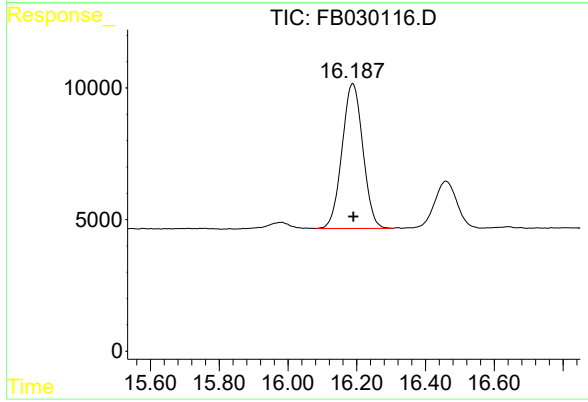

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.001 min
Response: 231154
Conc: 9.42 ng/ml