

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062623\
 Data File : FB030120.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jun 2023 15:03
 Operator : YP/AJ
 Sample : FB062623GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 26 15:24:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
 Quant Title :
 QLast Update : Mon Jun 26 14:31:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	219770	16.724 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	593617	31.577 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	635427	30.218 ng/ml
3) t n-Heptane	7.751	228754	11.211 ng/ml
4) t Benzene	7.888	262622	10.716 ng/ml
6) t Toluene	10.620	756821	31.895 ng/ml
7) t Ethylbenzene	13.056	234667	10.427 ng/ml
8) t m-Xylene	13.189	467128	20.541 ng/ml
9) t O-Xylene	13.916	453251	19.992 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	435990	19.064 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062623\
Data File : FB030120.D
Signal(s) : FID2B.CH
Acq On : 26 Jun 2023 15:03
Operator : YP/AJ
Sample : FB062623GR0ICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 26 15:24:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062623.M
Quant Title :
QLast Update : Mon Jun 26 14:31:24 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

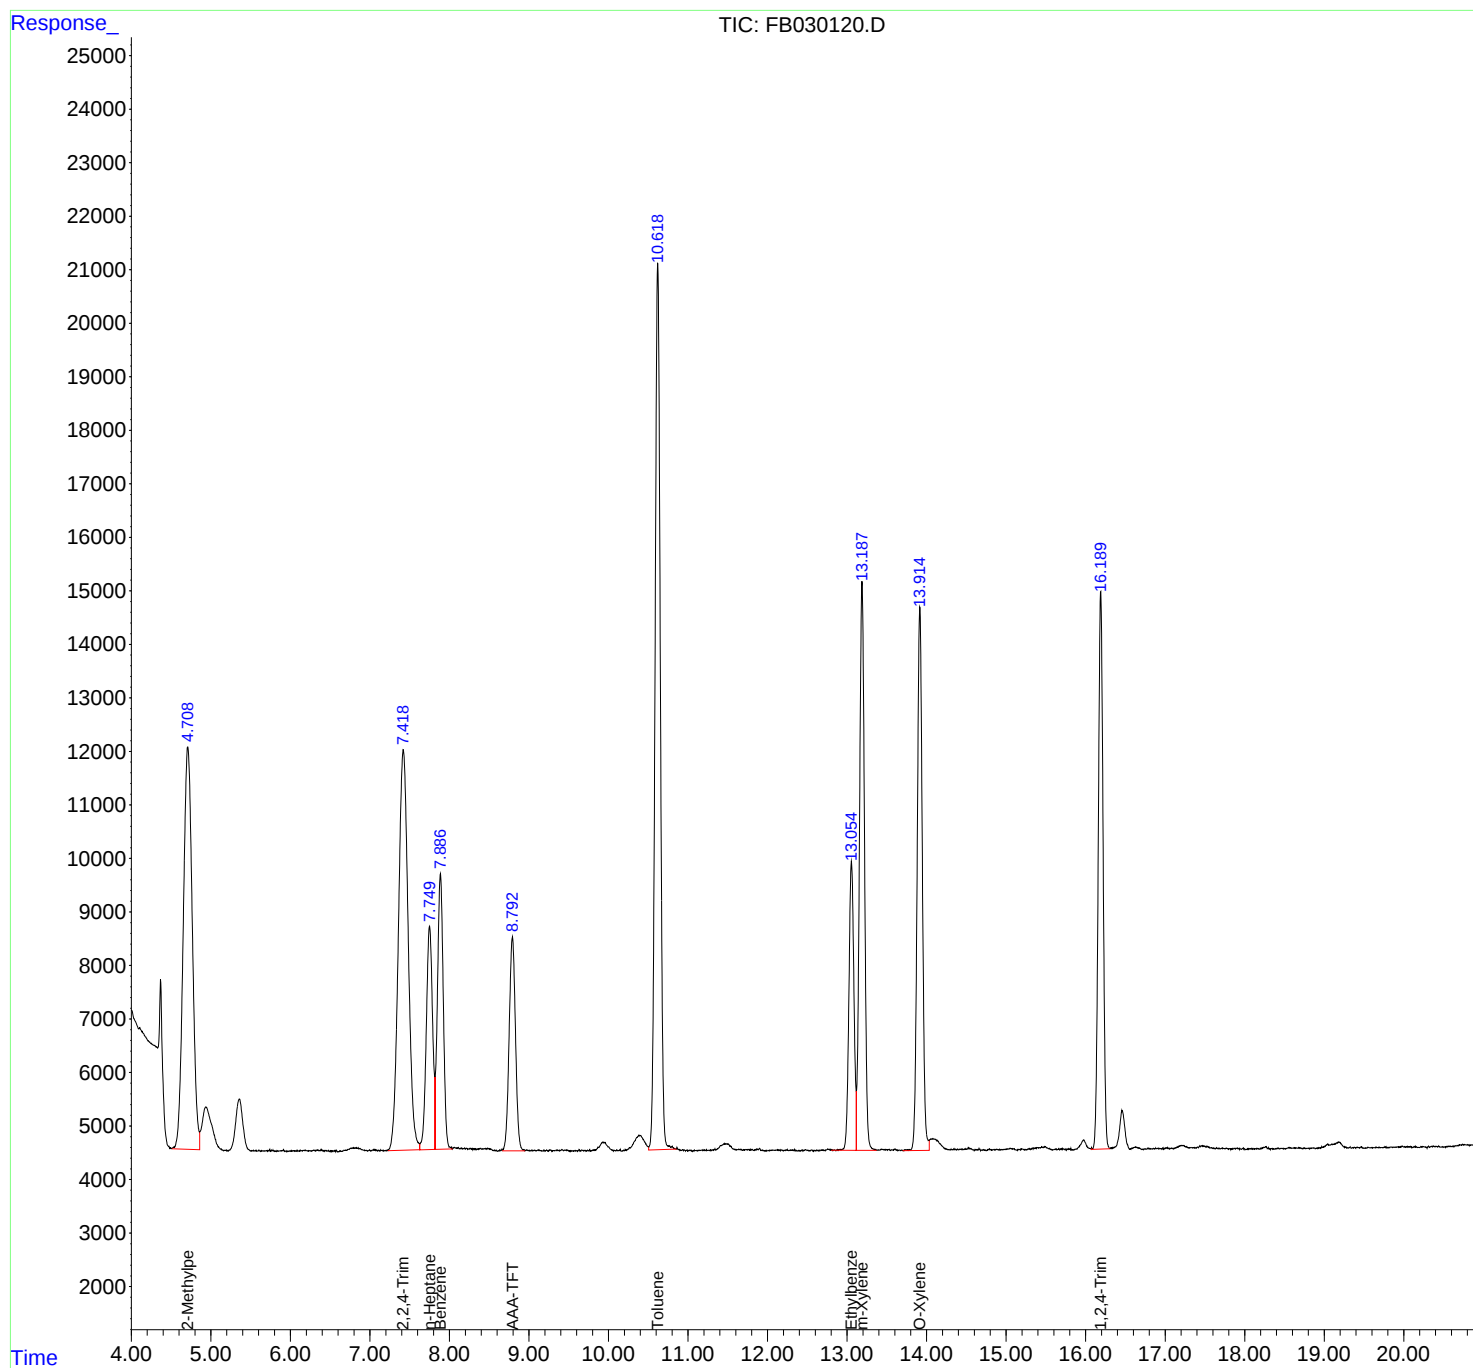

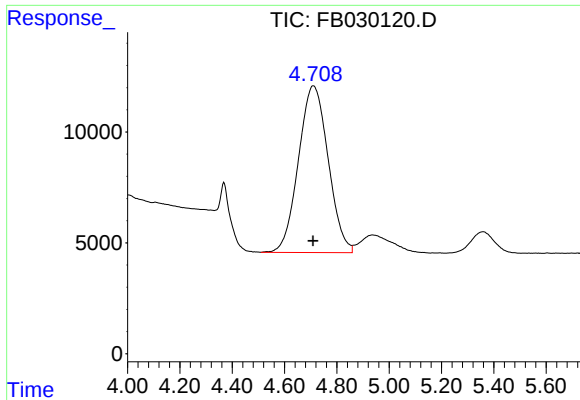


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 593617
Conc: 31.58 ng/ml

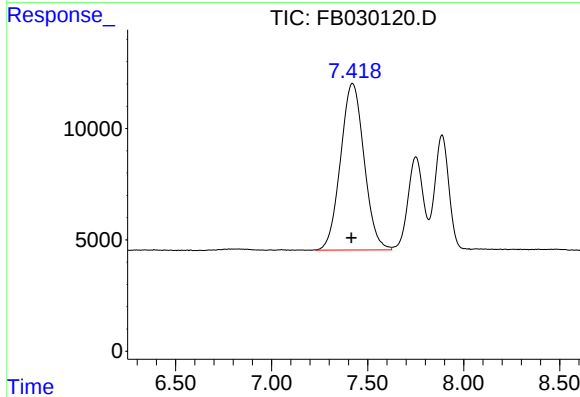


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.004 min
Response: 635427
Conc: 30.22 ng/ml

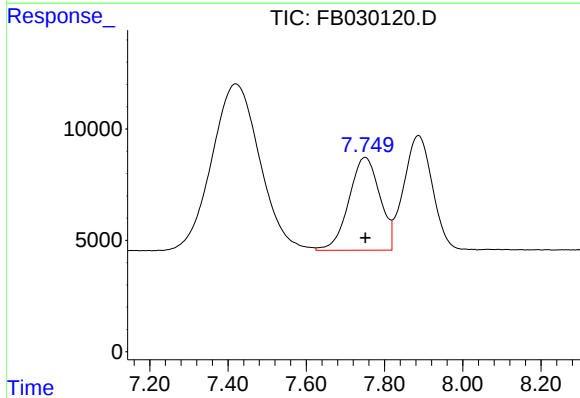


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 228754
Conc: 11.21 ng/ml

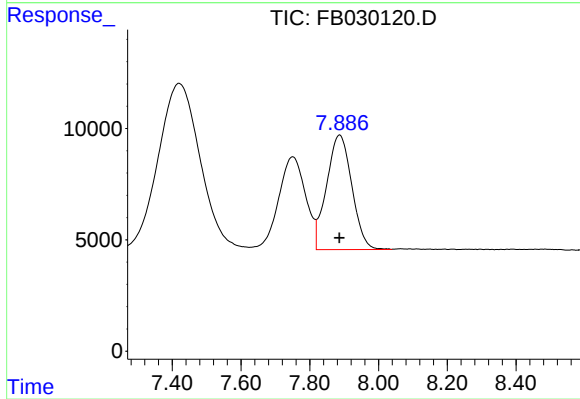


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 262622
Conc: 10.72 ng/ml

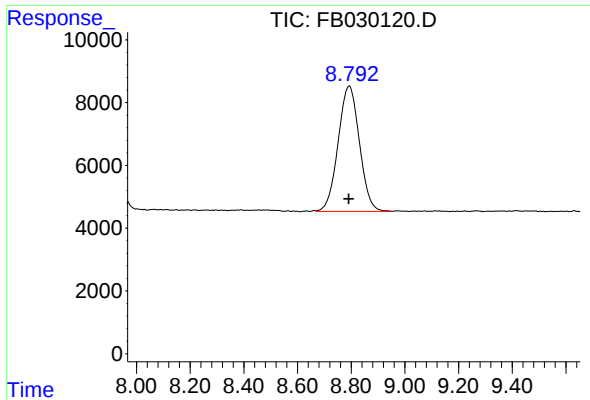


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 219770
Conc: 16.72 ng/ml

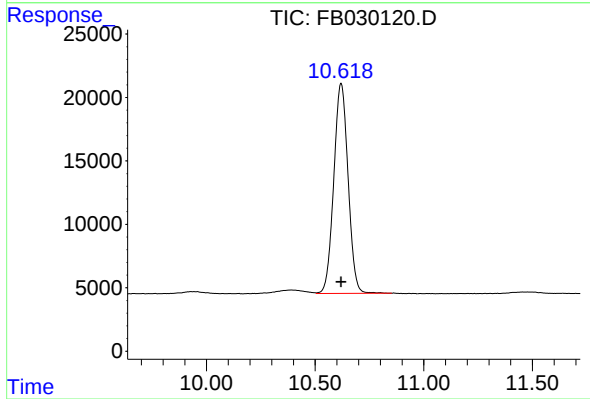


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 756821
Conc: 31.90 ng/ml

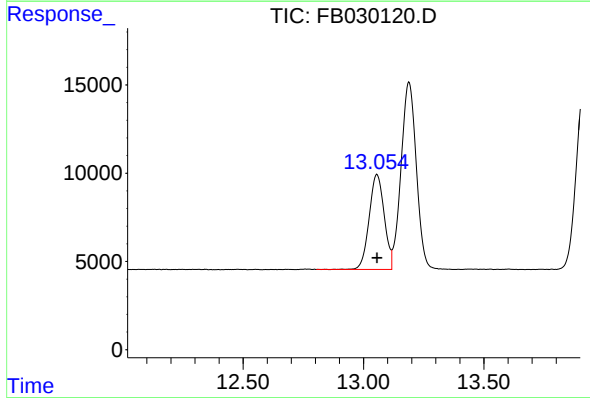


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 234667
Conc: 10.43 ng/ml

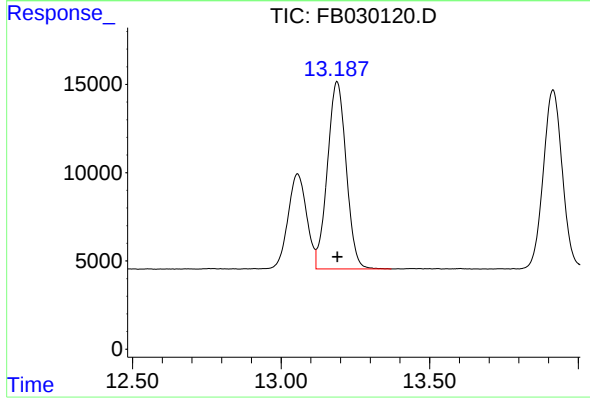

#8 m-Xylene

R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 467128
Conc: 20.54 ng/ml

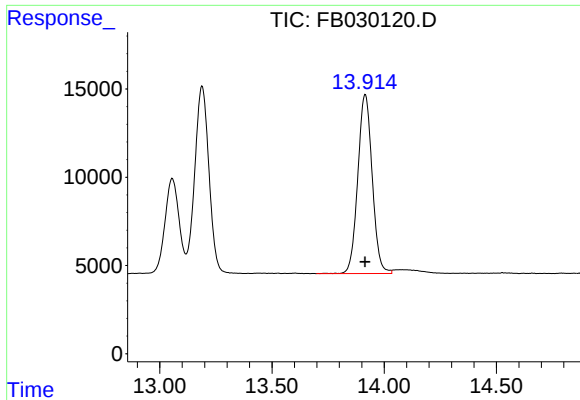


#9 O-Xylene

R.T.: 13.916 min

Delta R.T.: 0.000 min

Response: 453251

Conc: 19.99 ng/ml

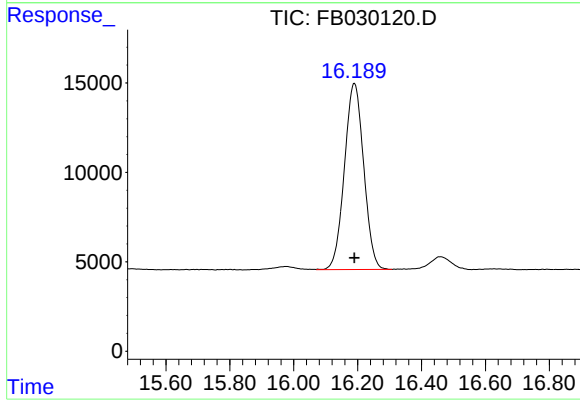

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min

Delta R.T.: 0.000 min

Response: 435990

Conc: 19.06 ng/ml