

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062625\
 Data File : FB031941.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jun 2025 16:09
 Operator : YP/AJ
 Sample : Q2413-05 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-73

Integration File: Calibration.e
 Quant Time: Jun 27 00:30:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	241049	15.624 ng/ml
Target Compounds			
6) t Toluene	10.619	5613	0.157 ng/ml
8) t m-Xylene	13.192	6552	0.200 ng/ml
9) t O-Xylene	13.919	5355	0.173 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	11170	0.422 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062625\
Data File : FB031941.D
Signal(s) : FID2B.CH
Acq On : 26 Jun 2025 16:09
Operator : YP/AJ
Sample : Q2413-05 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-73

Integration File: Calibration.e
Quant Time: Jun 27 00:30:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

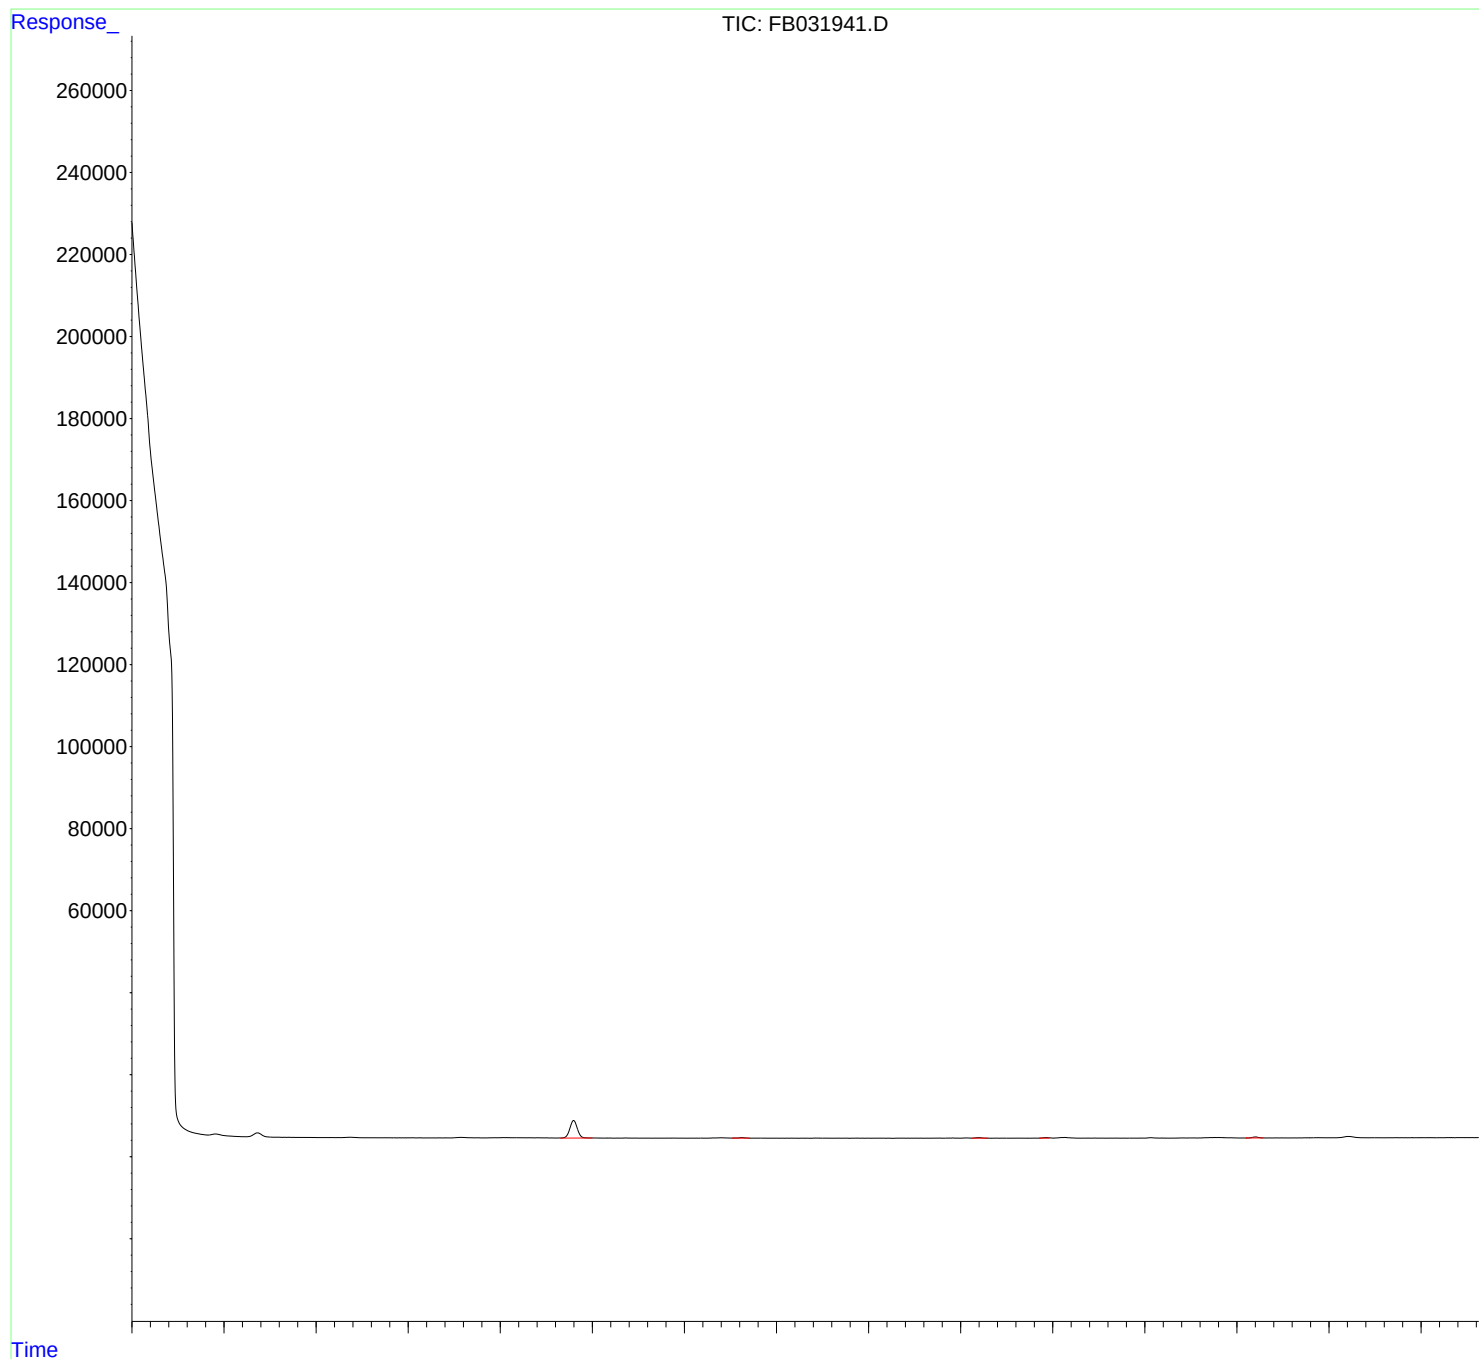


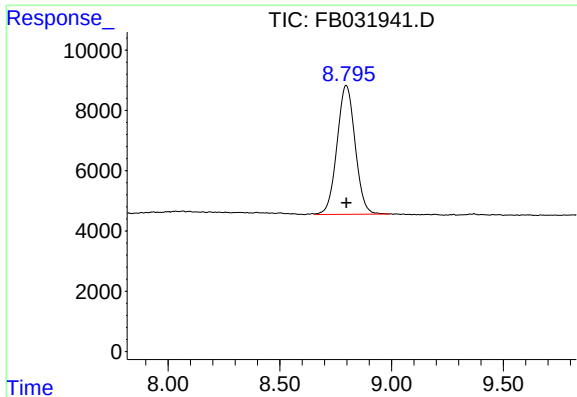

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 241049
Conc: 15.62 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-73

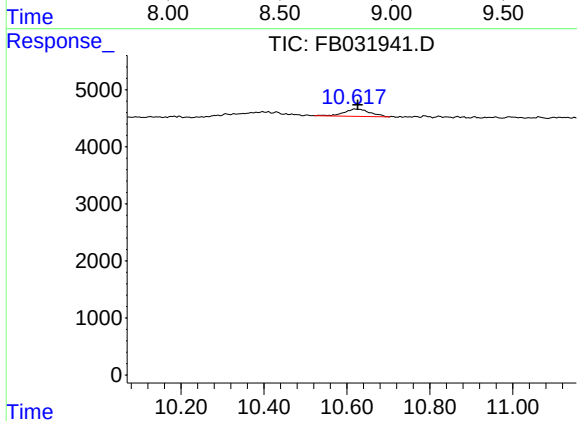


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.008 min
Response: 5613
Conc: 0.16 ng/ml

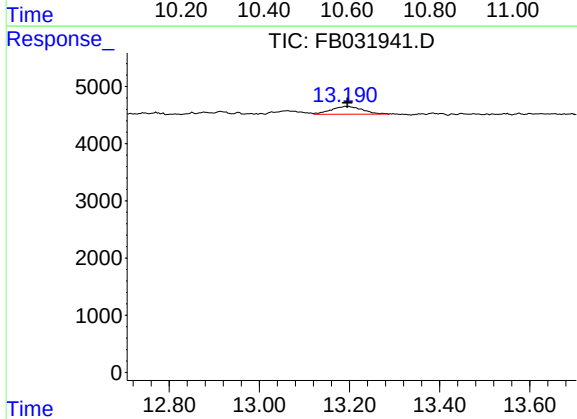


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.004 min
Response: 6552
Conc: 0.20 ng/ml

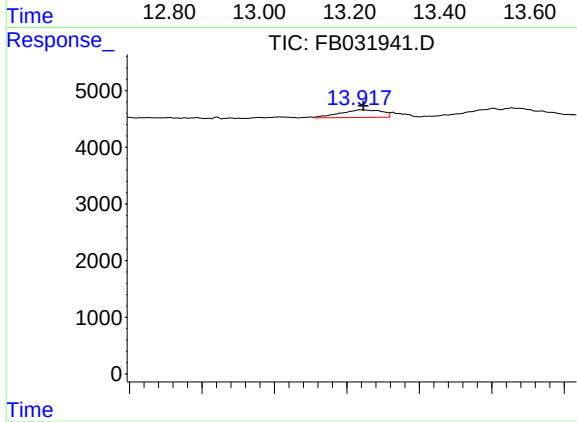

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.004 min
Response: 5355
Conc: 0.17 ng/ml

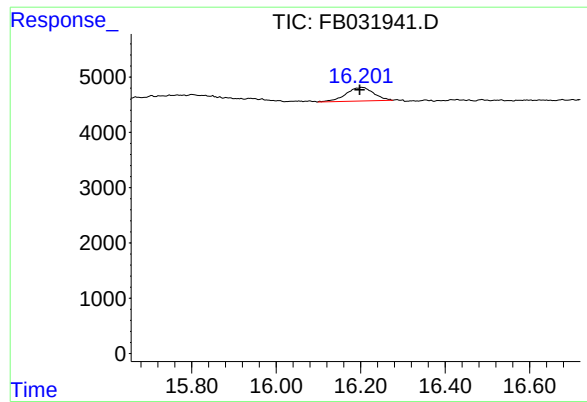

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: 0.005 min
Response: 11170
Conc: 0.42 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-73