

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062718\
 Data File : FB016442.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jun 2018 8:04 pm
 Operator : MJ/SJ
 Sample : J3048-05MSD
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 16 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 28 08:18:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.114	143101	20.362 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	257697	21.251 ng/ml
2) t 2,2,4-Trimethylpentane	7.732	287502	24.825 ng/ml
3) t n-Heptane	8.071	72129	6.591 ng/ml
4) t Benzene	8.210	131266	8.841 ng/ml
6) t Toluene	10.965	303350	24.439 ng/ml
7) t Ethylbenzene	13.415	118884	8.493 ng/ml
8) t m-Xylene	13.547	251024	16.492 ng/ml
9) t O-Xylene	14.279	269790	17.288 ng/ml
10) t 1,2,4-Trimethylbenzene	16.562	294101	17.076 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062718\
Data File : FB016442.D
Signal(s) : FID2B.CH
Acq On : 27 Jun 2018 8:04 pm
Operator : MJ/SJ
Sample : J3048-05MSD
Misc : 5.01g/5.00mL DI Water
ALS Vial : 16 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 28 08:18:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

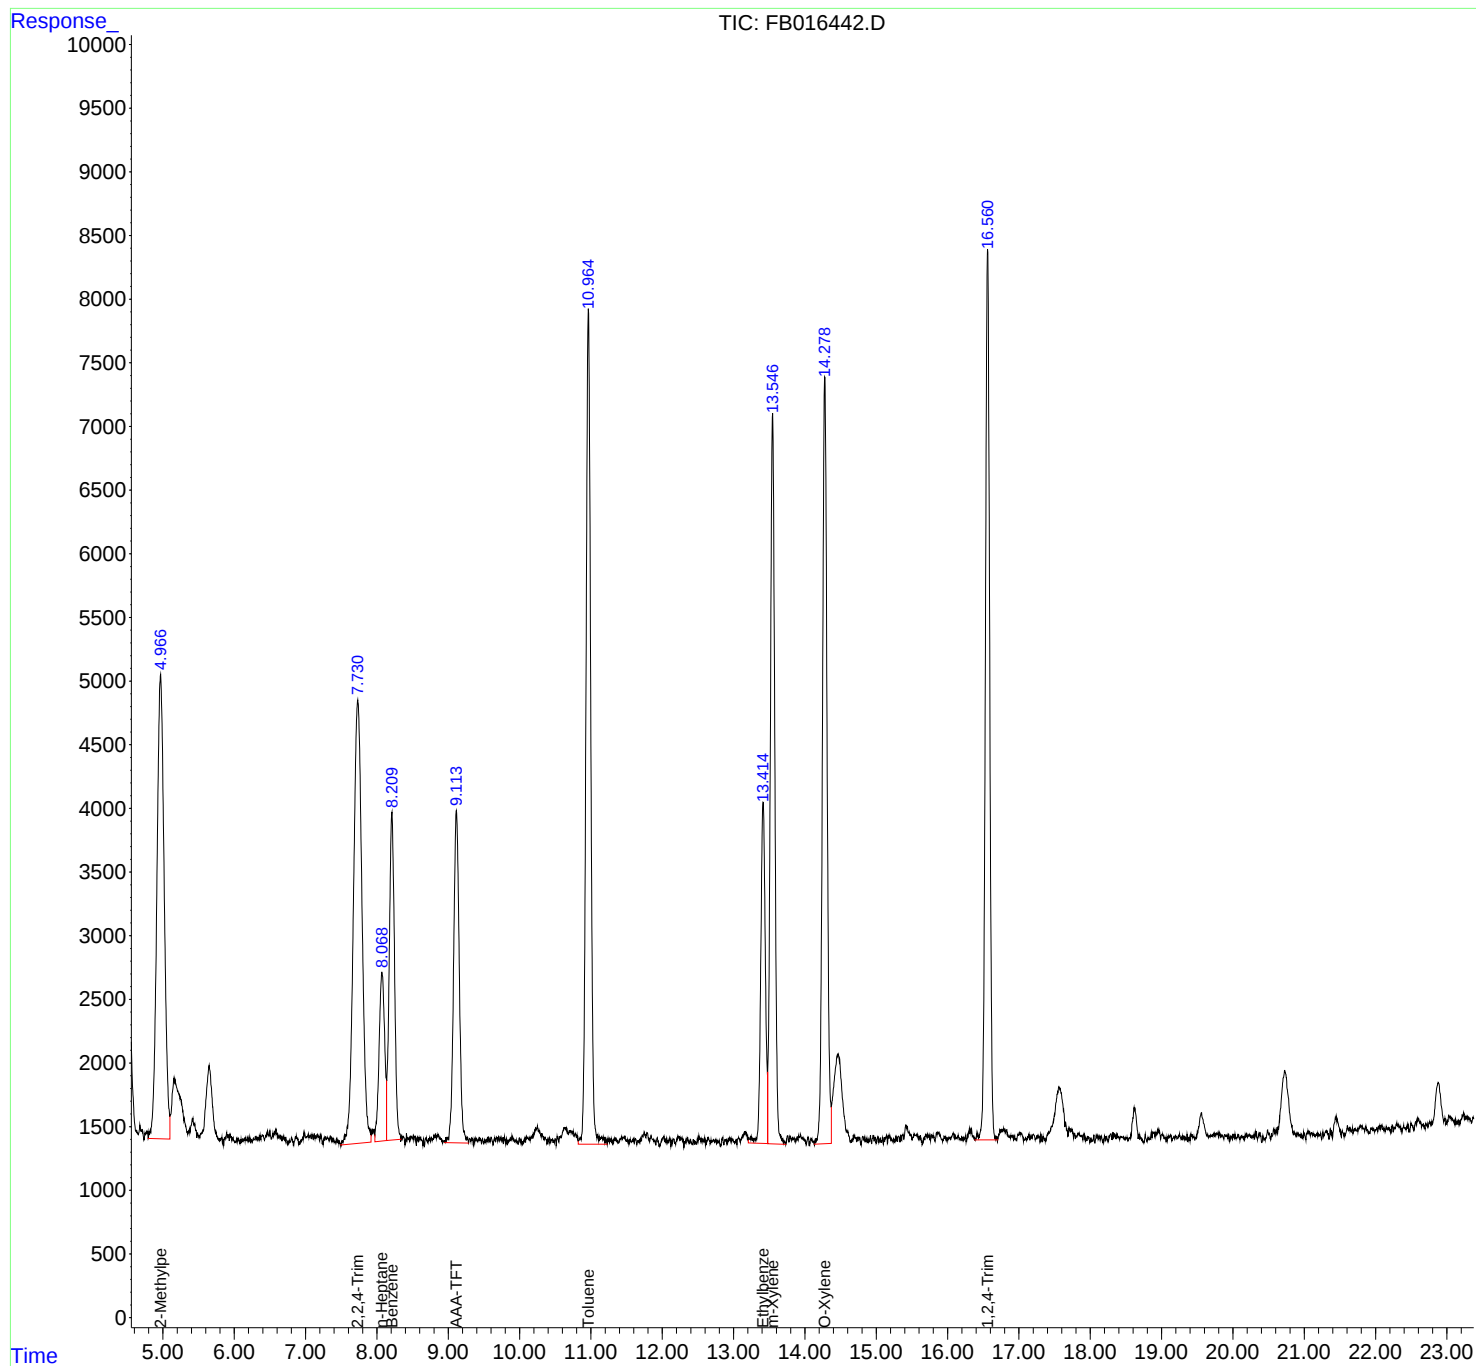

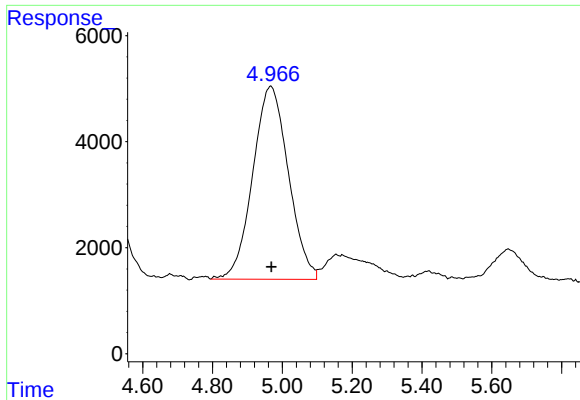


#1 2-Methylpentane

R.T.: 4.968 min
Delta R.T.: -0.001 min
Response: 257697
Conc: 21.25 ng/ml

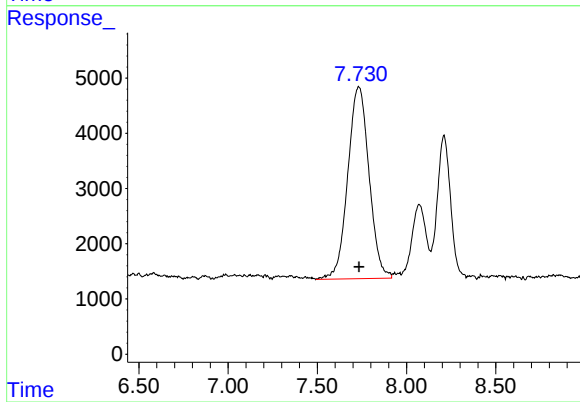


#2 2,2,4-Trimethylpentane

R.T.: 7.732 min
Delta R.T.: -0.002 min
Response: 287502
Conc: 24.83 ng/ml

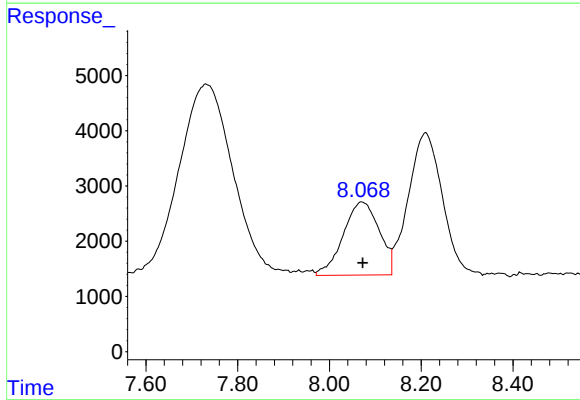


#3 n-Heptane

R.T.: 8.071 min
Delta R.T.: -0.002 min
Response: 72129
Conc: 6.59 ng/ml

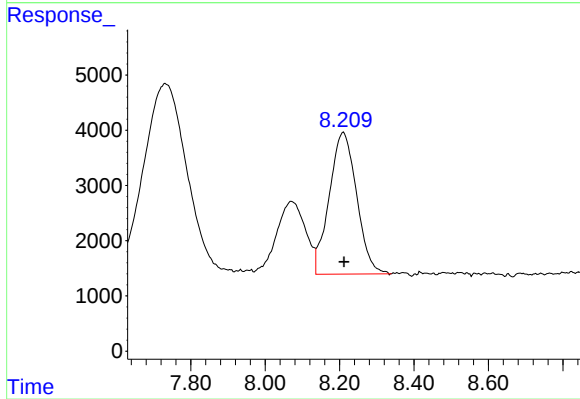


#4 Benzene

R.T.: 8.210 min
Delta R.T.: -0.001 min
Response: 131266
Conc: 8.84 ng/ml

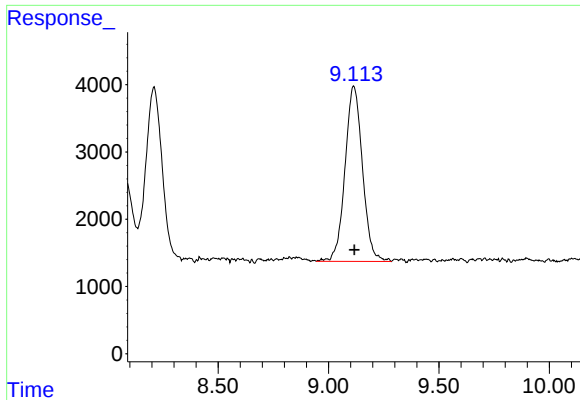


#5 AAA-TFT

R.T.: 9.114 min
Delta R.T.: -0.003 min
Response: 143101
Conc: 20.36 ng/ml

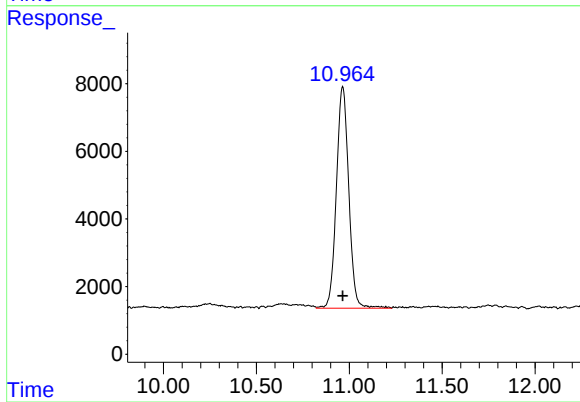


#6 Toluene

R.T.: 10.965 min
Delta R.T.: 0.000 min
Response: 303350
Conc: 24.44 ng/ml

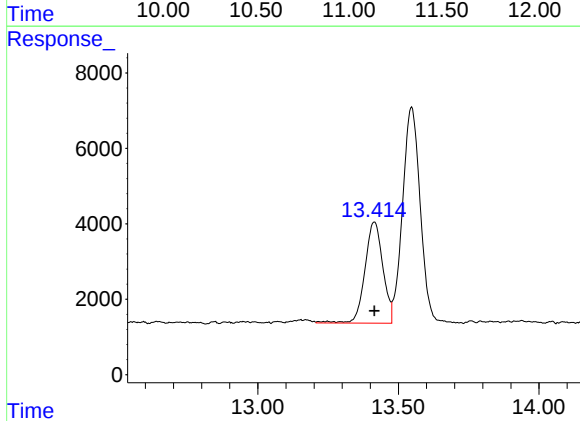


#7 Ethylbenzene

R.T.: 13.415 min
Delta R.T.: 0.000 min
Response: 118884
Conc: 8.49 ng/ml

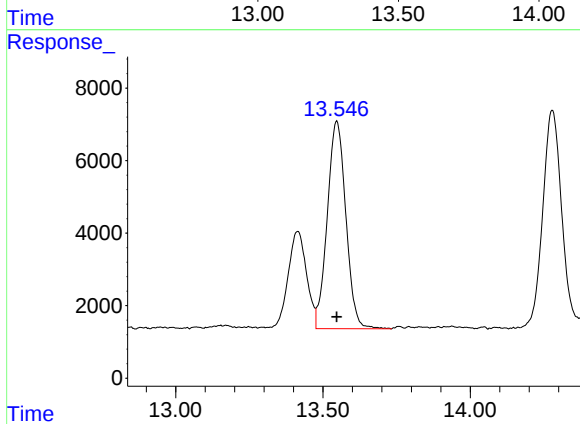


#8 m-Xylene

R.T.: 13.547 min
Delta R.T.: 0.000 min
Response: 251024
Conc: 16.49 ng/ml

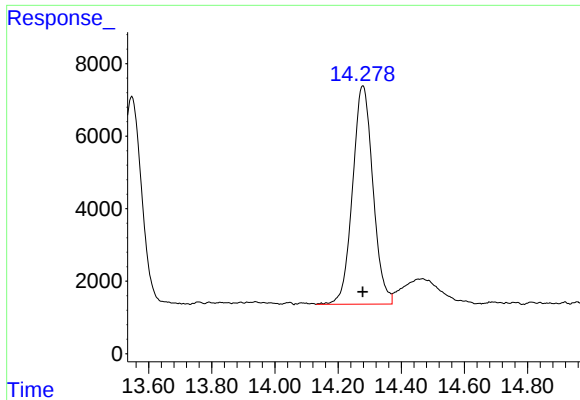

#9 O-Xylene

R.T.: 14.279 min
Delta R.T.: 0.000 min
Response: 269790
Conc: 17.29 ng/ml

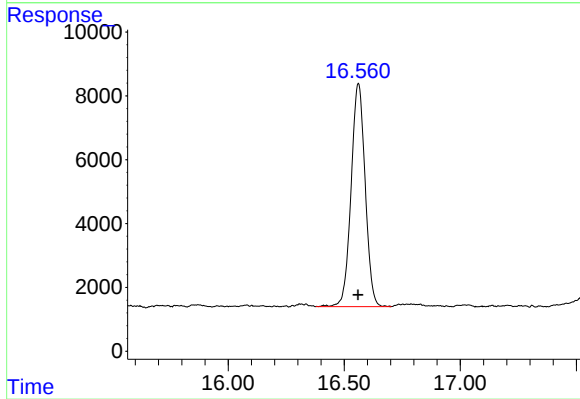

#10 1,2,4-Trimethylbenzene

R.T.: 16.562 min
Delta R.T.: 0.001 min
Response: 294101
Conc: 17.08 ng/ml