

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
 Data File : FB021519.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jun 2019 12:46
 Operator : MJ/SJ
 Sample : BSF0627S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 28 07:51:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.986	245425	17.750 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.859	894769	26.211 ng/ml
2) t 2,2,4-Trimethylpentane	7.606	789898	25.561 ng/ml
3) t n-Heptane	7.945	248784	8.500 ng/ml
4) t Benzene	8.080	298488	8.893 ng/ml
6) t Toluene	10.827	643308	28.163 ng/ml
7) t Ethylbenzene	13.272	240186	10.146 ng/ml
8) t m-Xylene	13.405	509460	20.100 ng/ml
9) t O-Xylene	14.135	522710	19.930 ng/ml
10) t 1,2,4-Trimethylbenzene	16.415	524976	19.981 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
Data File : FB021519.D
Signal(s) : FID2B.CH
Acq On : 27 Jun 2019 12:46
Operator : MJ/SJ
Sample : BSF0627S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 28 07:51:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

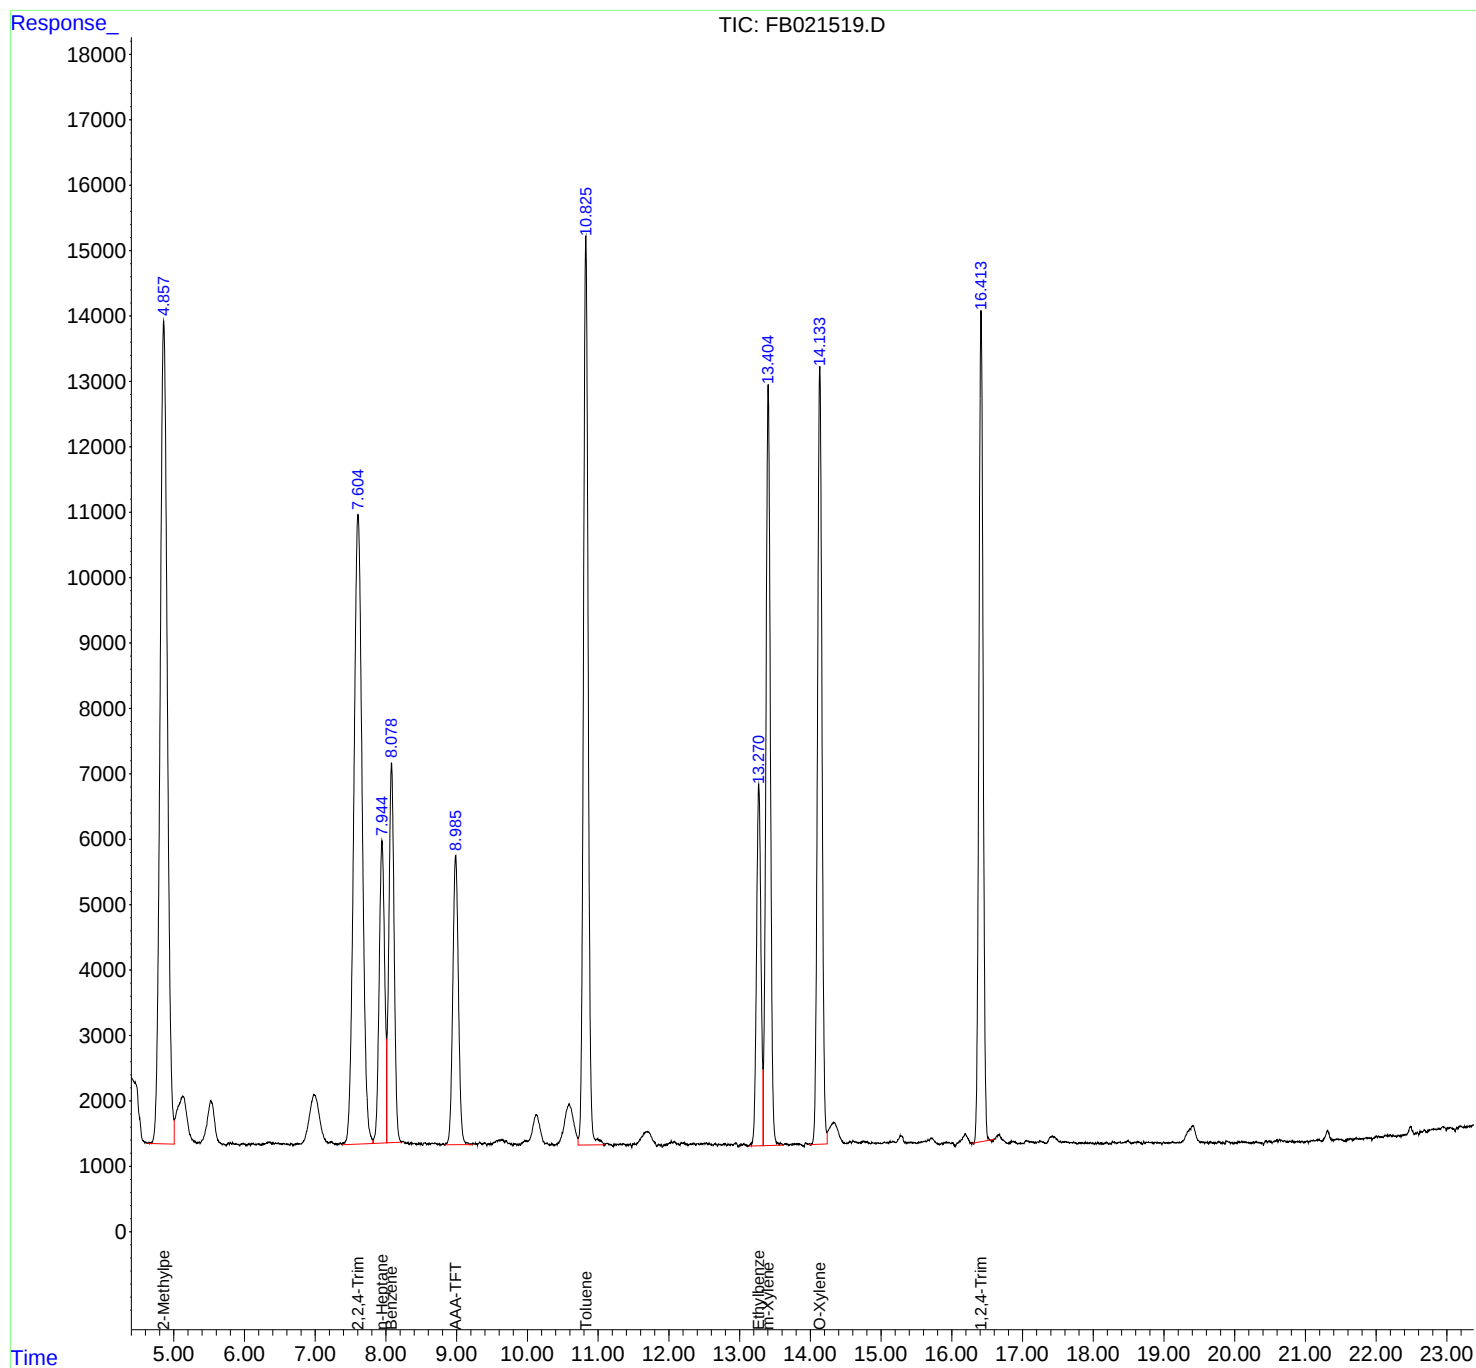

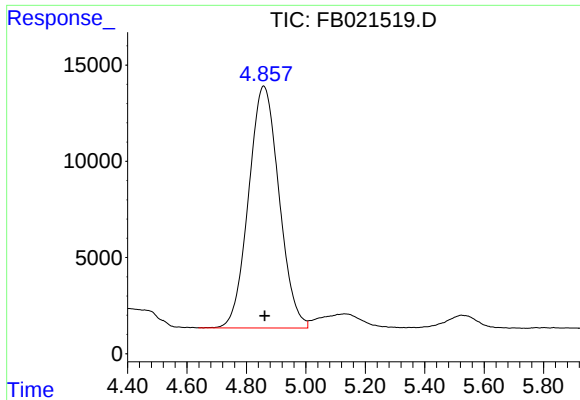


#1 2-Methylpentane

R.T.: 4.859 min
Delta R.T.: -0.002 min
Response: 894769
Conc: 26.21 ng/ml

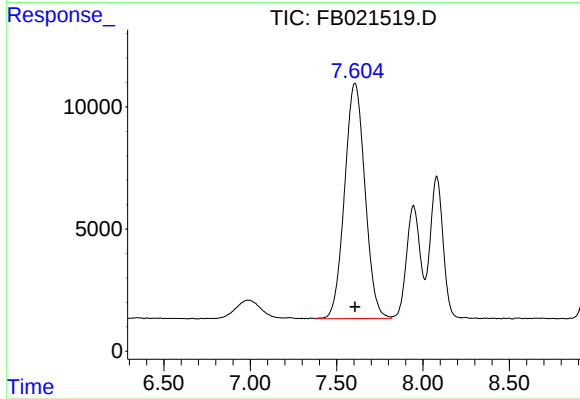


#2 2,2,4-Trimethylpentane

R.T.: 7.606 min
Delta R.T.: -0.002 min
Response: 789898
Conc: 25.56 ng/ml

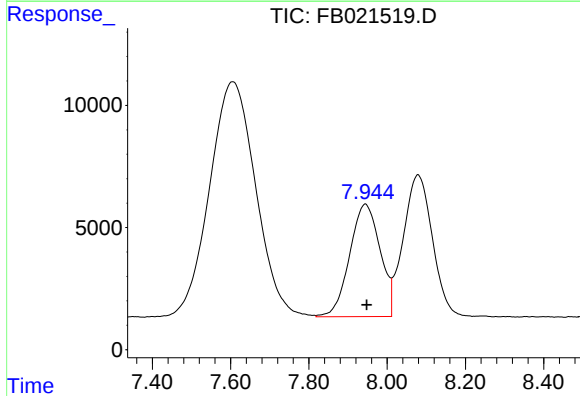


#3 n-Heptane

R.T.: 7.945 min
Delta R.T.: -0.003 min
Response: 248784
Conc: 8.50 ng/ml

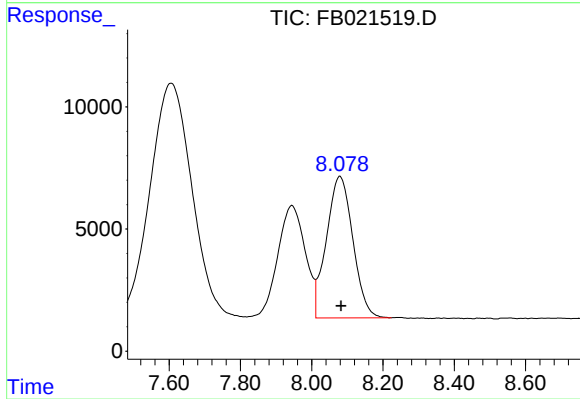


#4 Benzene

R.T.: 8.080 min
Delta R.T.: -0.003 min
Response: 298488
Conc: 8.89 ng/ml

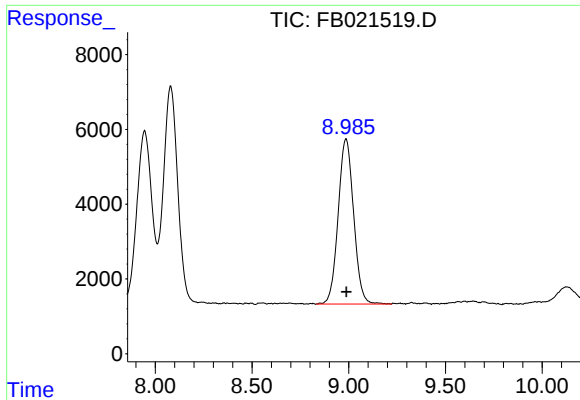


#5 AAA-TFT

R.T.: 8.986 min
Delta R.T.: -0.002 min
Response: 245425
Conc: 17.75 ng/ml

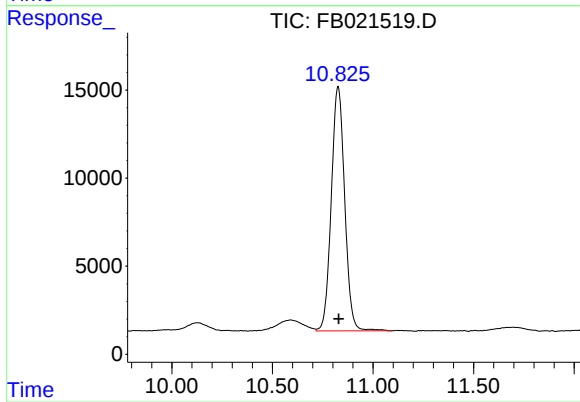


#6 Toluene

R.T.: 10.827 min
Delta R.T.: -0.003 min
Response: 643308
Conc: 28.16 ng/ml

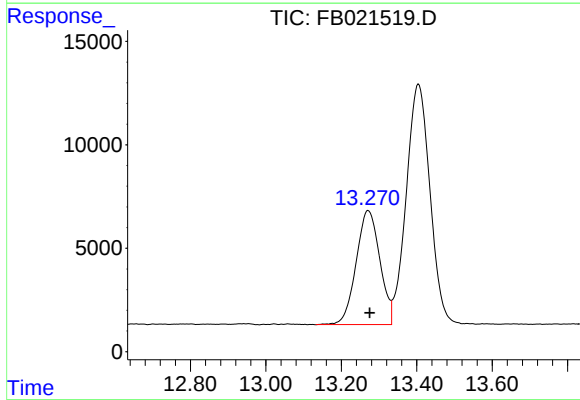


#7 Ethylbenzene

R.T.: 13.272 min
Delta R.T.: -0.003 min
Response: 240186
Conc: 10.15 ng/ml

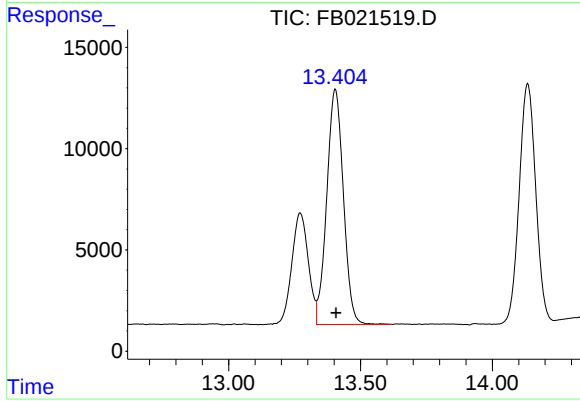


#8 m-Xylene

R.T.: 13.405 min
Delta R.T.: -0.003 min
Response: 509460
Conc: 20.10 ng/ml

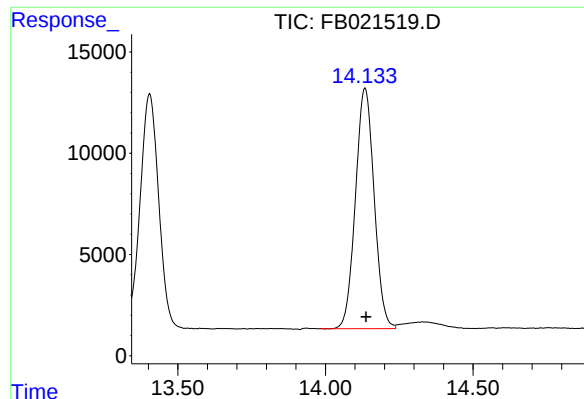

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: -0.003 min
Response: 522710
Conc: 19.93 ng/ml

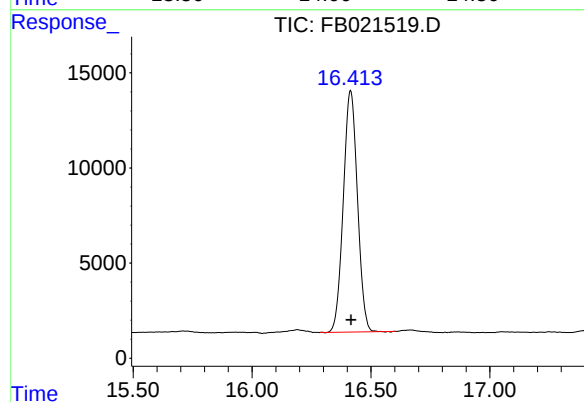

#10 1,2,4-Trimethylbenzene

R.T.: 16.415 min
Delta R.T.: -0.002 min
Response: 524976
Conc: 19.98 ng/ml