

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
 Data File : FB021522.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jun 2019 14:18
 Operator : MJ/SJ
 Sample : K3159-09MS
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 28 07:51:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.987	11877	0.859 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.860	44015	1.289 ng/ml
2) t 2,2,4-Trimethylpentane	7.603	35874	1.161 ng/ml
3) t n-Heptane	7.948	10529	0.360 ng/ml
4) t Benzene	8.072	5370	0.160 ng/ml
6) t Toluene	10.830	28648	1.254 ng/ml
7) t Ethylbenzene	13.276	9778	0.413 ng/ml
8) t m-Xylene	13.405	18658	0.736 ng/ml
9) t O-Xylene	14.140	16907	0.645 ng/ml
10) t 1,2,4-Trimethylbenzene	16.416	8942	0.340 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
Data File : FB021522.D
Signal(s) : FID2B.CH
Acq On : 27 Jun 2019 14:18
Operator : MJ/SJ
Sample : K3159-09MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 28 07:51:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

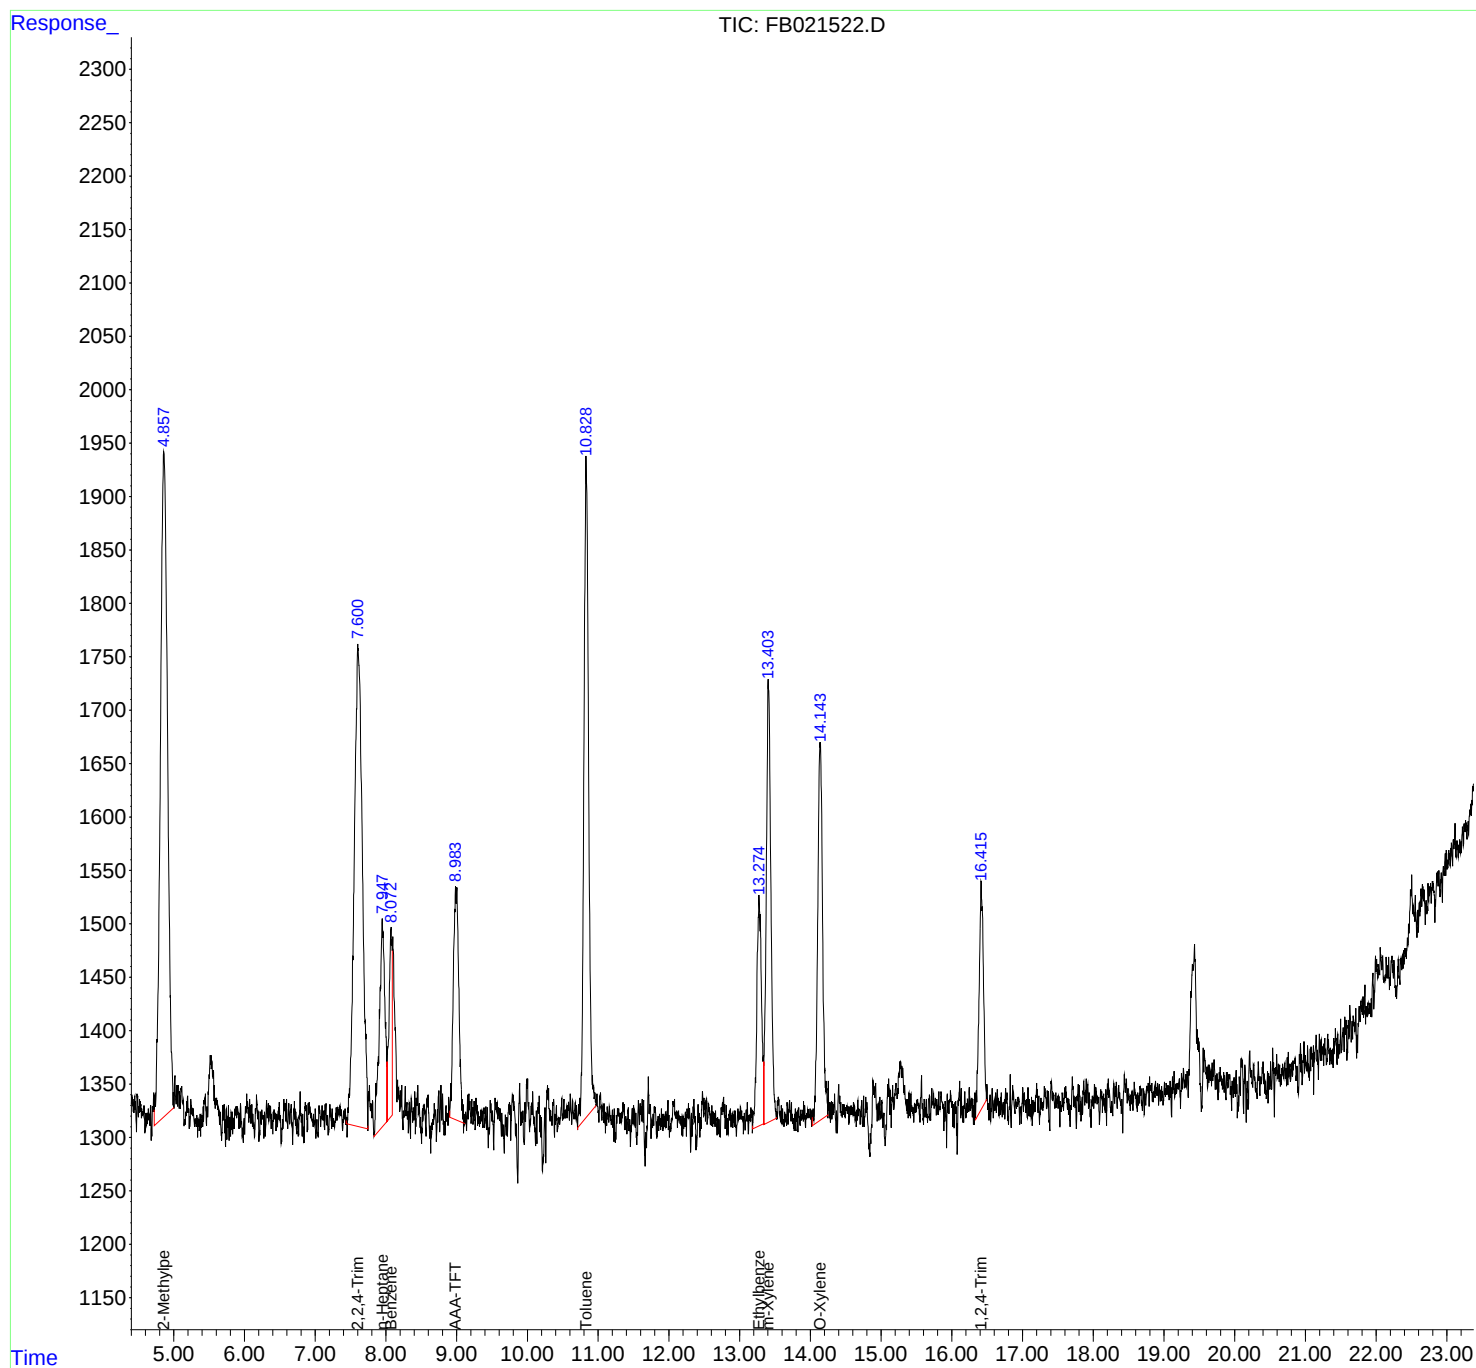

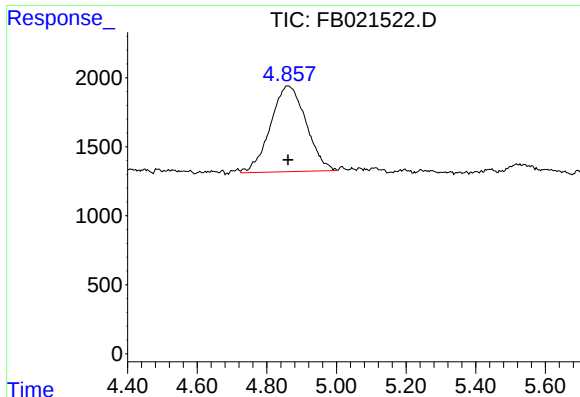


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: 0.000 min
Response: 44015
Conc: 1.29 ng/ml

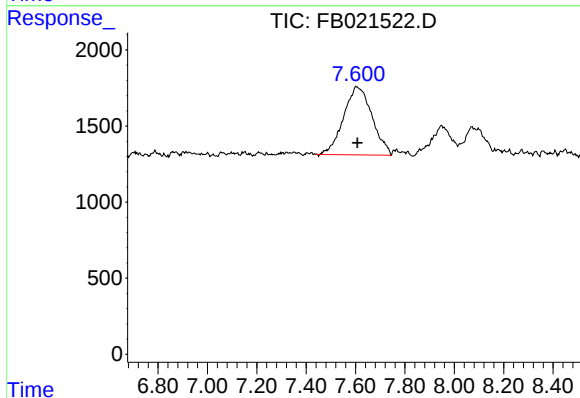


#2 2,2,4-Trimethylpentane

R.T.: 7.603 min
Delta R.T.: -0.005 min
Response: 35874
Conc: 1.16 ng/ml

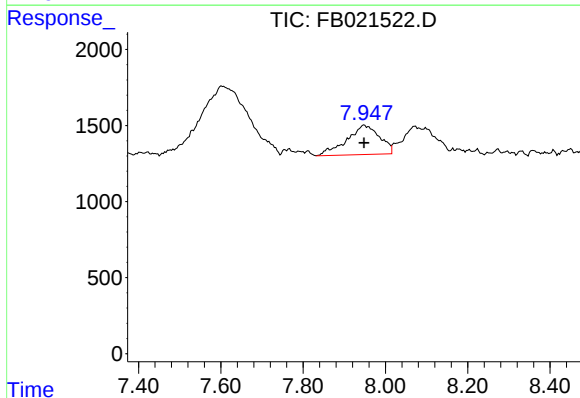


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 10529
Conc: 0.36 ng/ml

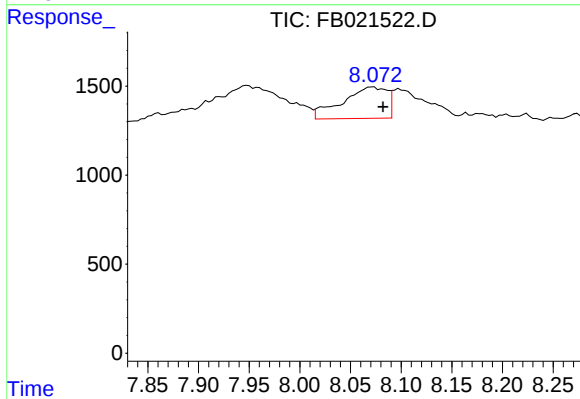


#4 Benzene

R.T.: 8.072 min
Delta R.T.: -0.010 min
Response: 5370
Conc: 0.16 ng/ml

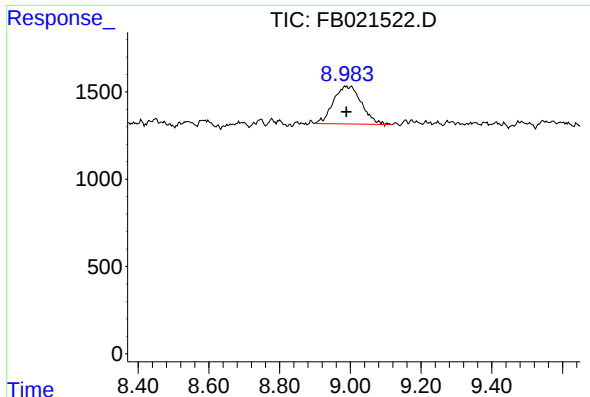


#5 AAA-TFT

R.T.: 8.987 min
Delta R.T.: -0.002 min
Response: 11877
Conc: 0.86 ng/ml

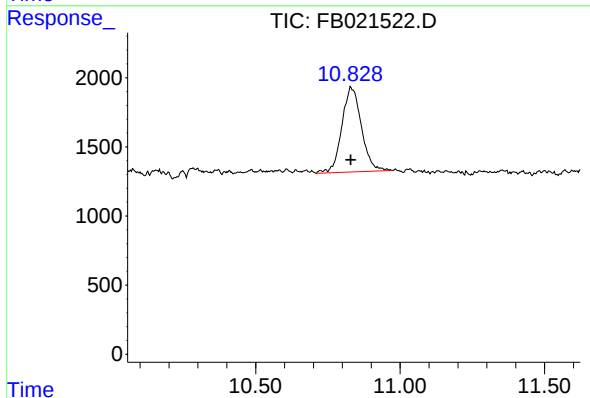


#6 Toluene

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 28648
Conc: 1.25 ng/ml

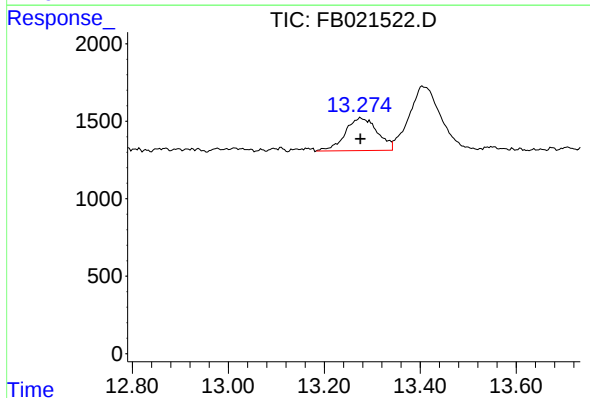


#7 Ethylbenzene

R.T.: 13.276 min
Delta R.T.: 0.000 min
Response: 9778
Conc: 0.41 ng/ml

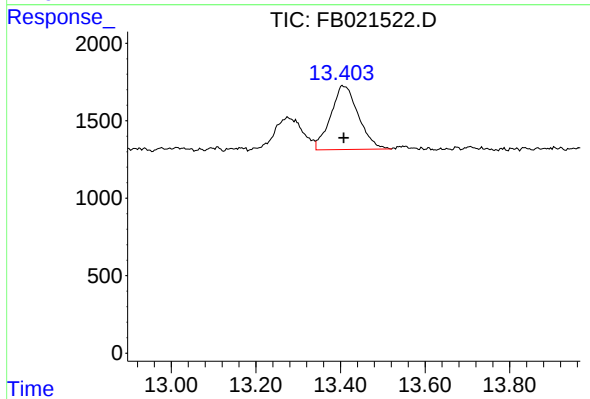


#8 m-Xylene

R.T.: 13.405 min
Delta R.T.: -0.003 min
Response: 18658
Conc: 0.74 ng/ml

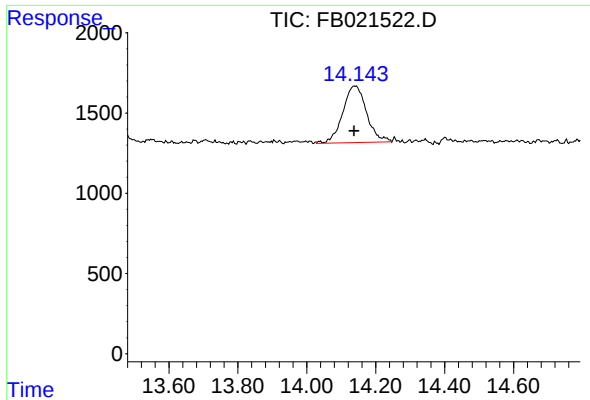

#9 O-Xylene

R.T.: 14.140 min
Delta R.T.: 0.002 min
Response: 16907
Conc: 0.64 ng/ml

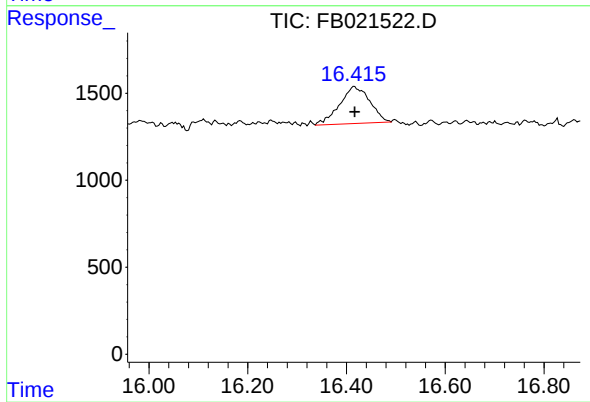

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: -0.001 min
Response: 8942
Conc: 0.34 ng/ml