

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
 Data File : FB021548.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2019 3:58
 Operator : MJ/SJ
 Sample : K3159-09MS
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 33 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 28 07:55:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	250461	18.115 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.860	893642	26.178 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	829041	26.827 ng/ml
3) t n-Heptane	7.947	254539	8.697 ng/ml
4) t Benzene	8.082	309684	9.227 ng/ml
6) t Toluene	10.828	635598	27.825 ng/ml
7) t Ethylbenzene	13.274	218726	9.239 ng/ml
8) t m-Xylene	13.406	465481	18.365 ng/ml
9) t O-Xylene	14.135	489959	18.682 ng/ml
10) t 1,2,4-Trimethylbenzene	16.415	477346	18.168 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
Data File : FB021548.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2019 3:58
Operator : MJ/SJ
Sample : K3159-09MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 33 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 28 07:55:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

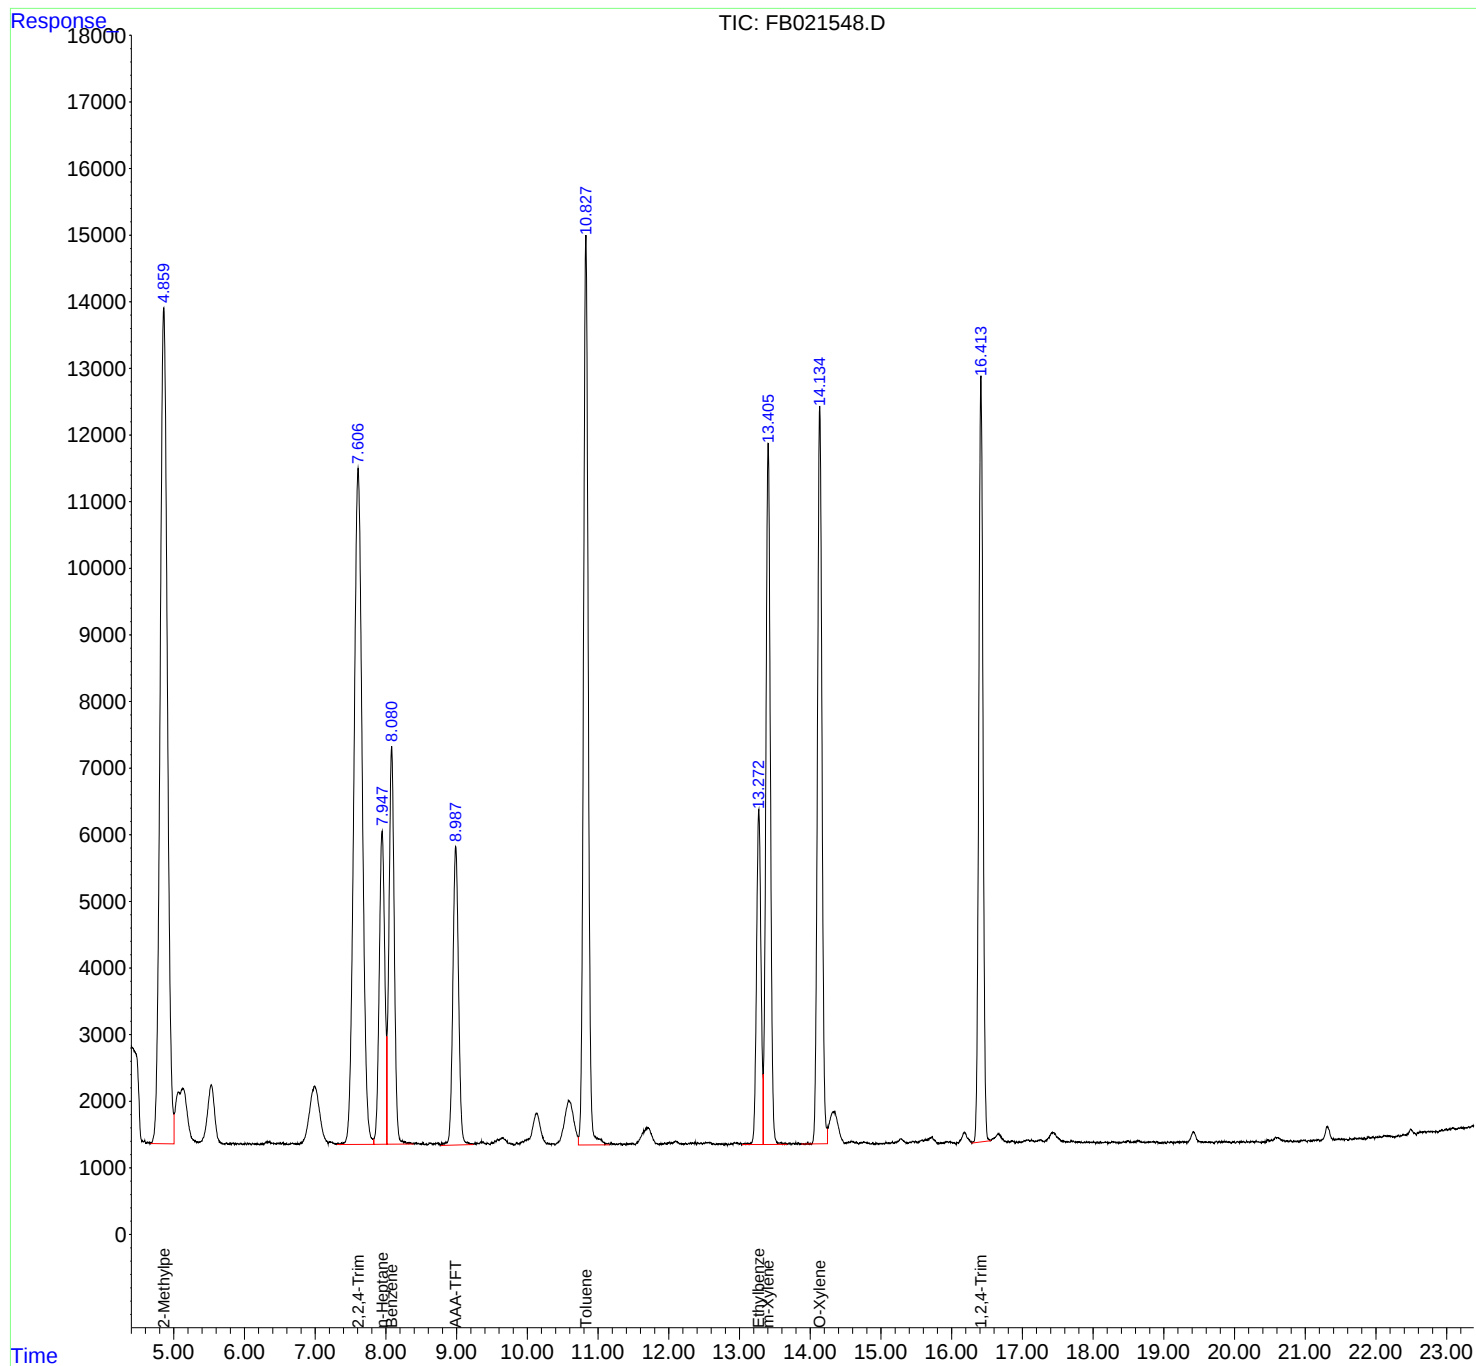

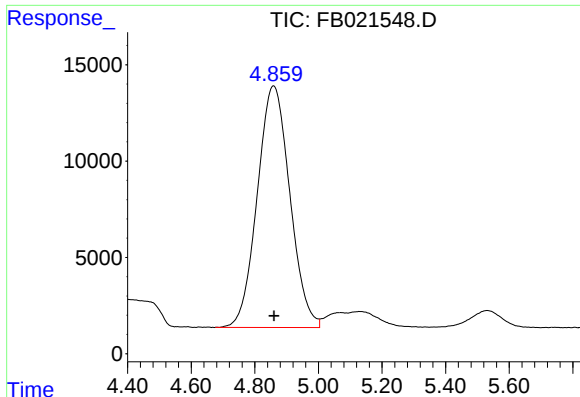


#1 2-Methylpentane

R.T.: 4.860 min
Delta R.T.: -0.001 min
Response: 893642
Conc: 26.18 ng/ml

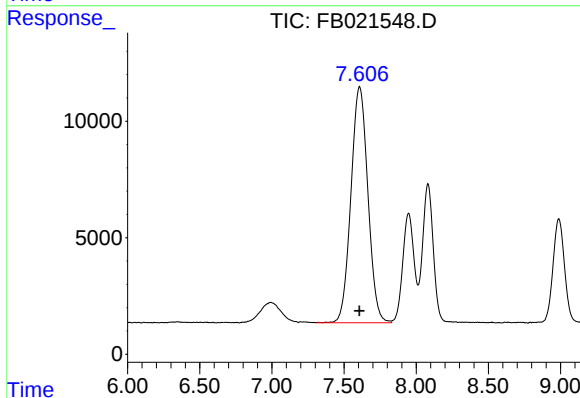


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 829041
Conc: 26.83 ng/ml

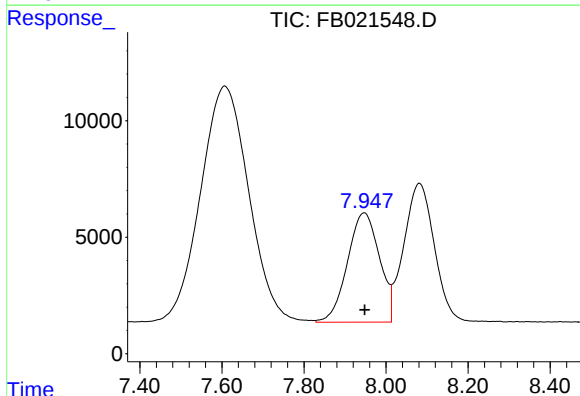


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 254539
Conc: 8.70 ng/ml

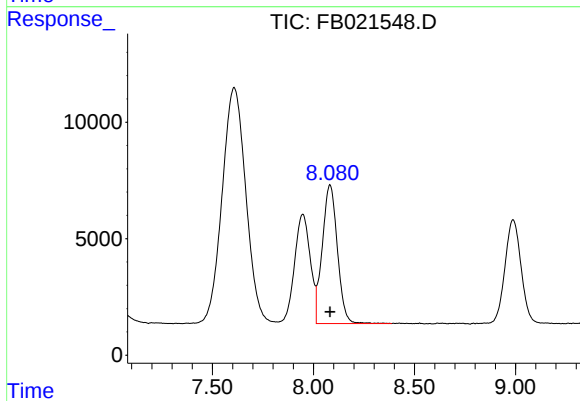


#4 Benzene

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 309684
Conc: 9.23 ng/ml

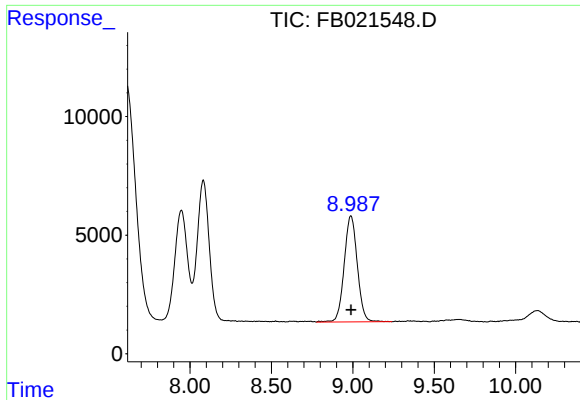


#5 AAA-TFT

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 250461
Conc: 18.11 ng/ml

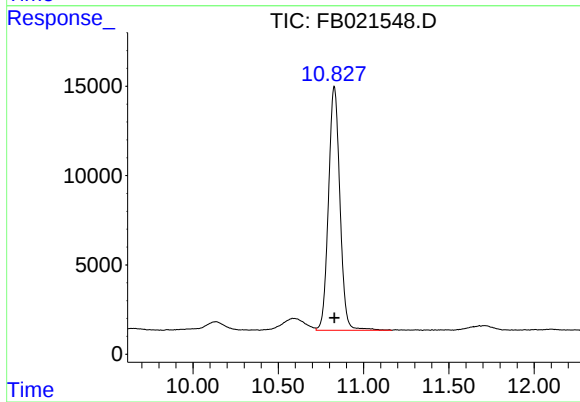


#6 Toluene

R.T.: 10.828 min
Delta R.T.: -0.001 min
Response: 635598
Conc: 27.83 ng/ml

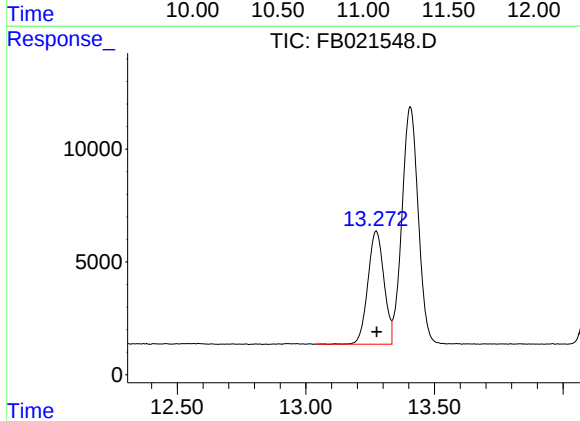


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: -0.002 min
Response: 218726
Conc: 9.24 ng/ml

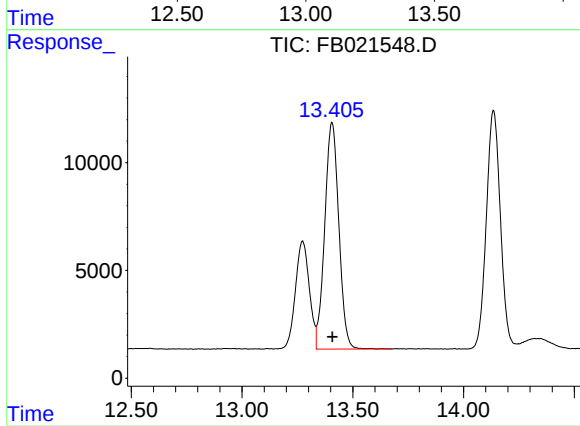


#8 m-Xylene

R.T.: 13.406 min
Delta R.T.: -0.001 min
Response: 465481
Conc: 18.37 ng/ml

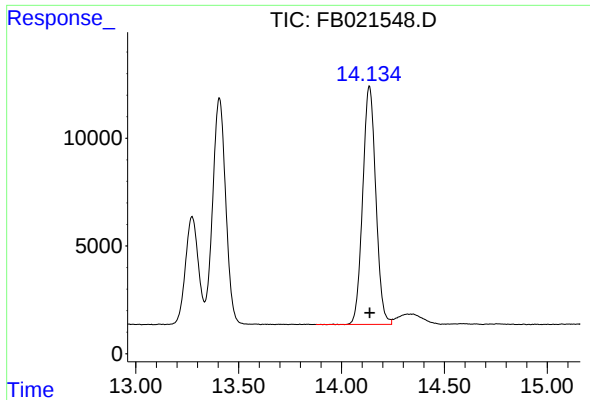

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: -0.002 min
Response: 489959
Conc: 18.68 ng/ml

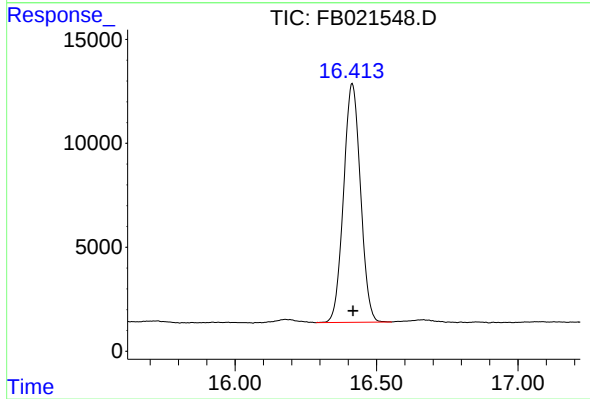

#10 1,2,4-Trimethylbenzene

R.T.: 16.415 min
Delta R.T.: -0.002 min
Response: 477346
Conc: 18.17 ng/ml