

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
Data File : FB021549.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2019 4:29
Operator : MJ/SJ
Sample : K3159-09MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 34 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 28 07:55:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.987	246137	17.802 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.859	878539	25.735 ng/ml
2) t 2,2,4-Trimethylpentane	7.606	834647	27.009 ng/ml
3) t n-Heptane	7.946	255349	8.724 ng/ml
4) t Benzene	8.081	300426	8.951 ng/ml
6) t Toluene	10.828	614106	26.884 ng/ml
7) t Ethylbenzene	13.273	213909	9.036 ng/ml
8) t m-Xylene	13.405	460097	18.153 ng/ml
9) t O-Xylene	14.135	486446	18.548 ng/ml
10) t 1,2,4-Trimethylbenzene	16.414	475577	18.101 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
Data File : FB021549.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2019 4:29
Operator : MJ/SJ
Sample : K3159-09MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 34 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 28 07:55:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

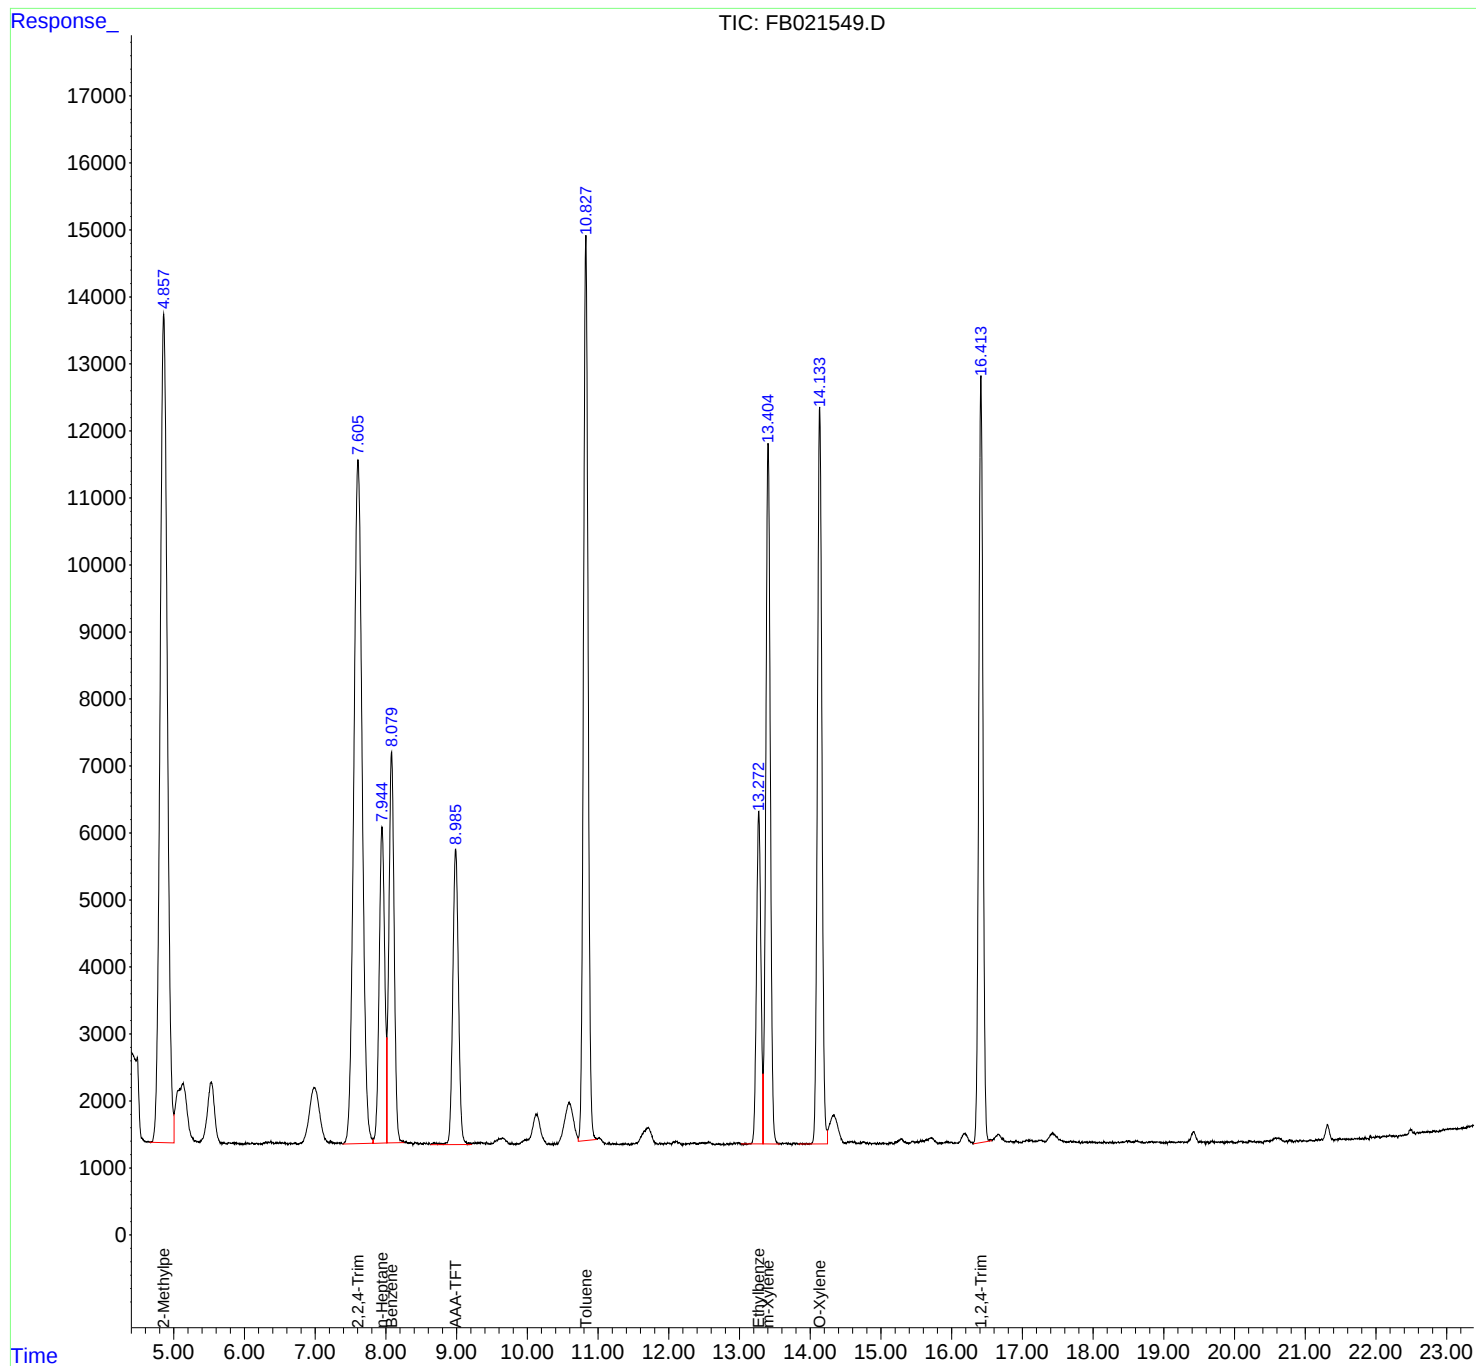

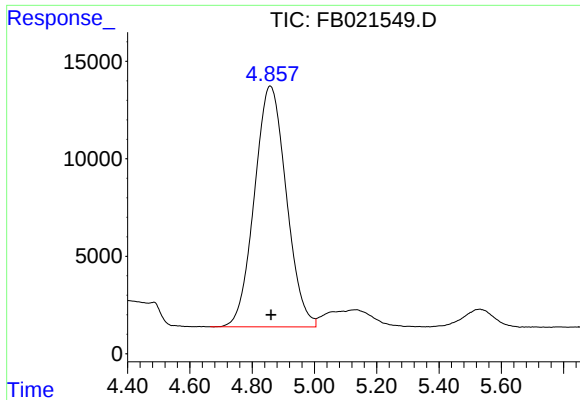


#1 2-Methylpentane

R.T.: 4.859 min
Delta R.T.: -0.002 min
Response: 878539
Conc: 25.74 ng/ml

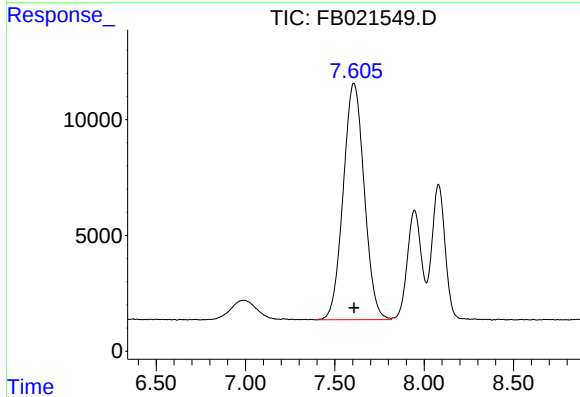


#2 2,2,4-Trimethylpentane

R.T.: 7.606 min
Delta R.T.: -0.002 min
Response: 834647
Conc: 27.01 ng/ml

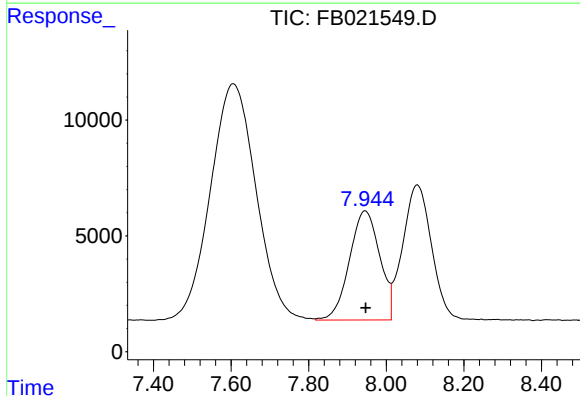


#3 n-Heptane

R.T.: 7.946 min
Delta R.T.: -0.002 min
Response: 255349
Conc: 8.72 ng/ml

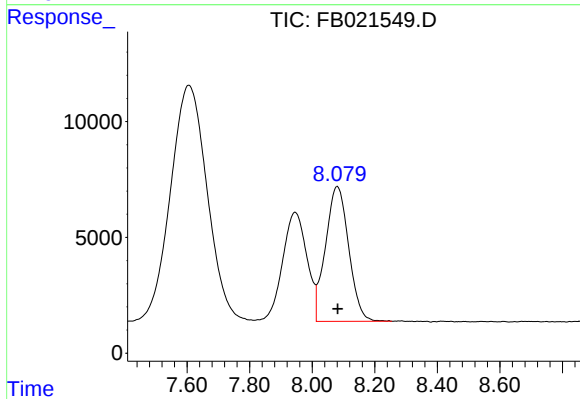


#4 Benzene

R.T.: 8.081 min
Delta R.T.: -0.002 min
Response: 300426
Conc: 8.95 ng/ml

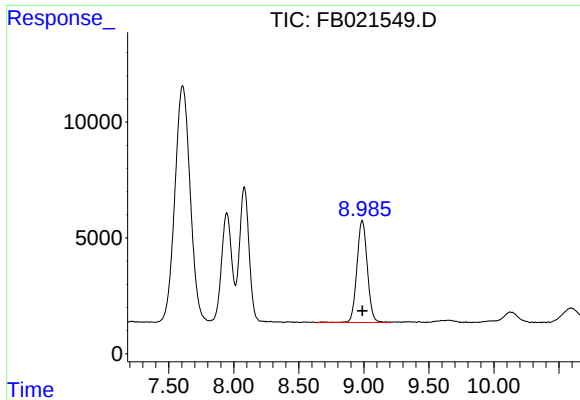


#5 AAA-TFT

R.T.: 8.987 min
Delta R.T.: -0.002 min
Response: 246137
Conc: 17.80 ng/ml

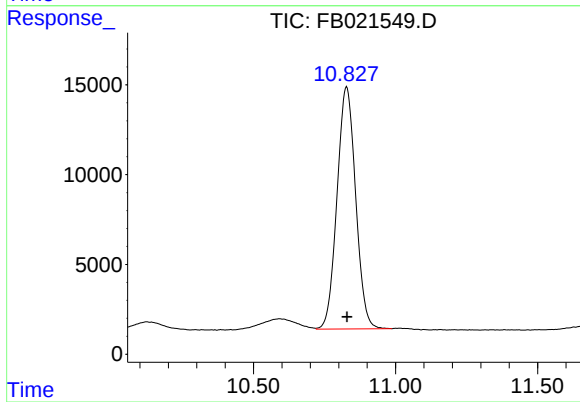


#6 Toluene

R.T.: 10.828 min
Delta R.T.: -0.002 min
Response: 614106
Conc: 26.88 ng/ml

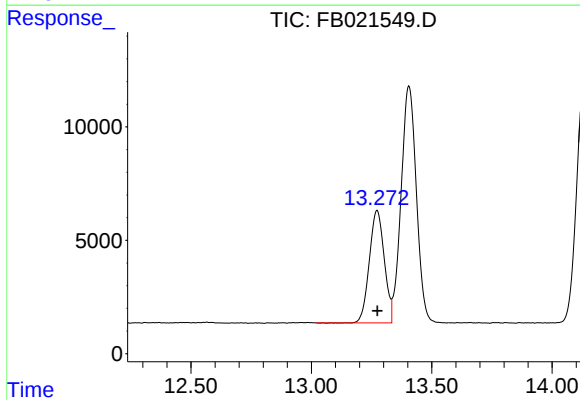


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: -0.002 min
Response: 213909
Conc: 9.04 ng/ml

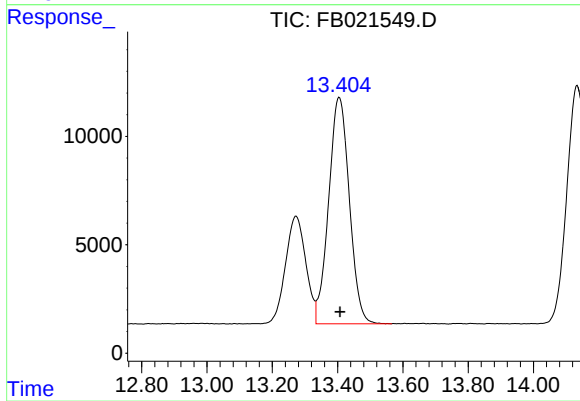


#8 m-Xylene

R.T.: 13.405 min
Delta R.T.: -0.003 min
Response: 460097
Conc: 18.15 ng/ml

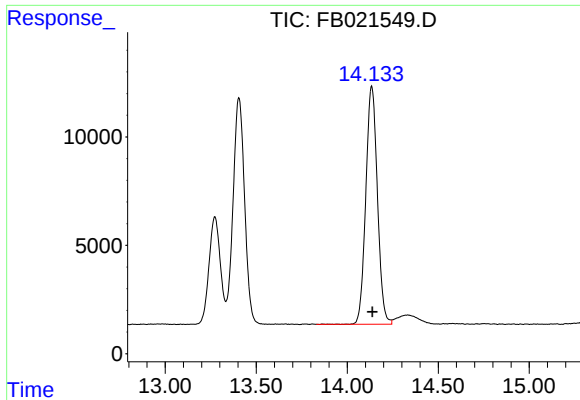

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: -0.003 min
Response: 486446
Conc: 18.55 ng/ml

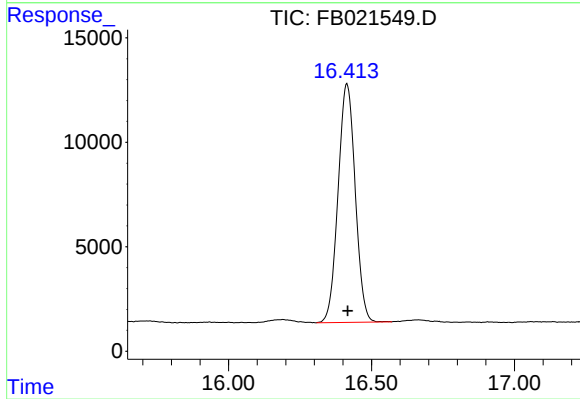

#10 1,2,4-Trimethylbenzene

R.T.: 16.414 min
Delta R.T.: -0.003 min
Response: 475577
Conc: 18.10 ng/ml