

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
 Data File : FB021523.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jun 2019 14:48
 Operator : MJ/SJ
 Sample : K3159-09MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 28 07:51:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	315416	22.812 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	844006	24.724 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	683943	22.132 ng/ml
3) t n-Heptane	7.947	191811	6.554 ng/ml
4) t Benzene	8.082	326444	9.726 ng/ml
6) t Toluene	10.829	661406	28.955 ng/ml
7) t Ethylbenzene	13.275	217545	9.190 ng/ml
8) t m-Xylene	13.407	452859	17.867 ng/ml
9) t O-Xylene	14.137	472172	18.003 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	419067	15.950 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062719\
Data File : FB021523.D
Signal(s) : FID2B.CH
Acq On : 27 Jun 2019 14:48
Operator : MJ/SJ
Sample : K3159-09MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 28 07:51:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

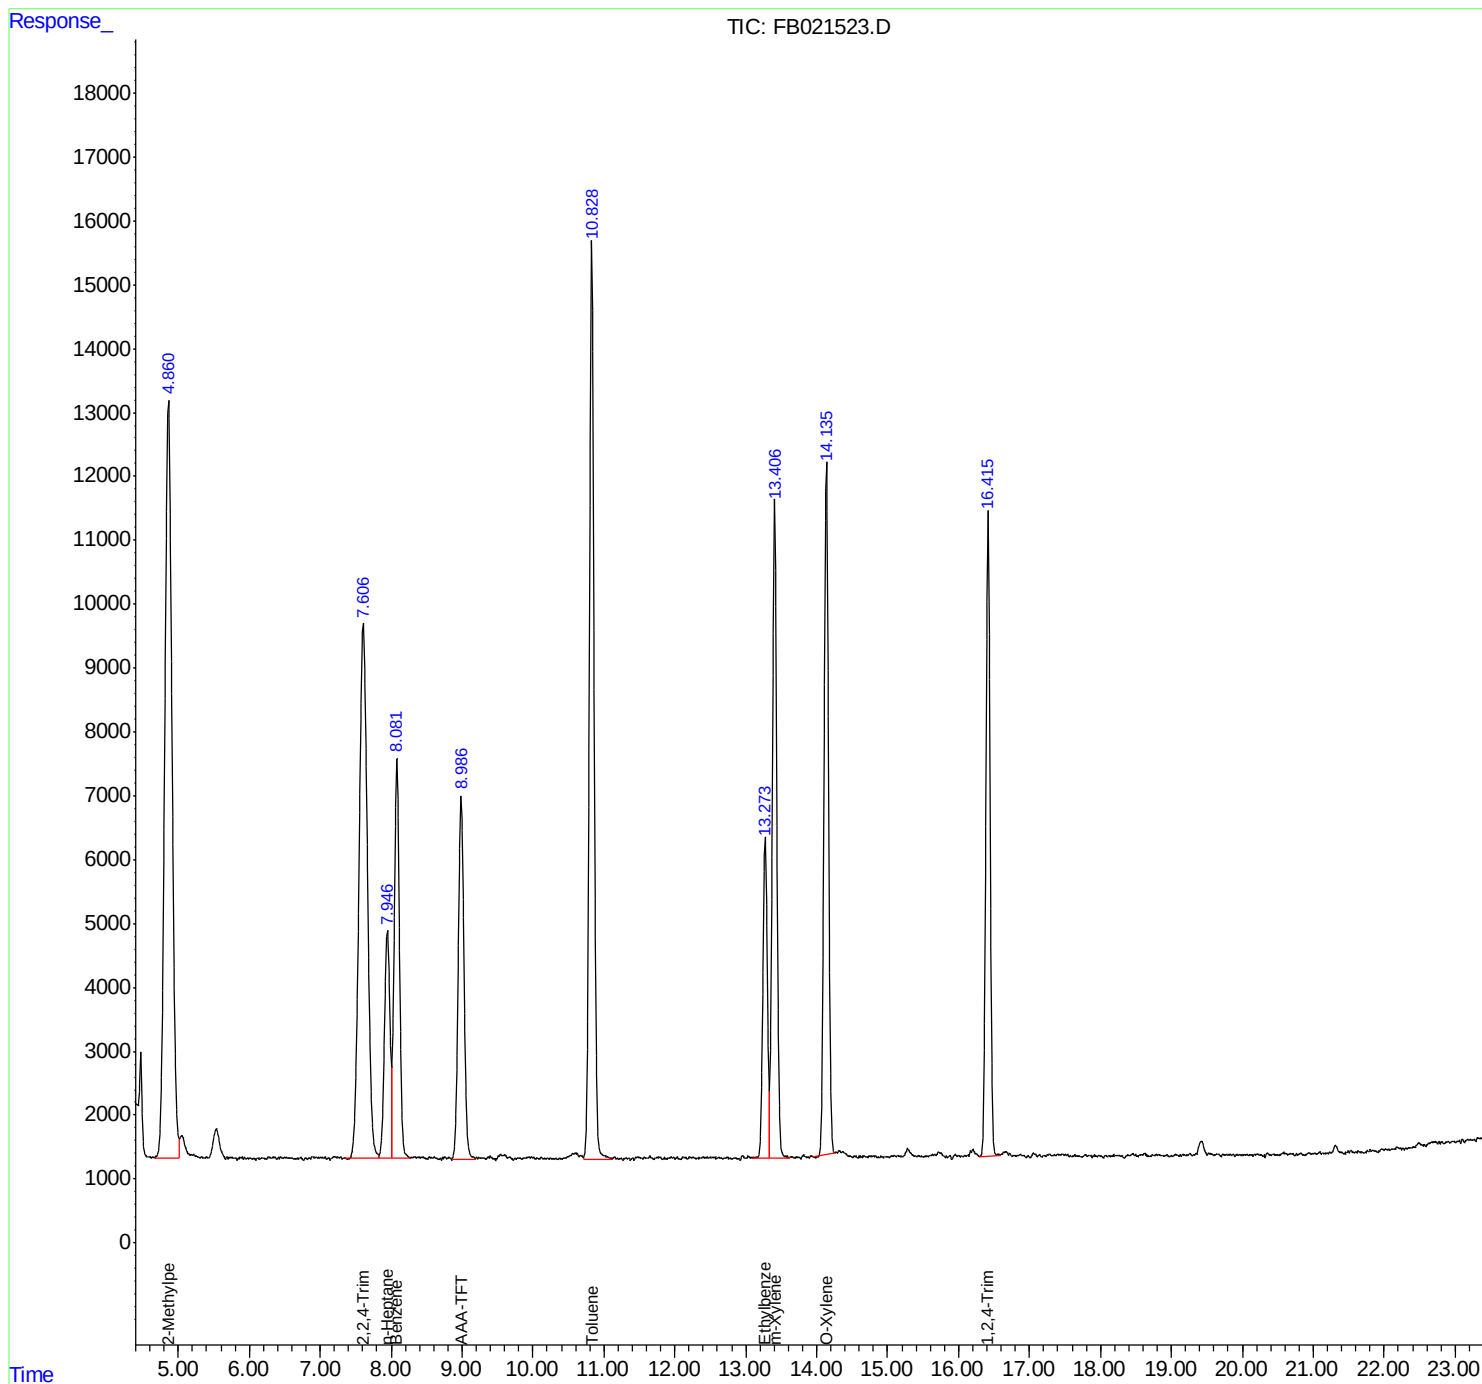

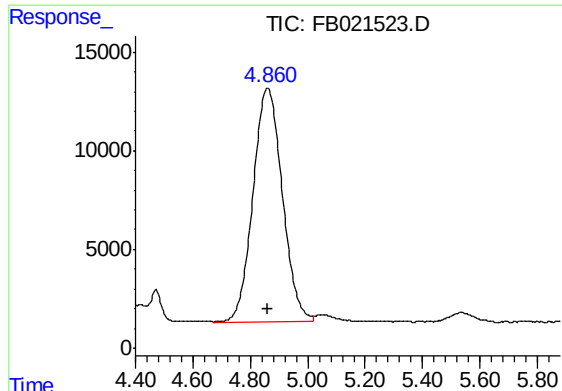


#1 2-Methylpentane

R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 844006
Conc: 24.72 ng/ml

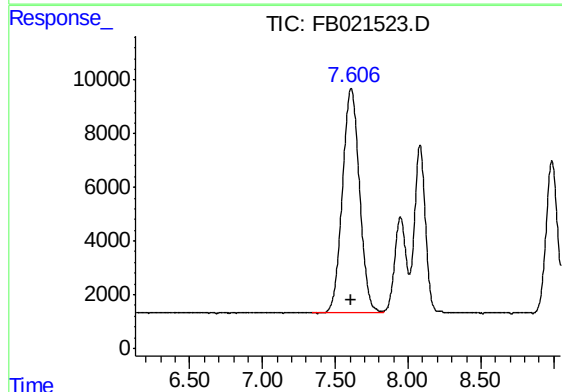


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 683943
Conc: 22.13 ng/ml

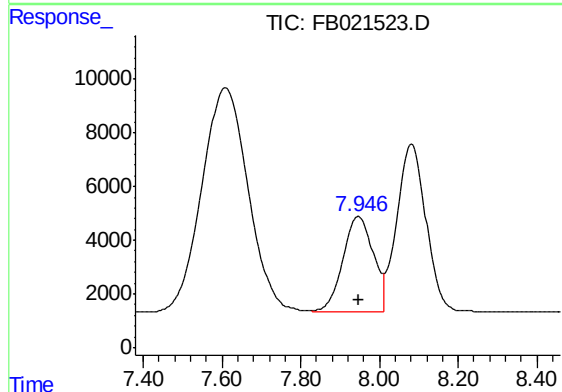


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: 0.000 min
Response: 191811
Conc: 6.55 ng/ml

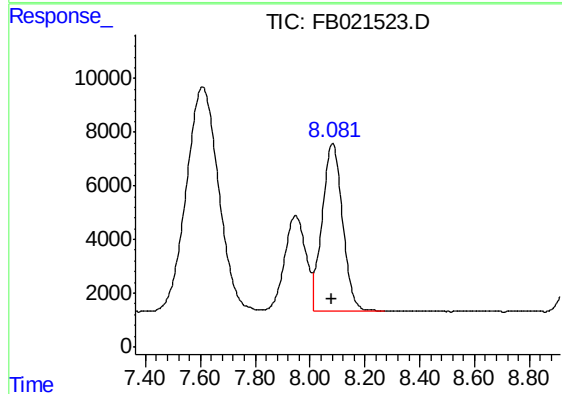


#4 Benzene

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 326444
Conc: 9.73 ng/ml

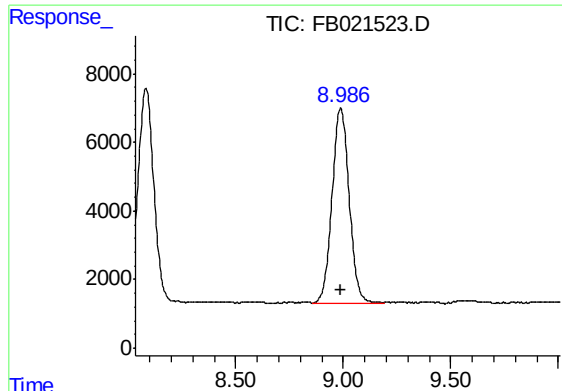


#5 AAA-TFT

R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 315416
Conc: 22.81 ng/ml

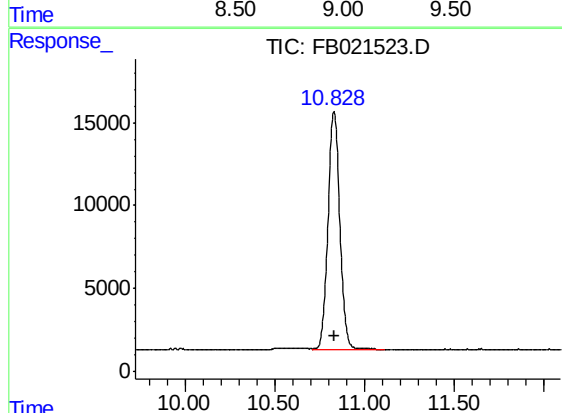


#6 Toluene

R.T.: 10.829 min
Delta R.T.: 0.000 min
Response: 661406
Conc: 28.96 ng/ml

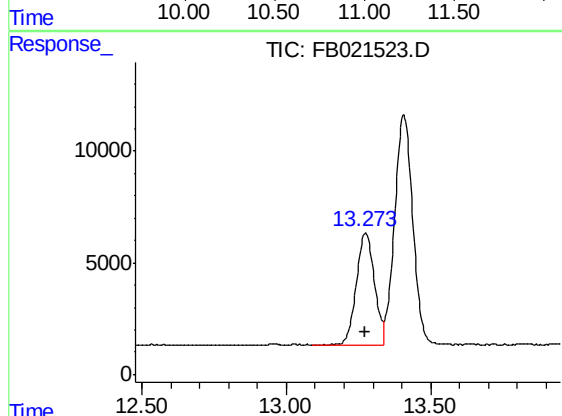


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: 0.000 min
Response: 217545
Conc: 9.19 ng/ml

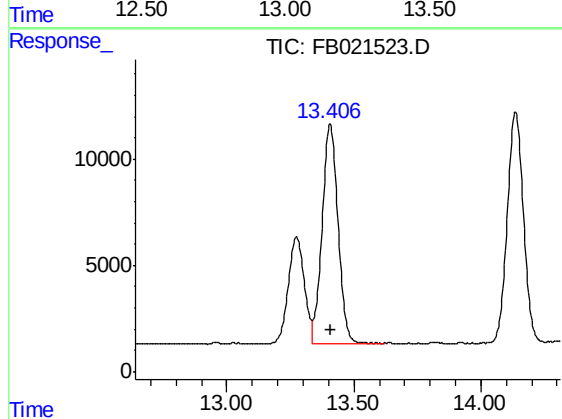


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: 0.000 min
Response: 452859
Conc: 17.87 ng/ml

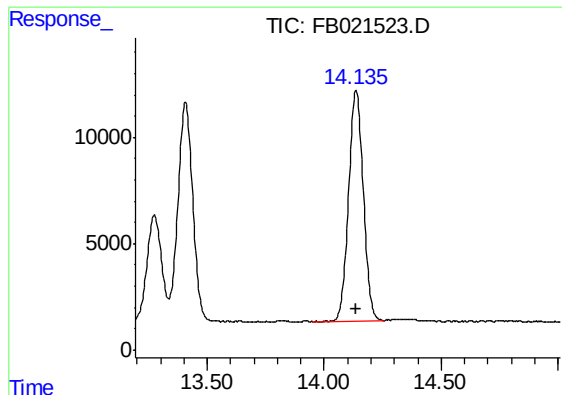

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: 0.000 min
Response: 472172
Conc: 18.00 ng/ml

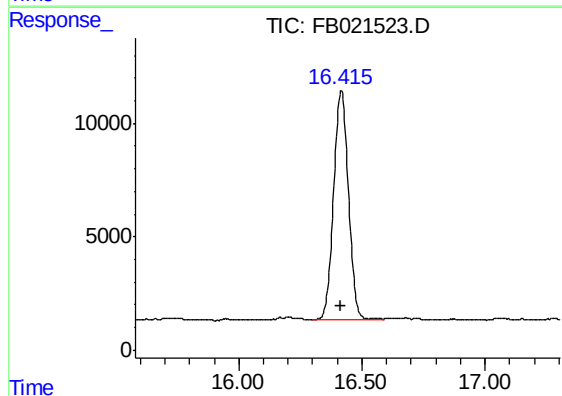

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: 0.000 min
Response: 419067
Conc: 15.95 ng/ml