

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
 Data File : FB027549.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jun 2022 20:26
 Operator : AJ/MA
 Sample : N3494-19
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 28 04:27:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	137785	12.284 ng/ml
Target Compounds			
4) t Benzene	7.889	12805	0.628 ng/ml
9) t O-Xylene	13.923	710	0.041 ng/ml
10) t 1,2,4-Trimethylbenzene	16.219	4614	0.269 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
Data File : FB027549.D
Signal(s) : FID2B.CH
Acq On : 27 Jun 2022 20:26
Operator : AJ/MA
Sample : N3494-19
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 28 04:27:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

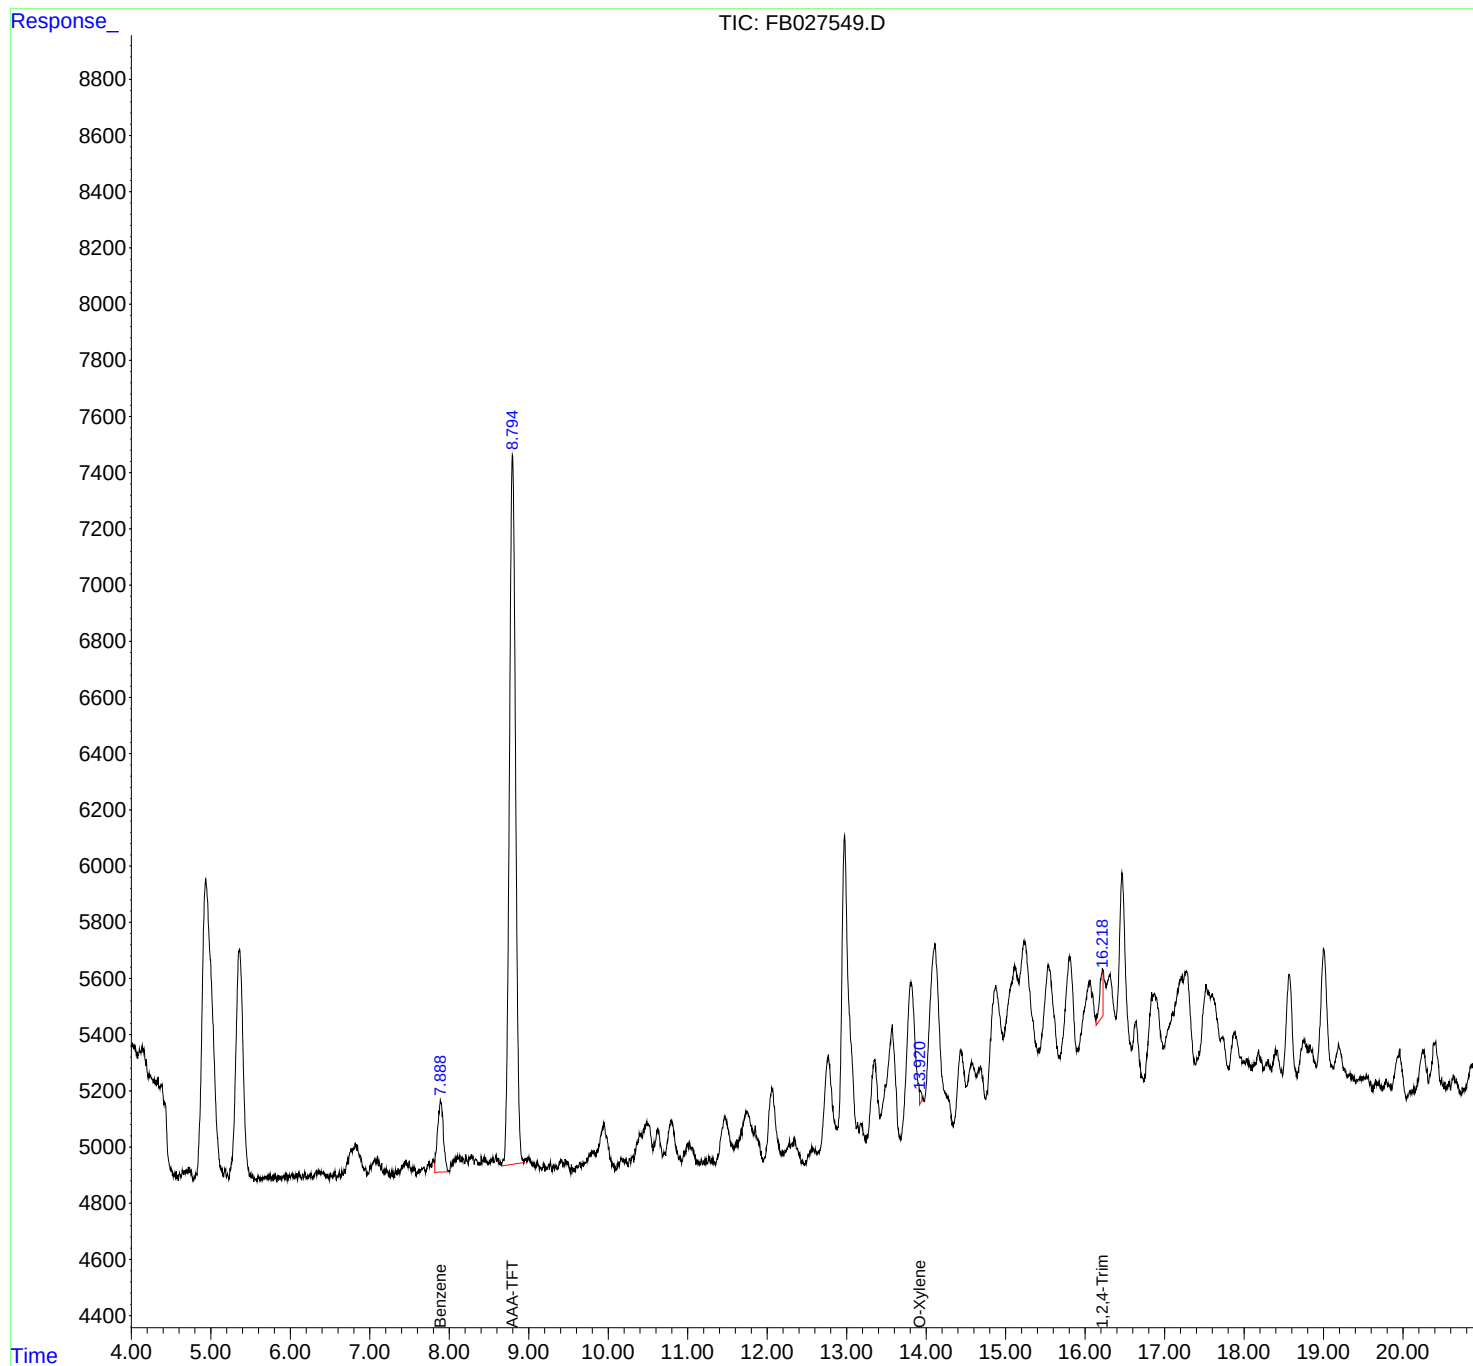


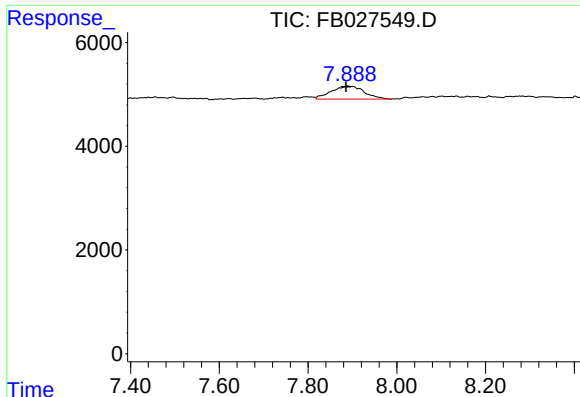

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.004 min
Response: 12805
Conc: 0.63 ng/ml

Instrument :
FID_B
ClientSampleId :

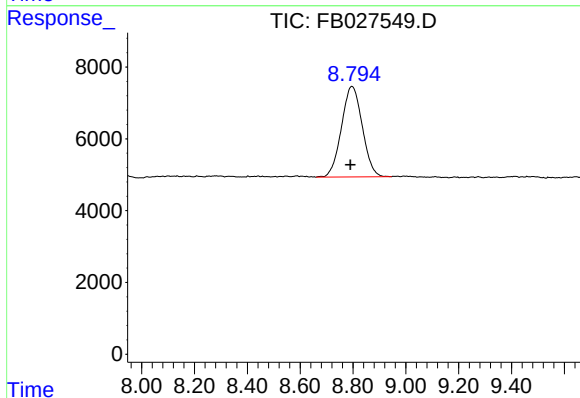


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 137785
Conc: 12.28 ng/ml

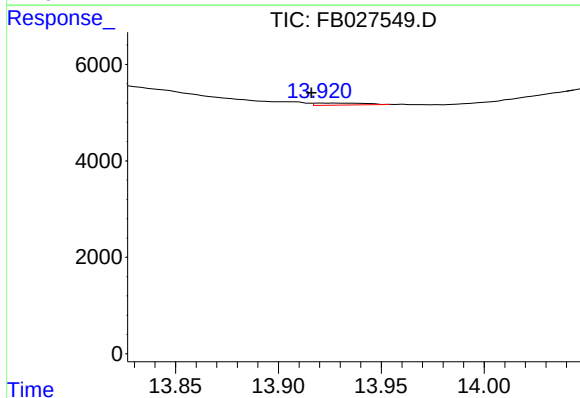

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.007 min
Response: 710
Conc: 0.04 ng/ml

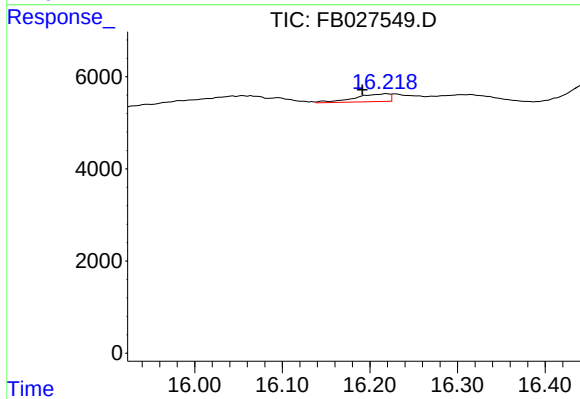

#10 1,2,4-Trimethylbenzene

R.T.: 16.219 min
Delta R.T.: 0.028 min
Response: 4614
Conc: 0.27 ng/ml